
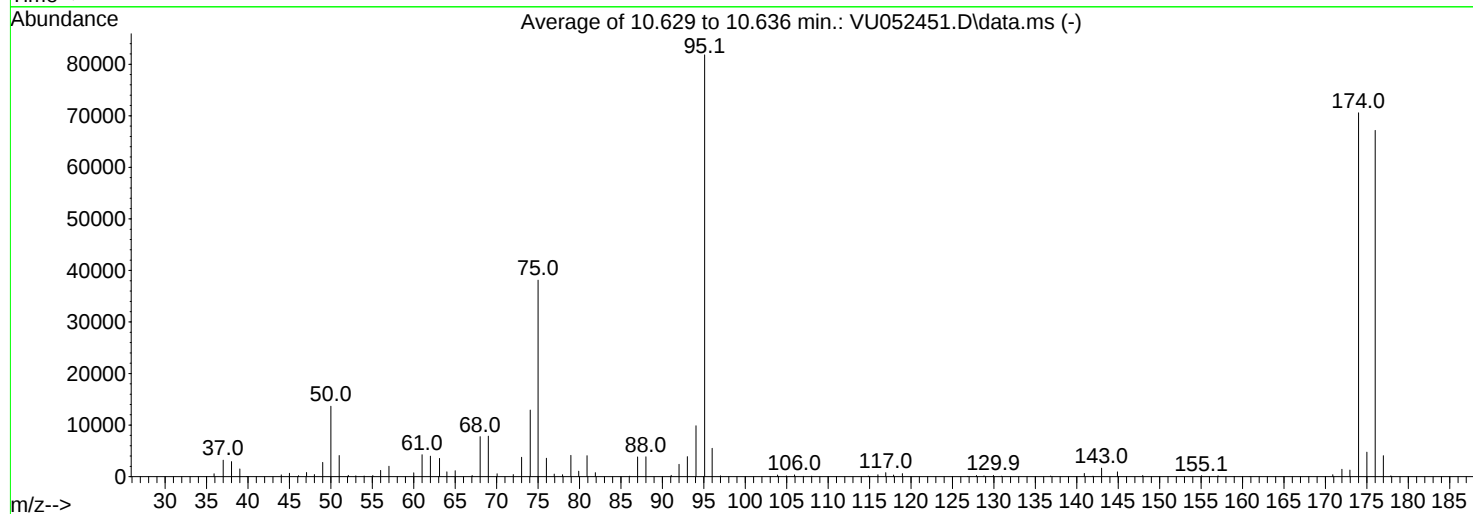


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
 Data File : VU052451.D
 Acq On : 19 Dec 2022 09:52
 Operator : JC/MD
 Sample : BFB011
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB011

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 02 00:27:38 2022

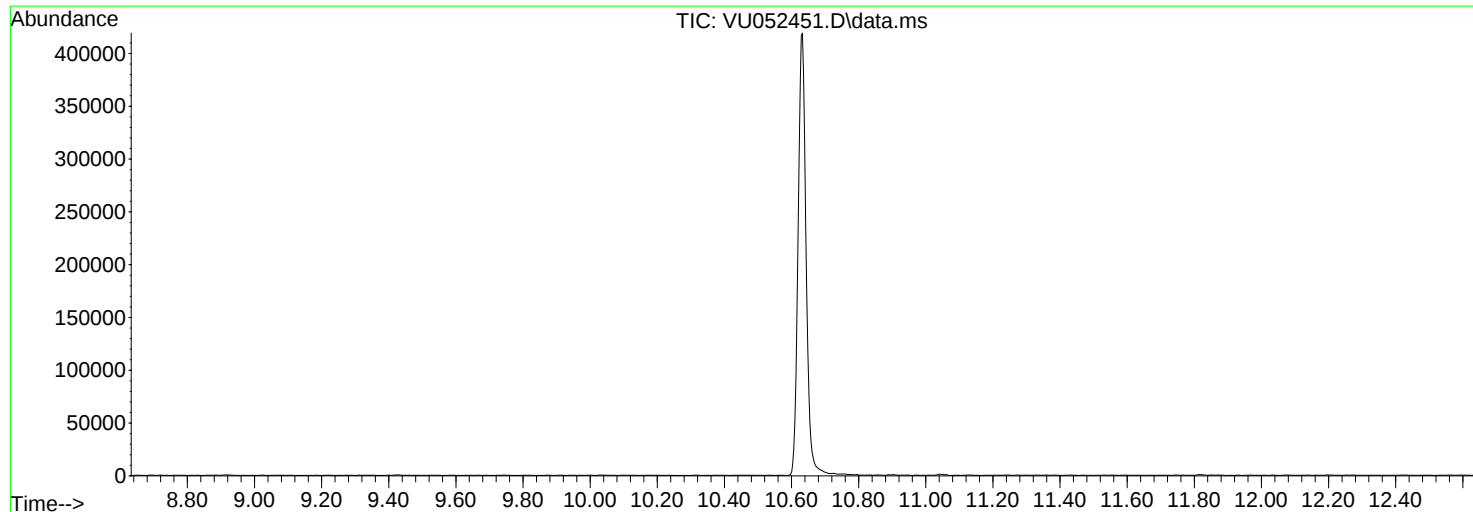

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	13673	PASS
75	95	30	80	46.6	38112	PASS
95	95	100	100	100.0	81821	PASS
96	95	5	9	6.7	5498	PASS
173	174	0.00	2	1.8	1283	PASS
174	95	50	120	86.3	70584	PASS
175	174	5	9	6.7	4757	PASS
176	174	95	101	95.1	67152	PASS
177	176	5	9	6.1	4081	PASS

m/z	Abundance
35.90	605.0
37.00	3492.0
38.00	3074.0
39.00	1590.0
39.90	295.0
44.00	677.0
45.00	723.0
46.10	204.0
47.00	870.0
48.00	440.0
49.00	2851.0
50.00	14497.0
51.00	4292.0
52.10	268.0
52.90	169.0
54.00	119.0
55.00	255.0
56.00	1288.0
57.00	2140.0
60.00	792.0
61.00	4400.0
62.00	4064.0
63.10	3753.0
64.00	886.0
65.00	1156.0
67.10	231.0
68.00	8192.0
69.00	8435.0
70.00	594.0
72.00	380.0
73.00	4093.0
74.10	13025.0
75.00	40216.0
76.00	3557.0
77.00	517.0
78.00	437.0
78.90	4199.0
79.90	1160.0
80.90	4131.0
81.90	796.0
86.10	143.0
87.00	3982.0
88.00	3883.0
91.00	243.0
92.00	2505.0
93.00	4031.0
94.10	10176.0
95.10	83720.0
96.00	5654.0
97.00	185.0
103.90	276.0
105.00	168.0
105.90	396.0
108.00	139.0
114.90	105.0
116.00	378.0
117.00	840.0
117.90	302.0
119.00	696.0
127.90	242.0
128.80	148.0
129.90	267.0
136.90	110.0
140.90	628.0
141.90	114.0
143.00	1680.0
144.90	1008.0
147.90	211.0
155.10	226.0
157.00	140.0
160.90	104.0
170.90	408.0
172.00	1413.0
173.00	1237.0
174.00	70720.0
175.00	4969.0
176.00	67664.0
177.00	4170.0
177.90	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
39.90	223.0
44.00	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	507.0
37.00	2814.0
38.00	2652.0
39.00	1340.0
39.80	214.0
44.00	504.0
45.00	567.0
46.10	176.0
47.10	737.0
48.00	331.0
49.00	2626.0
50.00	12444.0
51.00	3794.0
52.10	195.0
53.10	147.0
54.00	121.0
55.10	182.0
56.00	1117.0
57.00	1837.0
60.00	692.0
61.00	3934.0
62.00	3719.0
63.10	3266.0
64.00	966.0
65.00	1097.0
67.00	224.0
68.00	7075.0
69.00	7085.0
70.10	507.0
72.00	400.0
73.00	3362.0
74.00	12295.0
75.00	34768.0
76.00	3408.0
76.90	453.0
77.90	316.0
79.00	3928.0
79.90	967.0
80.90	3851.0
81.90	727.0
86.00	104.0
87.00	3564.0
88.00	3636.0
91.10	265.0
92.00	2136.0
93.00	3598.0
94.00	9086.0
95.10	77200.0
96.00	5219.0
97.00	118.0
103.90	329.0
104.90	125.0
106.00	309.0
107.00	112.0
114.80	143.0
116.00	335.0
116.90	709.0
117.90	296.0
118.90	472.0
126.90	117.0
127.90	205.0
128.80	145.0
130.00	258.0
130.90	136.0
136.80	113.0
140.90	607.0
142.00	104.0
143.00	1531.0
144.90	840.0
148.00	196.0
155.00	173.0
157.10	146.0
170.90	393.0
172.00	1389.0
172.90	1278.0
174.00	67968.0
175.00	4445.0
176.00	64624.0
177.00	3907.0
177.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	586.0
37.00	3310.0
38.00	3049.0
39.00	1584.0
39.80	245.0
44.00	594.0
45.00	709.0
46.10	214.0
47.00	808.0
48.00	411.0
49.00	2840.0
50.00	14079.0
51.00	4251.0
52.10	255.0
53.00	160.0
54.00	128.0
55.00	216.0
56.00	1271.0
57.00	2098.0
60.00	786.0
61.00	4407.0
62.00	4158.0
63.10	3640.0
64.00	954.0
65.00	1181.0
67.00	231.0
68.00	8015.0
69.00	8029.0
70.00	555.0
72.00	433.0
73.00	3867.0
74.00	13393.0
75.00	39352.0
76.00	3736.0
76.90	535.0
77.90	373.0
78.90	4246.0
79.90	1043.0
80.90	4265.0
81.90	786.0
87.00	3934.0
88.00	4050.0
91.00	273.0
92.00	2539.0
93.00	4042.0
94.00	10399.0
95.10	84544.0
96.00	5621.0
97.00	166.0
103.90	317.0
105.00	148.0
106.00	367.0
107.00	105.0
108.00	123.0
114.90	141.0
116.00	390.0
117.00	792.0
117.90	332.0
119.00	605.0
126.80	111.0
127.90	217.0
128.80	156.0
130.00	271.0
130.90	134.0
136.80	124.0
140.90	632.0
141.90	102.0
143.00	1690.0
144.90	962.0
147.90	215.0
155.10	205.0
157.00	150.0
159.00	103.0
170.90	360.0
172.00	1494.0
173.00	1335.0
174.00	73064.0
175.00	4856.0
176.00	69168.0
177.00	4165.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011