

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057044.D
 Acq On : 19 Dec 2023 15:09
 Operator : MD/SY
 Sample : 05830-06 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	106	rVB	104859	120027	7.71%	1.552%
2	1.907	184	192	208	rVB	77286	107414	6.90%	1.389%
3	2.563	383	396	414	rBV2	173033	298730	19.18%	3.863%
4	3.042	530	545	560	rBV2	18141	36702	2.36%	0.475%
5	4.621	1025	1036	1068	rBV	78474	251786	16.16%	3.256%
6	5.055	1156	1171	1202	rBV	152145	340172	21.84%	4.399%
7	5.309	1235	1250	1266	rVB2	33189	74810	4.80%	0.967%
8	5.718	1357	1377	1399	rBV2	278203	721960	46.35%	9.336%
9	6.242	1527	1540	1568	rBV	254980	502740	32.28%	6.501%
10	6.537	1619	1632	1652	rBV	47303	91001	5.84%	1.177%
11	6.685	1664	1678	1702	rBV	167630	335087	21.51%	4.333%
12	7.560	1934	1950	1973	rBV	79829	149293	9.58%	1.931%
13	7.894	2040	2054	2078	rBV	322989	582547	37.40%	7.533%
14	8.177	2129	2142	2162	rBV	48744	89306	5.73%	1.155%
15	8.547	2242	2257	2273	rBV	909949	1557672	100.00%	20.144%
16	8.631	2273	2283	2311	rVB2	309189	610509	39.19%	7.895%
17	9.412	2513	2526	2550	rBV	362854	637184	40.91%	8.240%
18	10.749	2930	2942	2963	rBV	117230	194830	12.51%	2.520%
19	11.807	3258	3271	3293	rBV	330563	541642	34.77%	7.004%
20	12.187	3377	3389	3407	rBV	288416	489450	31.42%	6.329%




Sum of corrected areas: 7732862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057044.D
Acq On : 19 Dec 2023 15:09
Operator : MD/SY
Sample : 05830-06 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

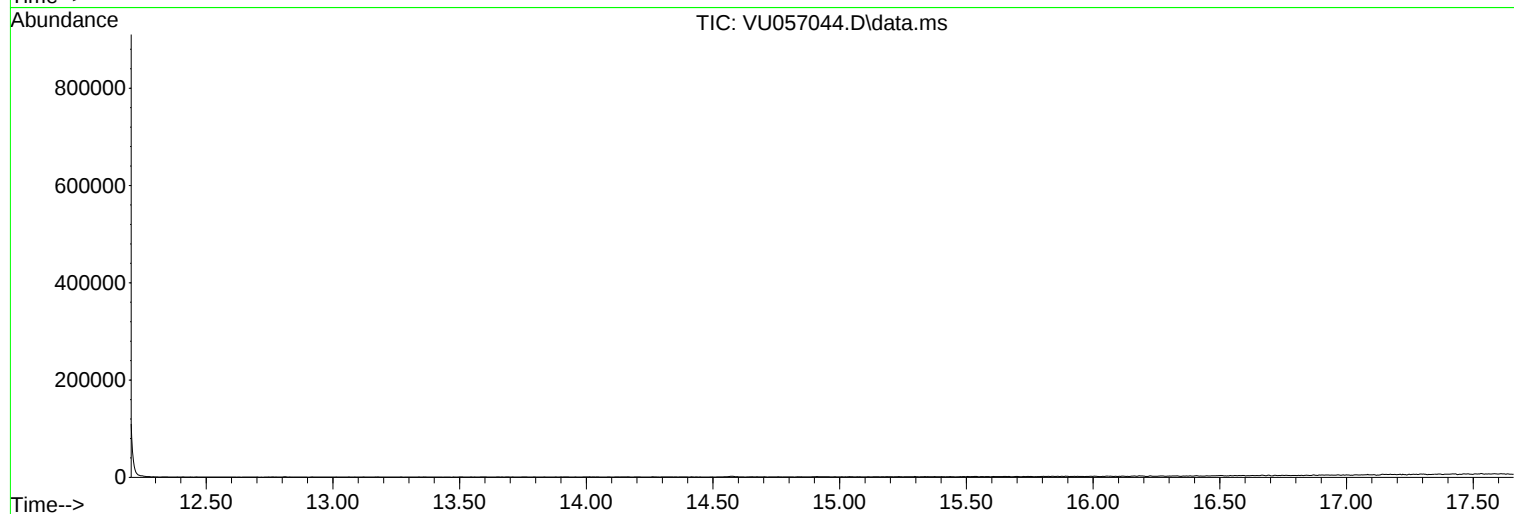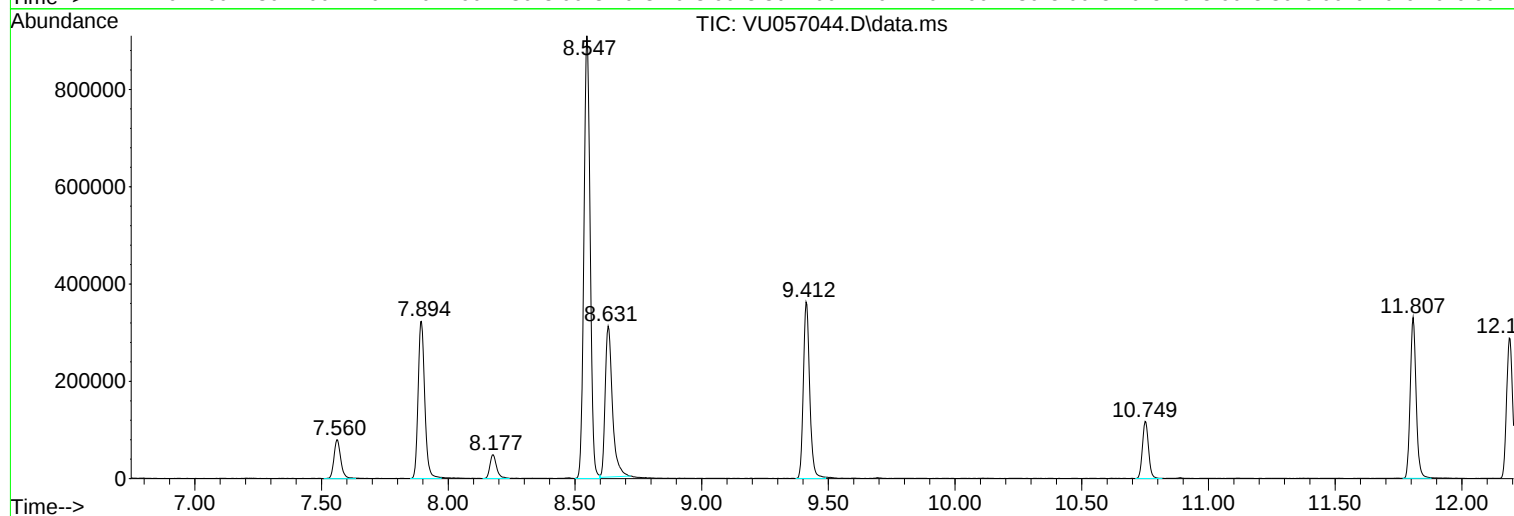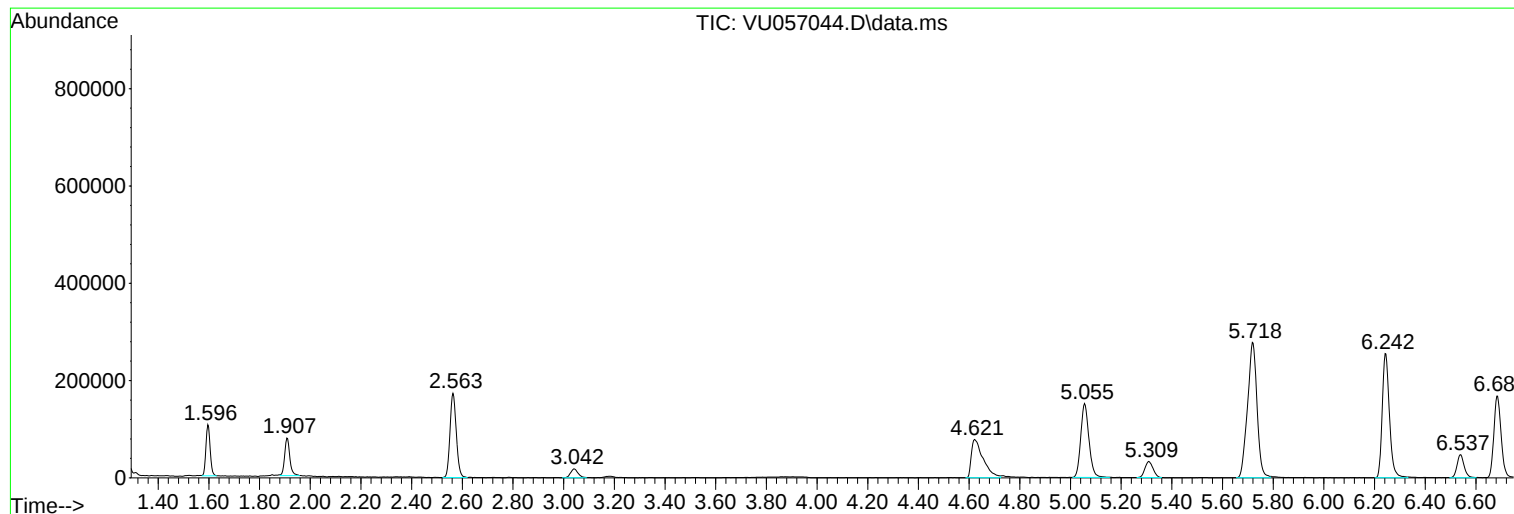

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057044.D
Acq On : 19 Dec 2023 15:09
Operator : MD/SY
Sample : 05830-06 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057044.D
Acq On : 19 Dec 2023 15:09
Operator : MD/SY
Sample : 05830-06 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc