

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057050.D
 Acq On : 19 Dec 2023 17:35
 Operator : MD/SY
 Sample : 05843-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C93

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	115	rVB	97077	114623	16.68%	1.960%
2	1.907	183	192	208	rVB	75476	109344	15.91%	1.870%
3	2.563	383	396	410	rBV	152516	250352	36.43%	4.281%
4	4.621	1025	1036	1056	rBV2	78282	205471	29.90%	3.514%
5	5.055	1156	1171	1192	rBV	151647	336527	48.97%	5.755%
6	5.718	1355	1377	1397	rBV2	263486	687270	100.00%	11.753%
7	6.242	1527	1540	1566	rBV	263910	509288	74.10%	8.709%
8	6.685	1664	1678	1708	rBV	161744	325601	47.38%	5.568%
9	7.560	1935	1950	1973	rBV2	78702	145809	21.22%	2.493%
10	7.894	2040	2054	2072	rBV	314063	556420	80.96%	9.515%
11	7.968	2074	2077	2091	rVB3	5763	8051	1.17%	0.138%
12	8.177	2131	2142	2161	rBV	47623	84220	12.25%	1.440%
13	8.631	2271	2283	2315	rBV2	295936	603670	87.84%	10.323%
14	9.412	2513	2526	2547	rBV	373302	648733	94.39%	11.094%
15	9.499	2547	2553	2565	rVB8	6273	11520	1.68%	0.197%
16	10.750	2927	2942	2962	rBV	114614	190187	27.67%	3.252%
17	10.891	2975	2986	2995	rVB2	6774	11313	1.65%	0.193%
18	11.807	3259	3271	3297	rBV	347846	570526	83.01%	9.756%
19	12.187	3374	3389	3409	rBV	288999	478753	69.66%	8.187%




Sum of corrected areas: 5847678

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057050.D
Acq On : 19 Dec 2023 17:35
Operator : MD/SY
Sample : 05843-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

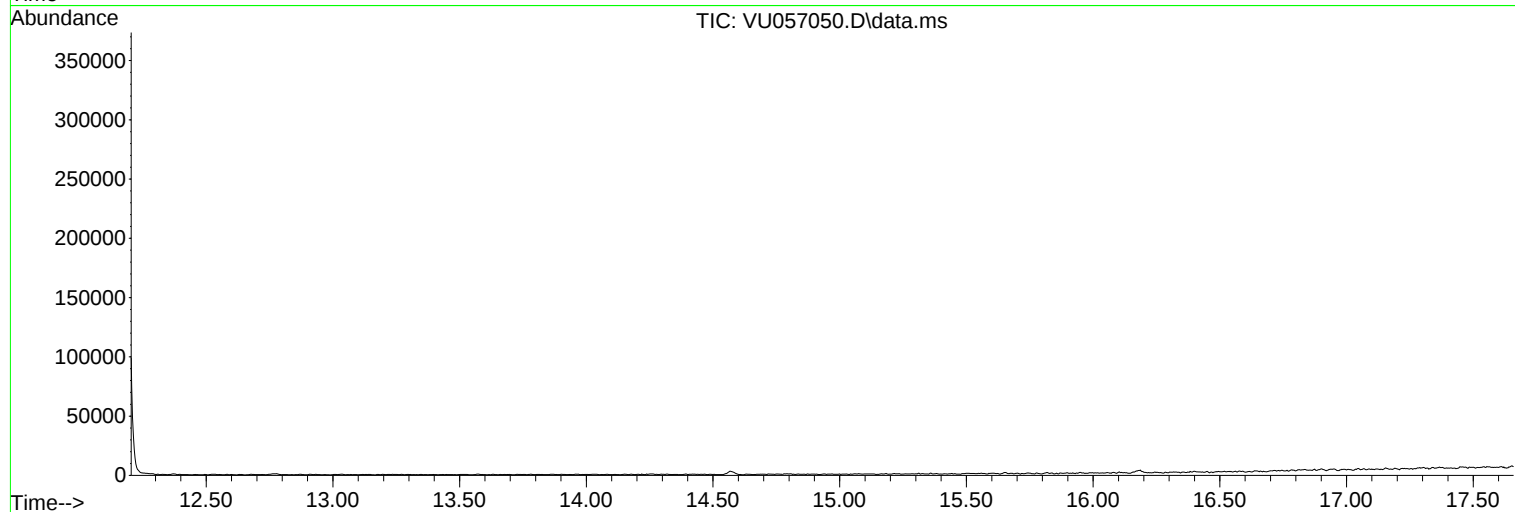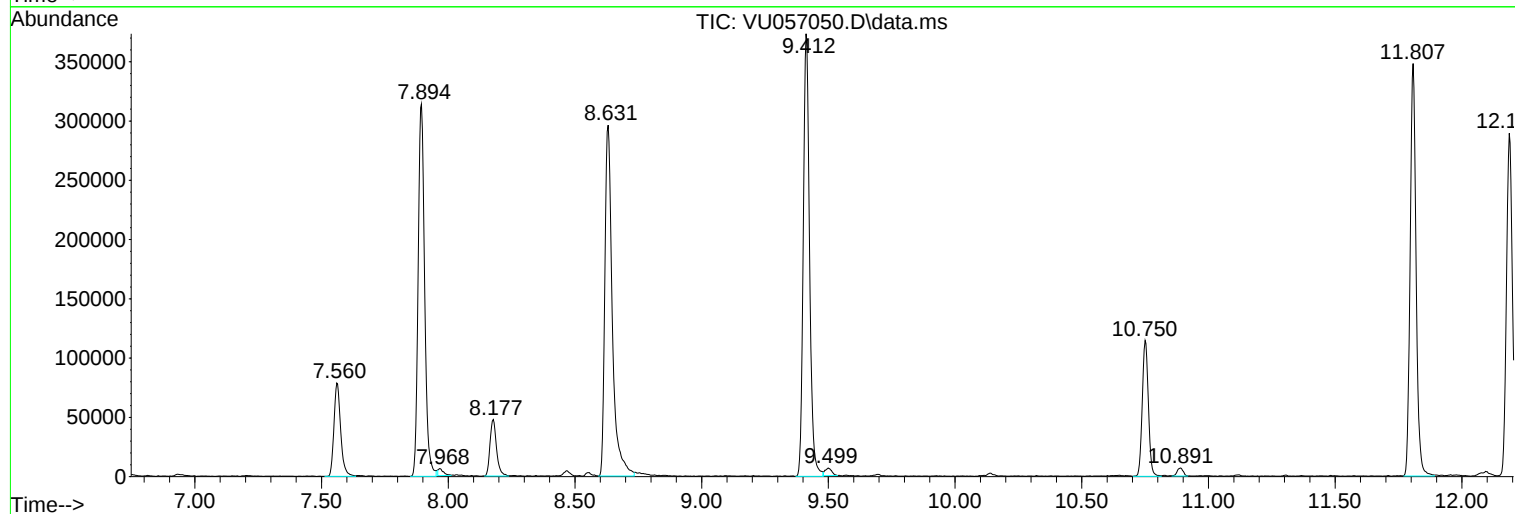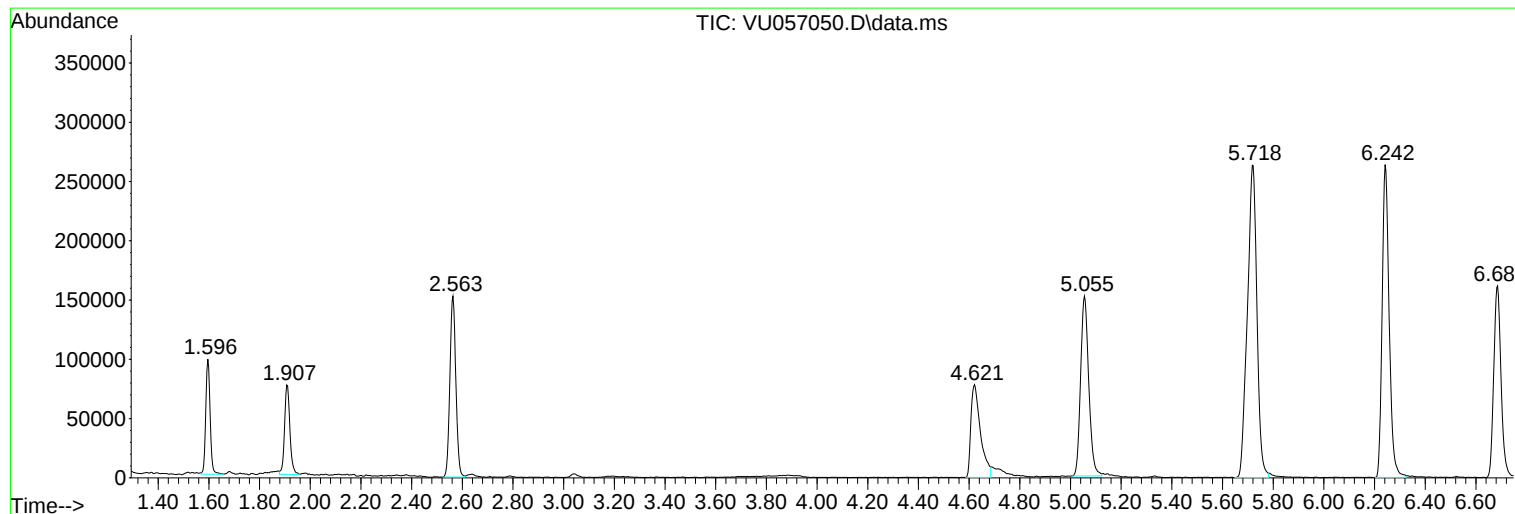

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057050.D
Acq On : 19 Dec 2023 17:35
Operator : MD/SY
Sample : 05843-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057050.D
Acq On : 19 Dec 2023 17:35
Operator : MD/SY
Sample : 05843-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc