

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057059.D
 Acq On : 19 Dec 2023 21:37
 Operator : MD/SY
 Sample : 05865-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rVB	96949	113392	16.66%	1.980%
2	1.907	184	192	209	rVB	76736	107451	15.78%	1.877%
3	2.563	384	396	412	rBV	152220	244255	35.88%	4.266%
4	3.187	576	590	596	rBV7	3915	9311	1.37%	0.163%
5	4.618	1024	1035	1066	rBV2	78002	214653	31.53%	3.749%
6	5.055	1155	1171	1206	rVB	140377	323087	47.46%	5.643%
7	5.718	1351	1377	1406	rBV2	262530	680743	100.00%	11.890%
8	6.245	1525	1541	1564	rBV	243118	485125	71.26%	8.473%
9	6.685	1664	1678	1704	rBV	160196	317005	46.57%	5.537%
10	7.560	1935	1950	1966	rBV2	75328	138497	20.34%	2.419%
11	7.894	2041	2054	2072	rBV	312170	556889	81.81%	9.726%
12	8.174	2130	2141	2157	rBV	47958	84690	12.44%	1.479%
13	8.467	2222	2232	2244	rBV3	5849	9823	1.44%	0.172%
14	8.550	2249	2258	2269	rVB4	9670	15876	2.33%	0.277%
15	8.631	2271	2283	2315	rBV3	297309	593072	87.12%	10.358%
16	9.412	2513	2526	2551	rBV	352284	616570	90.57%	10.769%
17	10.750	2929	2942	2963	rVB	113301	183723	26.99%	3.209%
18	10.888	2975	2985	2997	rBV3	11294	17437	2.56%	0.305%
19	11.807	3259	3271	3290	rBV	330084	543189	79.79%	9.487%
20	12.187	3376	3389	3406	rBV	281380	470725	69.15%	8.222%




Sum of corrected areas: 5725513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057059.D
Acq On : 19 Dec 2023 21:37
Operator : MD/SY
Sample : 05865-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

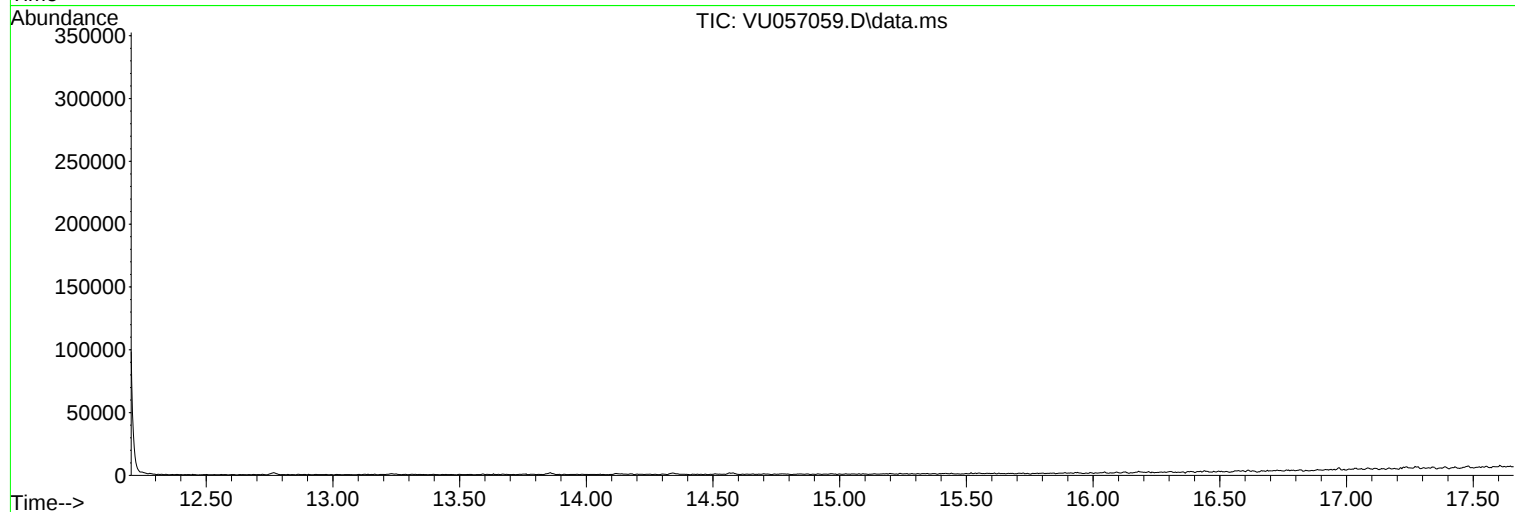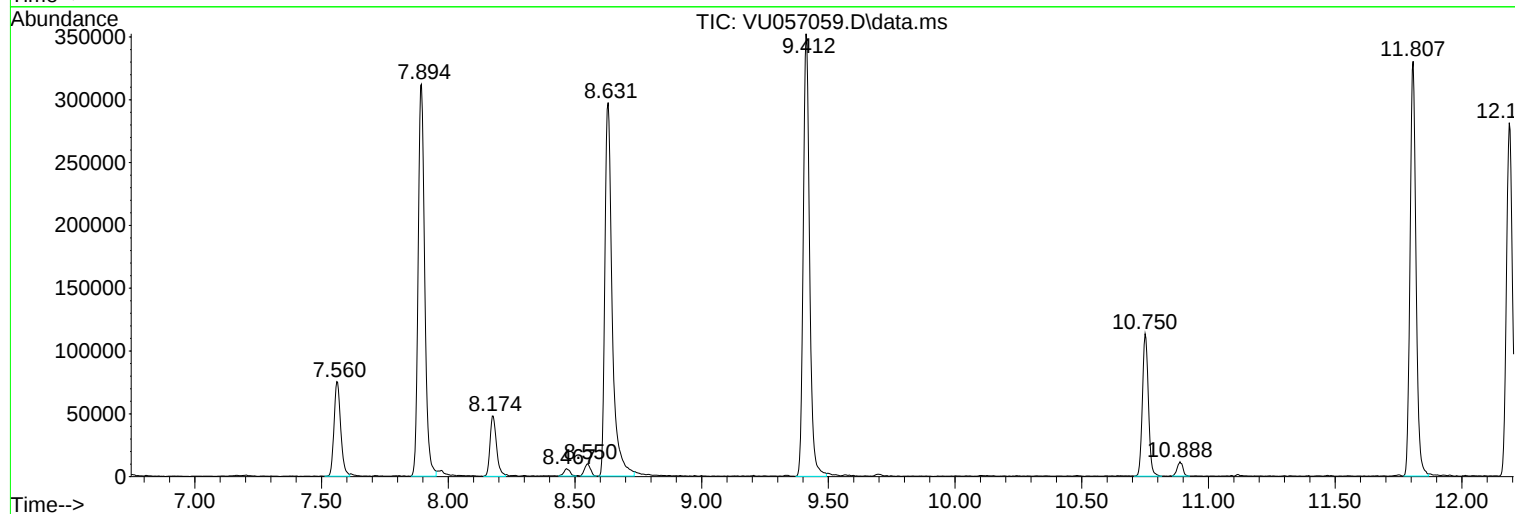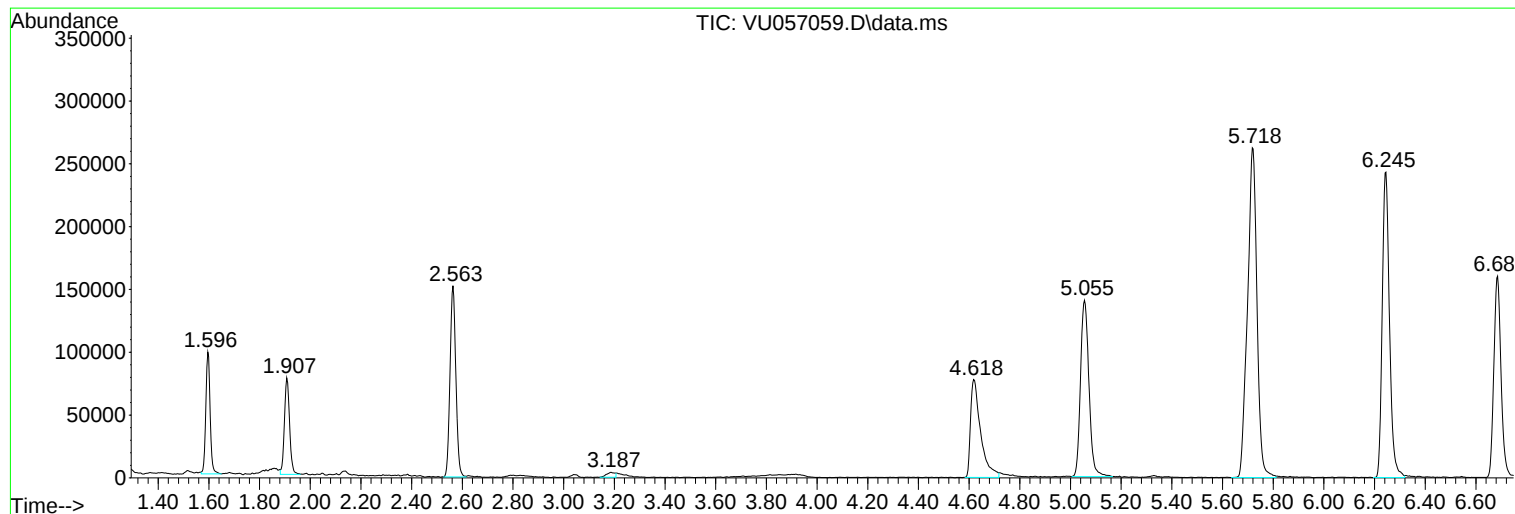

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057059.D
Acq On : 19 Dec 2023 21:37
Operator : MD/SY
Sample : 05865-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057059.D
Acq On : 19 Dec 2023 21:37
Operator : MD/SY
Sample : 05865-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc