

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057060.D
 Acq On : 19 Dec 2023 22:01
 Operator : MD/SY
 Sample : 05865-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	109	rVB	95862	112612	15.98%	1.936%
2	1.907	183	192	207	rVB	77129	106569	15.12%	1.832%
3	2.563	383	396	412	rBV	153378	250147	35.49%	4.300%
4	4.621	1025	1036	1062	rBV2	79438	217869	30.91%	3.745%
5	5.055	1155	1171	1193	rBV	150388	333485	47.32%	5.733%
6	5.717	1356	1377	1408	rBV2	270257	704763	100.00%	12.116%
7	6.242	1526	1540	1566	rBV	244637	482353	68.44%	8.292%
8	6.682	1661	1677	1699	rBV	169125	332708	47.21%	5.720%
9	7.560	1939	1950	1970	rBV	77680	142130	20.17%	2.443%
10	7.894	2041	2054	2077	rBV	317621	569021	80.74%	9.782%
11	8.177	2129	2142	2161	rBV	48477	84369	11.97%	1.450%
12	8.470	2224	2233	2244	rVB3	4281	7635	1.08%	0.131%
13	8.550	2249	2258	2269	rVB3	9281	15043	2.13%	0.259%
14	8.631	2271	2283	2317	rBV2	305802	612020	86.84%	10.521%
15	9.412	2512	2526	2553	rBV	351172	614688	87.22%	10.567%
16	10.749	2928	2942	2965	rVB	117107	194554	27.61%	3.345%
17	10.891	2976	2986	2996	rBV3	8446	14156	2.01%	0.243%
18	11.807	3259	3271	3293	rBV	331163	537649	76.29%	9.243%
19	12.187	3377	3389	3414	rBV2	285252	485211	68.85%	8.341%




Sum of corrected areas: 5816982

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057060.D
Acq On : 19 Dec 2023 22:01
Operator : MD/SY
Sample : 05865-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

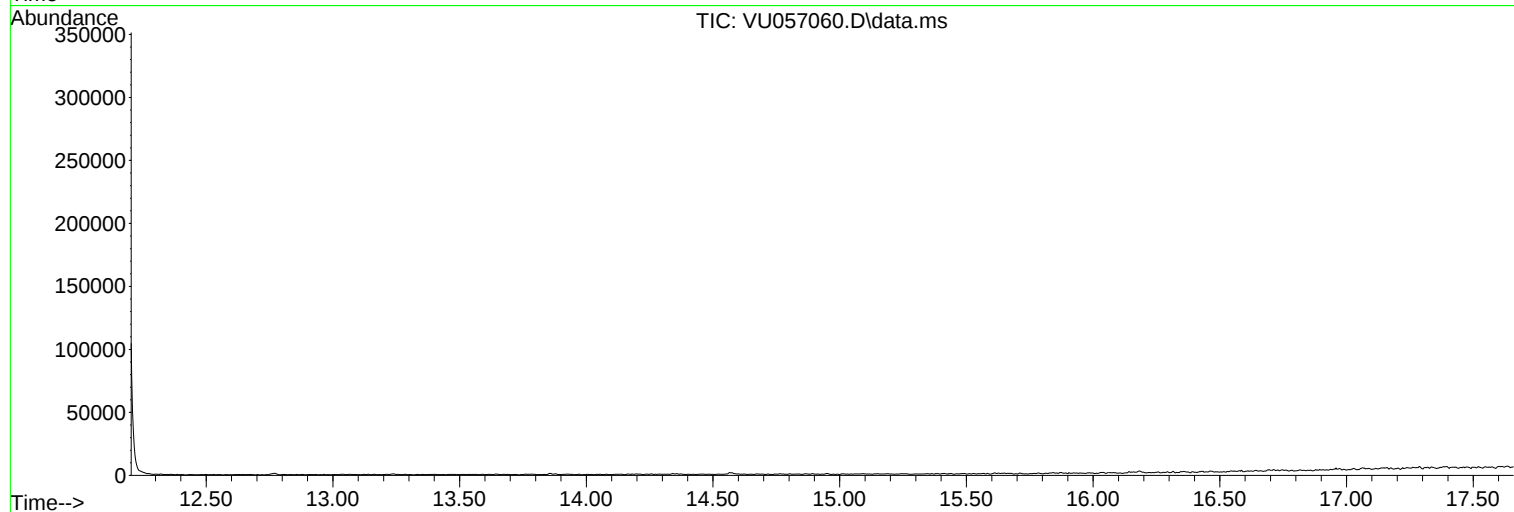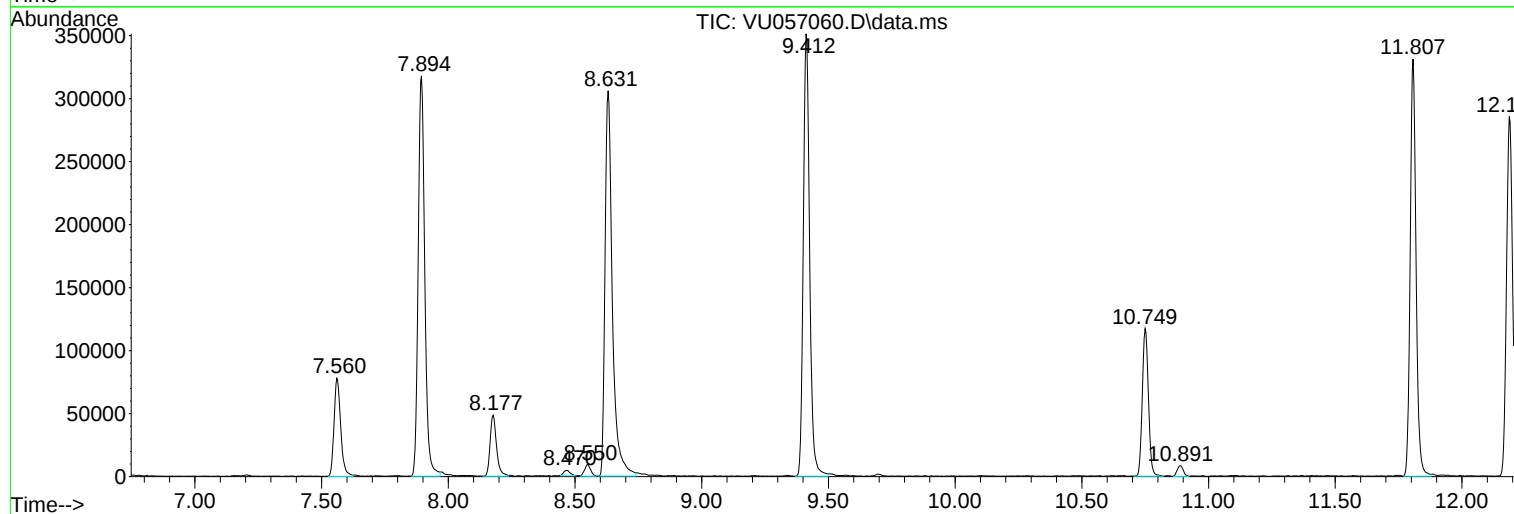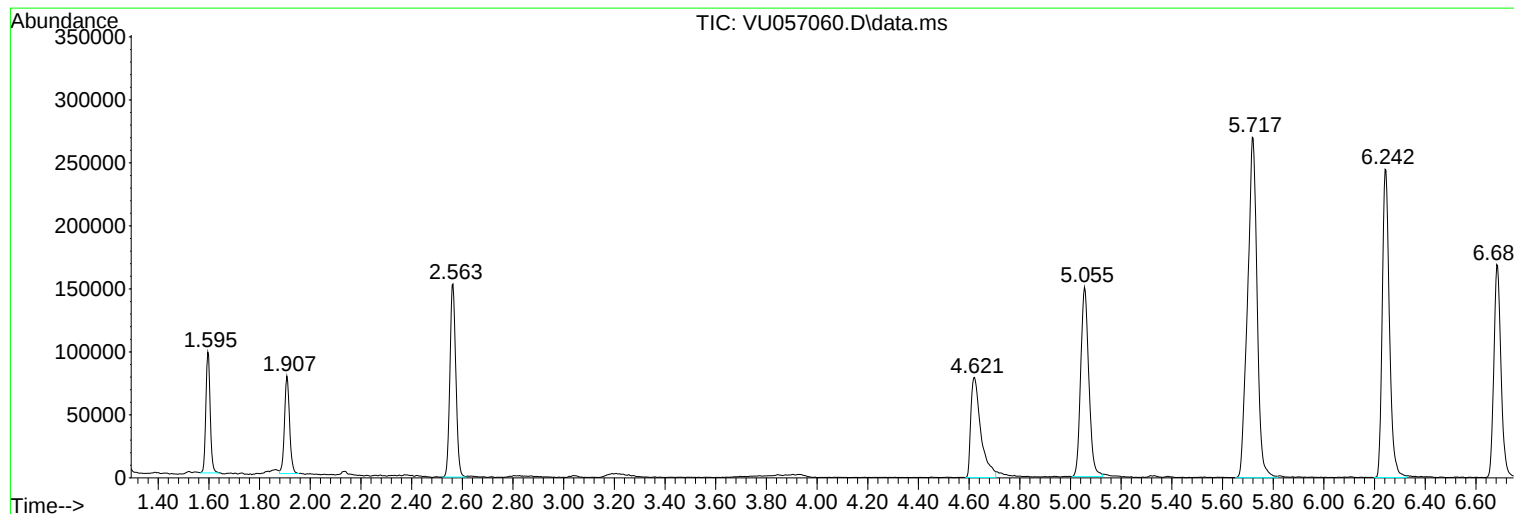

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057060.D
Acq On : 19 Dec 2023 22:01
Operator : MD/SY
Sample : 05865-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057060.D
Acq On : 19 Dec 2023 22:01
Operator : MD/SY
Sample : 05865-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc