

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057064.D
 Acq On : 19 Dec 2023 23:38
 Operator : MD/SY
 Sample : 05865-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C48

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	107	rVB	97321	111756	15.93%	1.925%
2	1.907	183	192	212	rVB	78395	108489	15.47%	1.868%
3	2.136	255	263	272	rVB2	8994	12906	1.84%	0.222%
4	2.563	382	396	411	rBV	152638	251248	35.82%	4.327%
5	4.621	1023	1036	1062	rBV2	81584	221444	31.57%	3.814%
6	5.055	1154	1171	1196	rBV	145714	335279	47.80%	5.774%
7	5.721	1357	1378	1405	rBV3	268565	701469	100.00%	12.080%
8	6.242	1528	1540	1563	rBV	240441	474955	67.71%	8.179%
9	6.685	1664	1678	1705	rBV	164222	329855	47.02%	5.681%
10	7.560	1938	1950	1972	rBV	79791	145063	20.68%	2.498%
11	7.894	2035	2054	2075	rBV	314757	564079	80.41%	9.714%
12	8.174	2128	2141	2160	rBV	47642	83930	11.96%	1.445%
13	8.550	2250	2258	2270	rBV6	8315	14198	2.02%	0.245%
14	8.631	2270	2283	2309	rBV2	310155	616131	87.83%	10.611%
15	9.412	2513	2526	2550	rBV	351431	604571	86.19%	10.412%
16	10.750	2929	2942	2959	rBV	116994	195048	27.81%	3.359%
17	10.888	2973	2985	2996	rVB3	5694	9297	1.33%	0.160%
18	11.807	3259	3271	3297	rBV	326607	538364	76.75%	9.271%
19	12.187	3374	3389	3410	rBV	286773	488608	69.65%	8.415%




Sum of corrected areas: 5806690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057064.D
Acq On : 19 Dec 2023 23:38
Operator : MD/SY
Sample : 05865-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

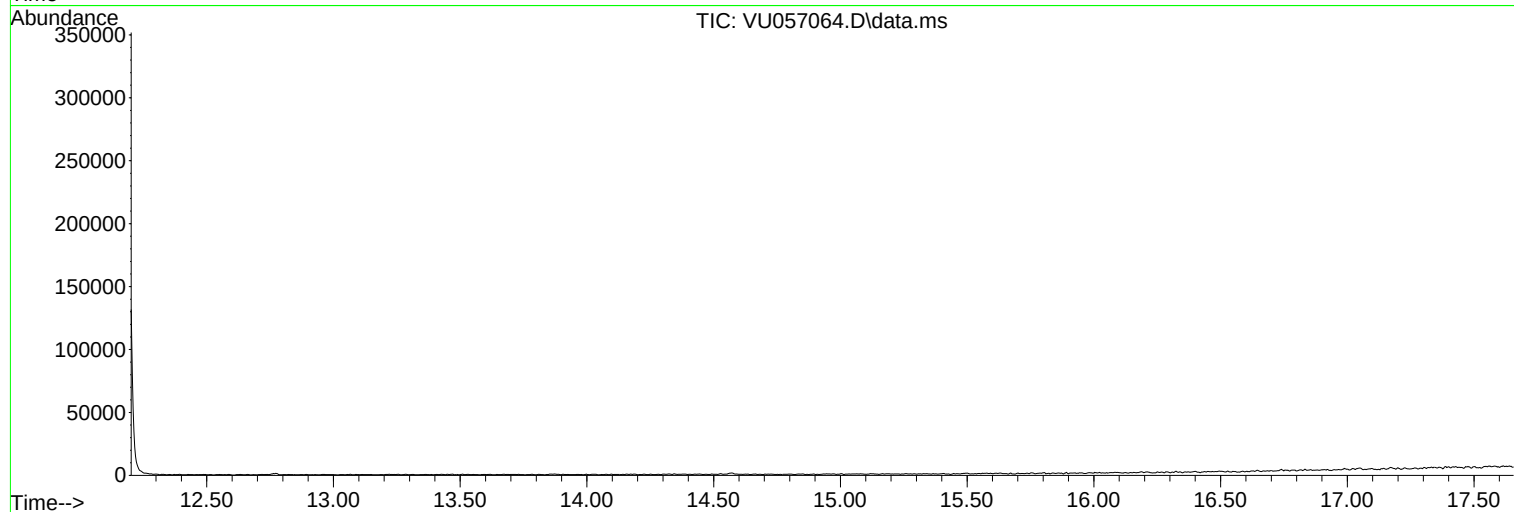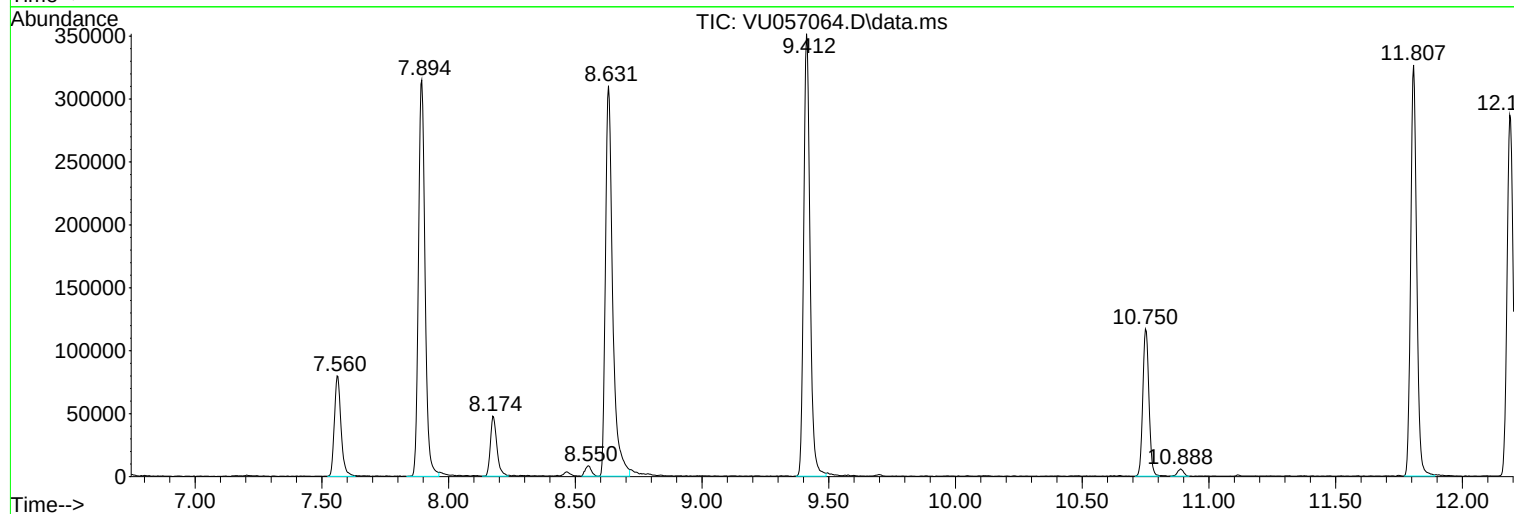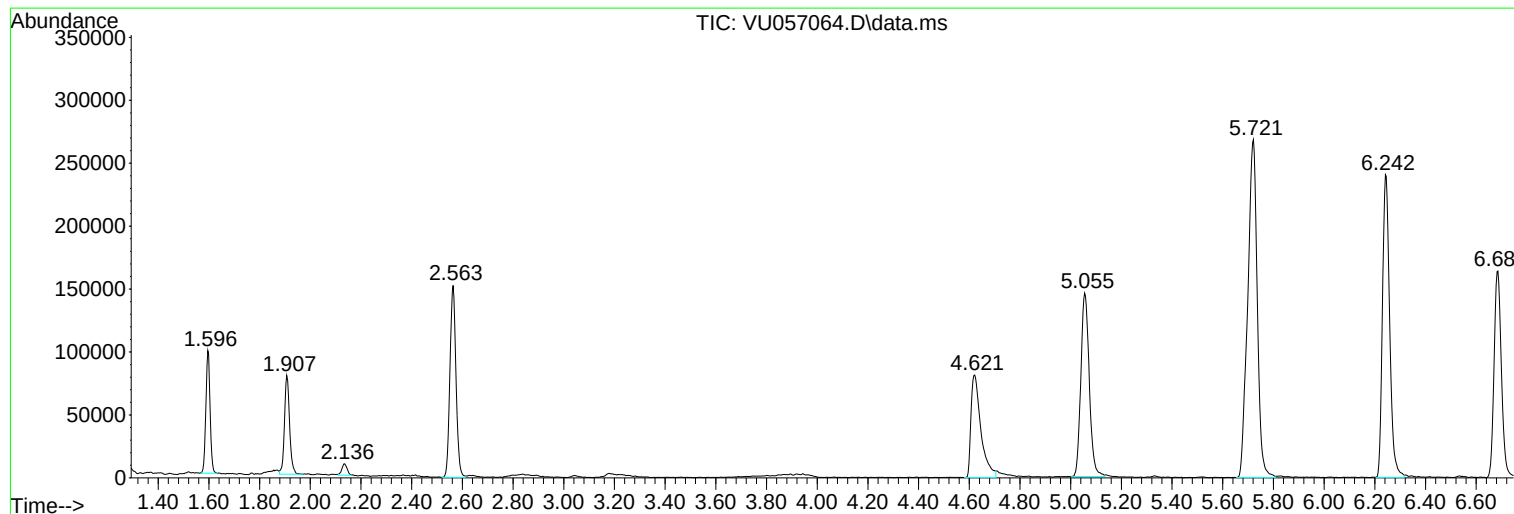

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057064.D
Acq On : 19 Dec 2023 23:38
Operator : MD/SY
Sample : 05865-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057064.D
Acq On : 19 Dec 2023 23:38
Operator : MD/SY
Sample : 05865-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc