

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057068.D
 Acq On : 20 Dec 2023 01:14
 Operator : MD/SY
 Sample : 05865-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C75

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	105	rBV	93237	107767	15.15%	1.660%
2	1.907	184	192	207	rVB	78335	109416	15.39%	1.685%
3	2.563	383	396	411	rBV	154956	255930	35.99%	3.942%
4	2.798	455	469	471	rBV3	4046	7269	1.02%	0.112%
5	3.184	576	589	593	rBV3	6129	11257	1.58%	0.173%
6	4.618	1022	1035	1065	rBV	81941	219330	30.84%	3.378%
7	5.055	1156	1171	1199	rVB	149653	347155	48.82%	5.347%
8	5.717	1358	1377	1401	rBV2	270223	711145	100.00%	10.954%
9	6.245	1527	1541	1564	rBV	243040	470564	66.17%	7.248%
10	6.685	1664	1678	1698	rBV	165906	332445	46.75%	5.121%
11	7.560	1938	1950	1964	rBV	78376	145519	20.46%	2.241%
12	7.894	2037	2054	2088	rBV	321393	580974	81.70%	8.949%
13	8.177	2131	2142	2162	rBV2	48250	85818	12.07%	1.322%
14	8.547	2241	2257	2272	rBV	393955	678408	95.40%	10.449%
15	8.630	2272	2283	2320	rVB2	317052	621393	87.38%	9.571%
16	9.412	2513	2526	2551	rBV	346447	600383	84.42%	9.248%
17	10.749	2931	2942	2960	rBV2	118265	194232	27.31%	2.992%
18	11.807	3258	3271	3294	rBV	311476	517054	72.71%	7.964%
19	12.187	3377	3389	3409	rBV2	289592	496199	69.77%	7.643%




Sum of corrected areas: 6492258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057068.D
Acq On : 20 Dec 2023 01:14
Operator : MD/SY
Sample : 05865-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

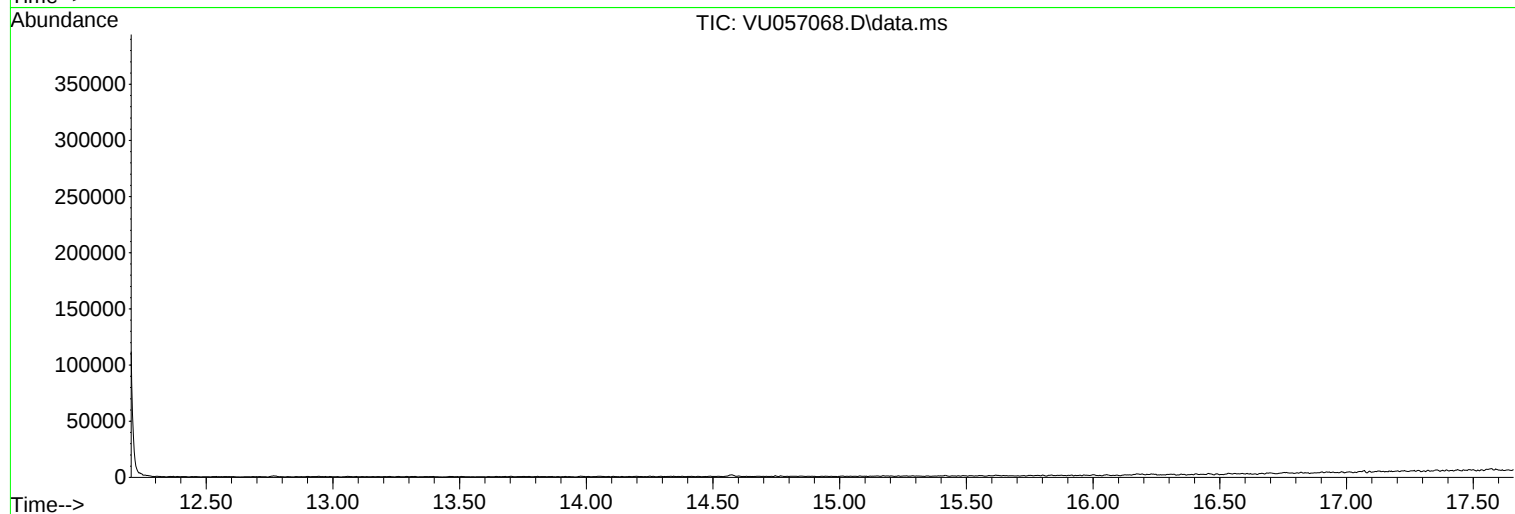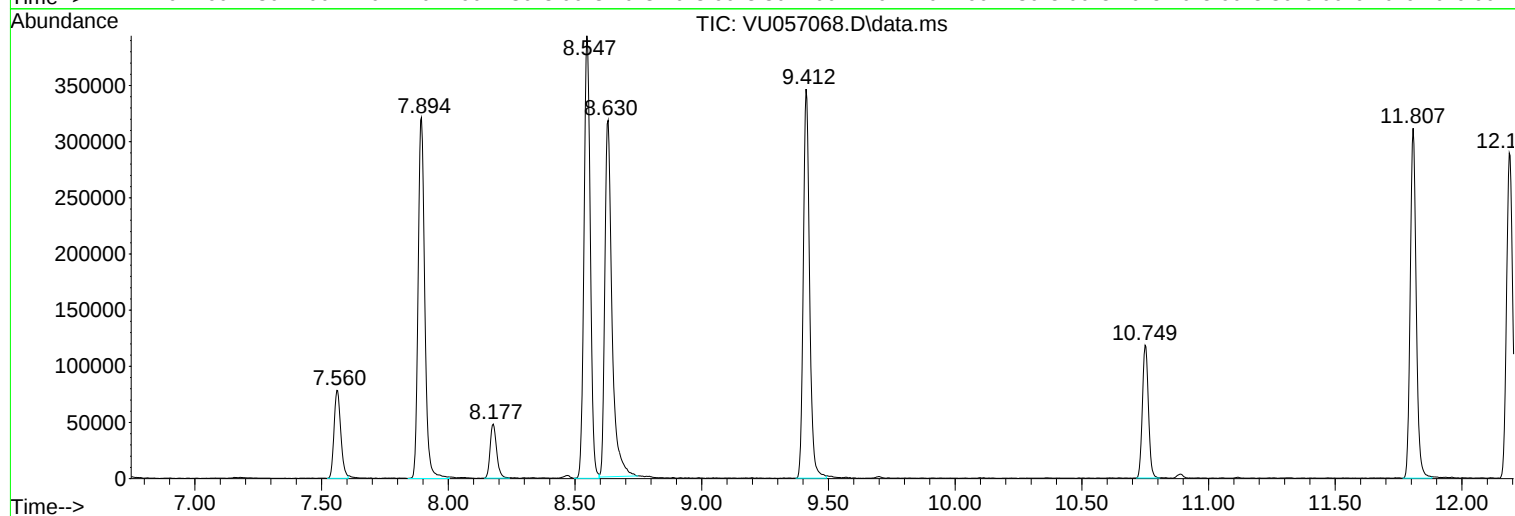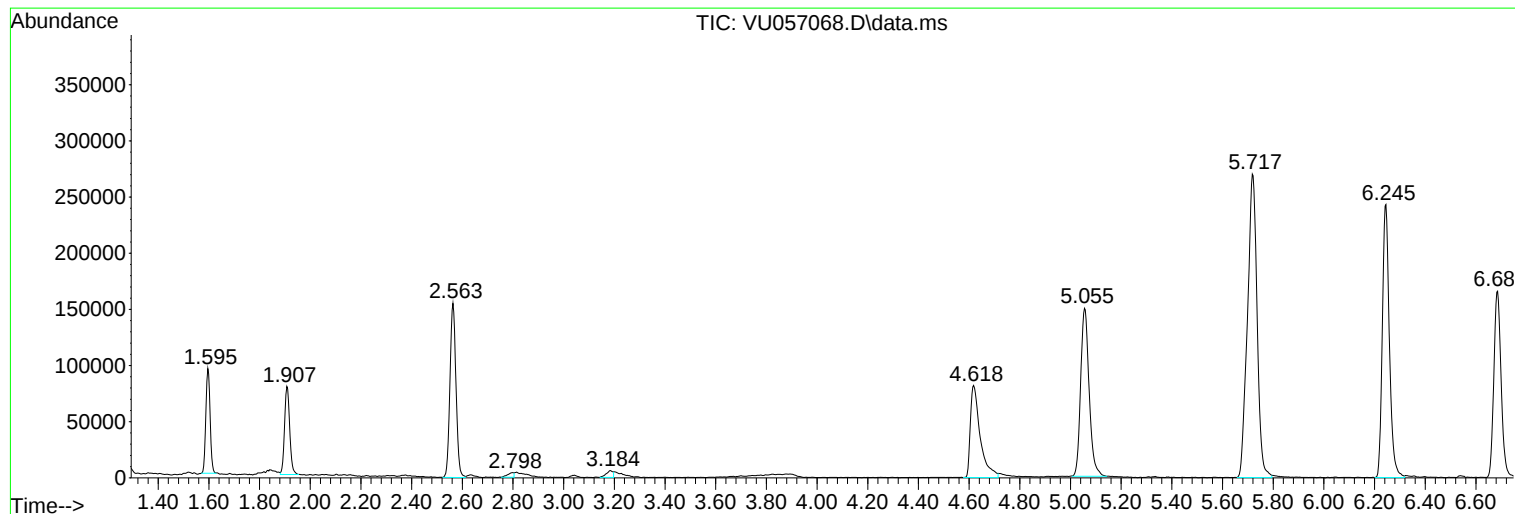

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057068.D
Acq On : 20 Dec 2023 01:14
Operator : MD/SY
Sample : 05865-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057068.D
Acq On : 20 Dec 2023 01:14
Operator : MD/SY
Sample : 05865-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc