

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057073.D
 Acq On : 20 Dec 2023 03:16
 Operator : MD/SY
 Sample : 05890-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGRT6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rVB	88869	100734	15.68%	1.824%
2	1.907	183	192	209	rVB	72488	100072	15.58%	1.812%
3	2.563	384	396	408	rBV	138979	226229	35.22%	4.096%
4	2.621	410	414	427	rVB2	3527	6501	1.01%	0.118%
5	3.042	531	545	560	rVB2	10479	19628	3.06%	0.355%
6	4.615	1024	1034	1064	rBV	73459	193643	30.14%	3.506%
7	4.808	1083	1094	1113	rBV2	12432	29913	4.66%	0.542%
8	5.055	1154	1171	1202	rVB	135769	311385	48.47%	5.637%
9	5.717	1356	1377	1405	rBV2	249926	642392	100.00%	11.630%
10	6.242	1526	1540	1560	rBV	227419	442622	68.90%	8.013%
11	6.682	1664	1677	1698	rBV	150963	298854	46.52%	5.410%
12	7.563	1939	1951	1974	rBV3	70972	131129	20.41%	2.374%
13	7.894	2041	2054	2068	rBV	286109	512293	79.75%	9.274%
14	7.965	2069	2076	2092	rVB2	28589	53259	8.29%	0.964%
15	8.177	2129	2142	2162	rBV2	42515	78142	12.16%	1.415%
16	8.550	2248	2258	2266	rBV7	4339	7514	1.17%	0.136%
17	8.627	2271	2282	2313	rBV2	279813	538441	83.82%	9.748%
18	8.788	2323	2332	2342	rVV4	14010	23495	3.66%	0.425%
19	9.412	2514	2526	2547	rBV	329846	571925	89.03%	10.354%
20	9.695	2604	2614	2623	rBV3	4839	7899	1.23%	0.143%
21	10.097	2728	2739	2757	rVB8	4661	11536	1.80%	0.209%
22	10.749	2931	2942	2961	rBV2	109392	178214	27.74%	3.226%
23	10.884	2974	2984	2996	rBV3	3897	6459	1.01%	0.117%
24	11.688	3227	3234	3243	rBV6	4485	6804	1.06%	0.123%
25	11.807	3257	3271	3292	rBV	313179	516564	80.41%	9.352%
26	12.064	3343	3351	3362	rBV6	8711	17935	2.79%	0.325%
27	12.187	3377	3389	3408	rBV	270014	452189	70.39%	8.186%
28	12.888	3599	3607	3622	rBV7	10557	18359	2.86%	0.332%
29	13.206	3694	3706	3718	rBV4	12736	19611	3.05%	0.355%




Sum of corrected areas: 5523741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057073.D
Acq On : 20 Dec 2023 03:16
Operator : MD/SY
Sample : 05890-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGRT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

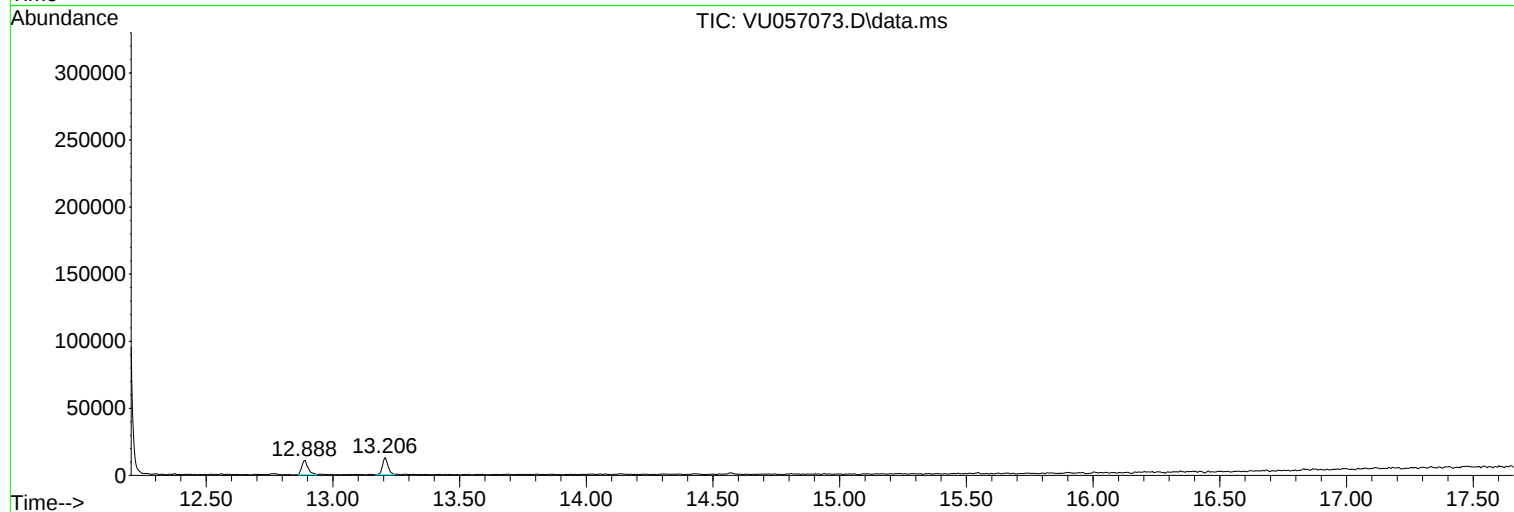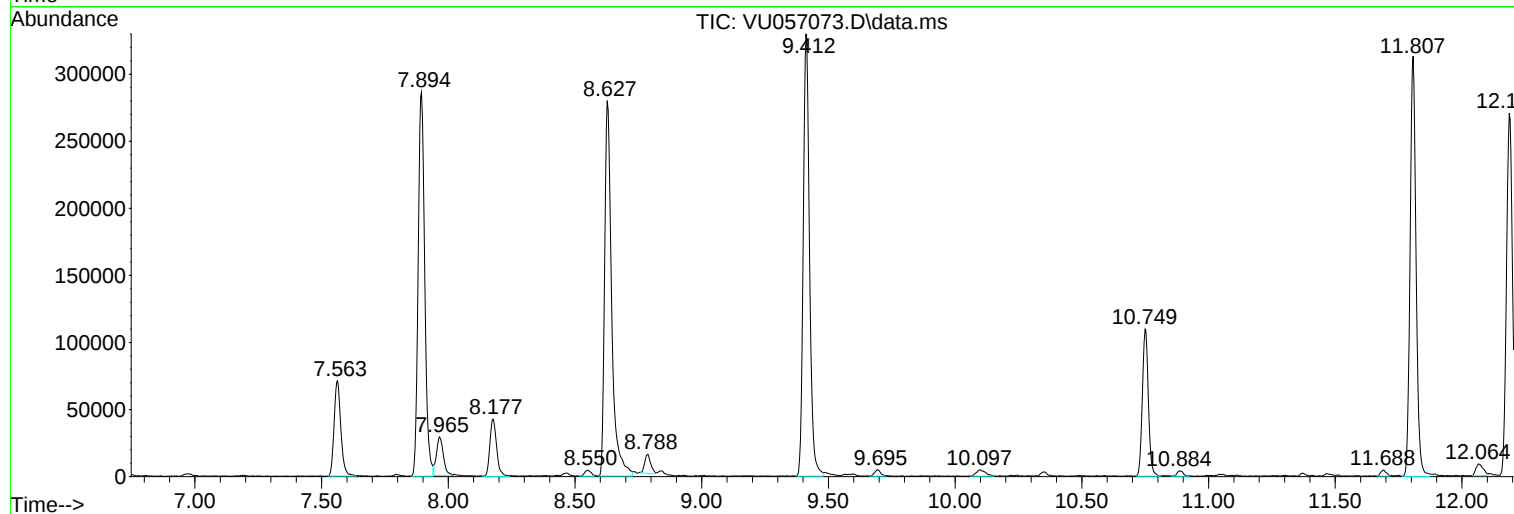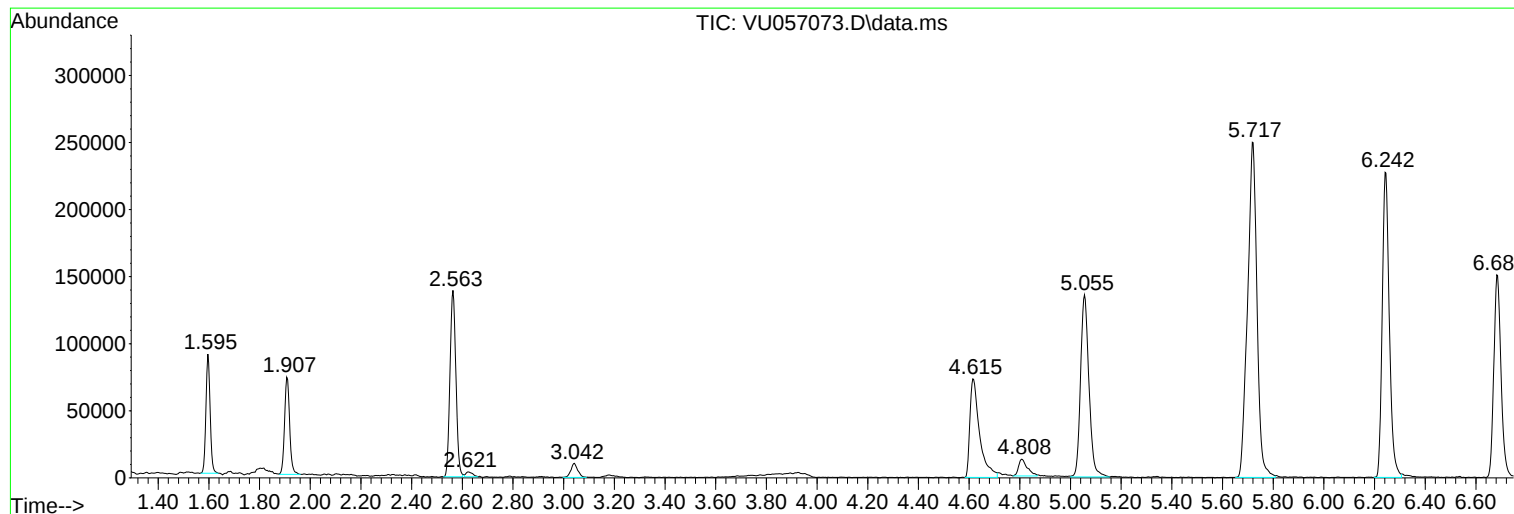

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057073.D
Acq On : 20 Dec 2023 03:16
Operator : MD/SY
Sample : 05890-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGRT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057073.D
Acq On : 20 Dec 2023 03:16
Operator : MD/SY
Sample : 05890-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGRT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc