

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057074.D
 Acq On : 20 Dec 2023 03:40
 Operator : MD/SY
 Sample : 05890-01DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGR39DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	106	rBV	90673	104231	7.43%	1.516%
2	1.907	183	192	205	rVB	74616	99571	7.09%	1.448%
3	2.563	383	396	412	rBV	142025	233227	16.62%	3.392%
4	3.042	533	545	562	rVB2	9984	19436	1.38%	0.283%
5	3.181	575	588	611	rBV2	6590	16263	1.16%	0.237%
6	4.615	1022	1034	1061	rBV	80013	210846	15.02%	3.067%
7	5.055	1155	1171	1204	rVB	141002	317786	22.64%	4.622%
8	5.721	1357	1378	1400	rBV2	250898	661217	47.11%	9.618%
9	6.242	1528	1540	1563	rBV	234482	458250	32.65%	6.665%
10	6.682	1664	1677	1703	rBV	153791	310309	22.11%	4.514%
11	7.560	1938	1950	1975	rBV2	74493	135997	9.69%	1.978%
12	7.894	2038	2054	2078	rBV	296486	532177	37.92%	7.741%
13	8.174	2131	2141	2161	rBV2	44304	78383	5.58%	1.140%
14	8.547	2243	2257	2273	rBV	827729	1403516	100.00%	20.415%
15	8.627	2273	2282	2312	rVB	296013	561269	39.99%	8.164%
16	9.412	2513	2526	2548	rBV	333525	580072	41.33%	8.437%
17	10.749	2930	2942	2958	rBV	114219	184413	13.14%	2.682%
18	11.807	3257	3271	3288	rBV	315195	512978	36.55%	7.461%
19	12.187	3375	3389	3408	rBV	269839	455149	32.43%	6.620%




Sum of corrected areas: 6875090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057074.D
Acq On : 20 Dec 2023 03:40
Operator : MD/SY
Sample : 05890-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

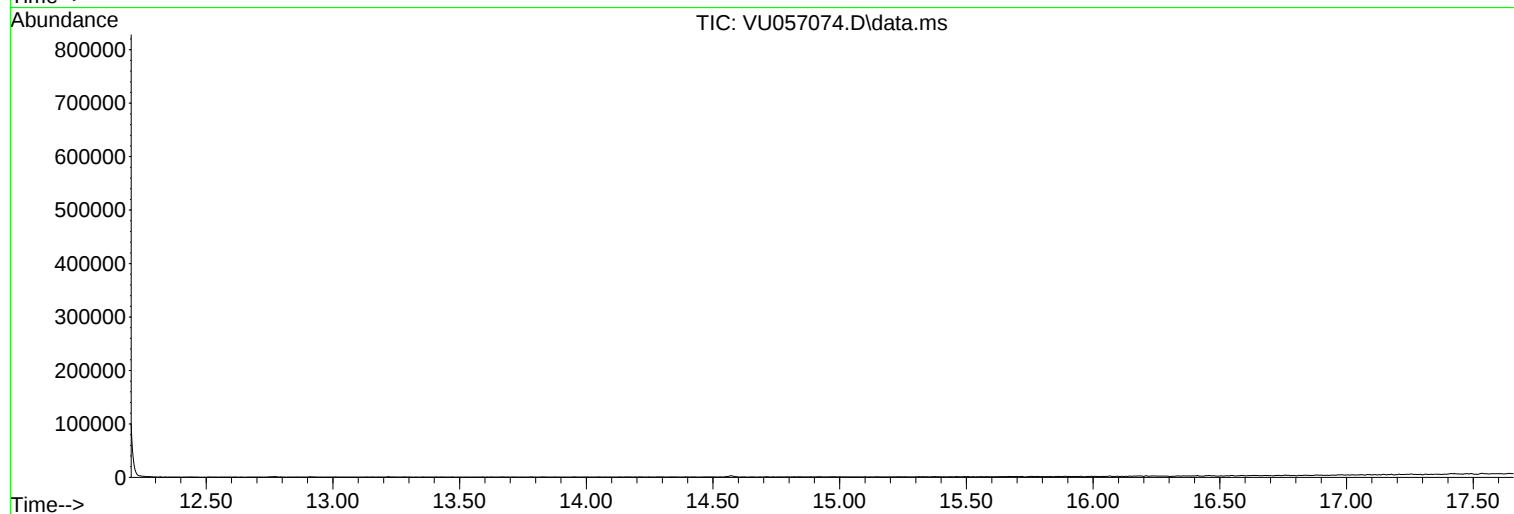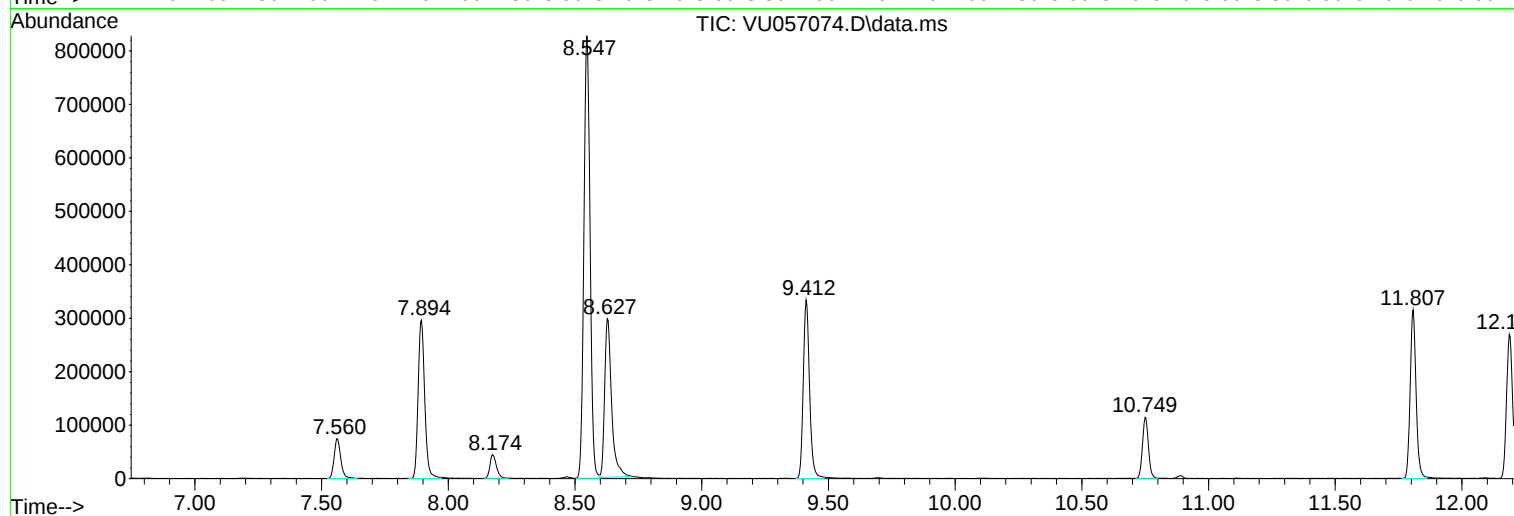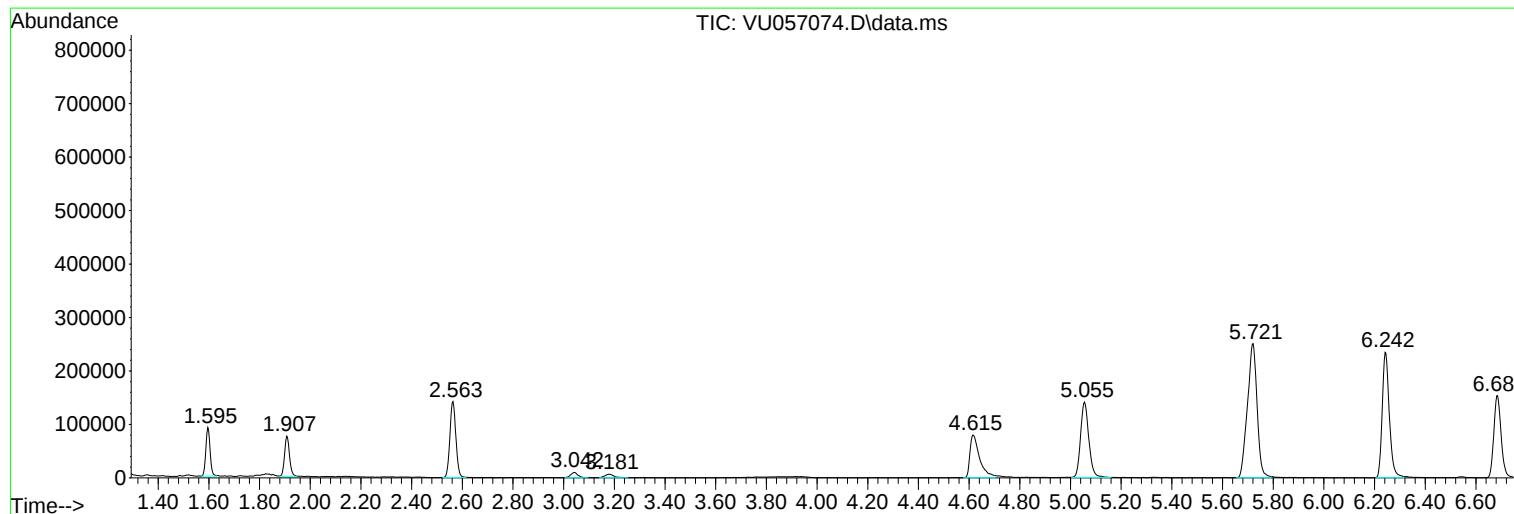

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057074.D
Acq On : 20 Dec 2023 03:40
Operator : MD/SY
Sample : 05890-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057074.D
Acq On : 20 Dec 2023 03:40
Operator : MD/SY
Sample : 05890-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------