

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
 Data File : VU057075.D
 Acq On : 20 Dec 2023 04:04
 Operator : MD/SY
 Sample : 05890-02DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGR40DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rVB	92856	108331	13.02%	1.634%
2	1.908	183	192	211	rVB	77019	107586	12.93%	1.623%
3	2.563	382	396	414	rBV	148627	247036	29.68%	3.727%
4	3.039	533	544	562	rVB3	9591	19733	2.37%	0.298%
5	3.178	574	587	606	rBV2	9137	21665	2.60%	0.327%
6	4.618	1021	1035	1071	rBV	86195	271650	32.64%	4.098%
7	5.055	1155	1171	1194	rBV	143200	324876	39.03%	4.901%
8	5.718	1356	1377	1399	rBV2	262891	687089	82.55%	10.366%
9	6.242	1528	1540	1569	rBV	240585	474688	57.03%	7.162%
10	6.534	1621	1631	1650	rVB4	13334	26838	3.22%	0.405%
11	6.682	1664	1677	1702	rBV	162470	323887	38.91%	4.886%
12	7.560	1936	1950	1974	rBV	78230	141328	16.98%	2.132%
13	7.894	2040	2054	2072	rBV	307569	551947	66.31%	8.327%
14	8.177	2131	2142	2159	rBV	48039	84553	10.16%	1.276%
15	8.547	2244	2257	2272	rBV	490859	832347	100.00%	12.558%
16	8.631	2272	2283	2315	rVB2	308159	602919	72.44%	9.096%
17	9.412	2513	2526	2554	rBV	351397	607261	72.96%	9.162%
18	10.750	2931	2942	2963	rBV	118455	193725	23.27%	2.923%
19	11.807	3258	3271	3290	rBV	321985	525040	63.08%	7.921%
20	12.187	3377	3389	3409	rBV	284091	475720	57.15%	7.177%




Sum of corrected areas: 6628219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057075.D
Acq On : 20 Dec 2023 04:04
Operator : MD/SY
Sample : 05890-02DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

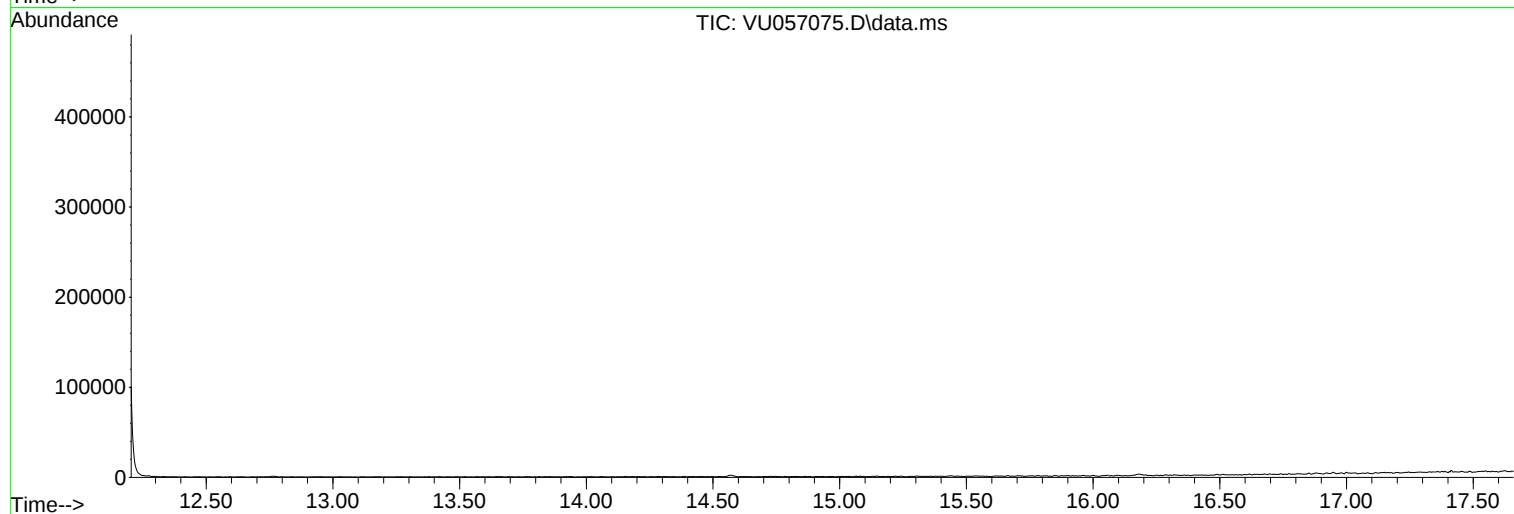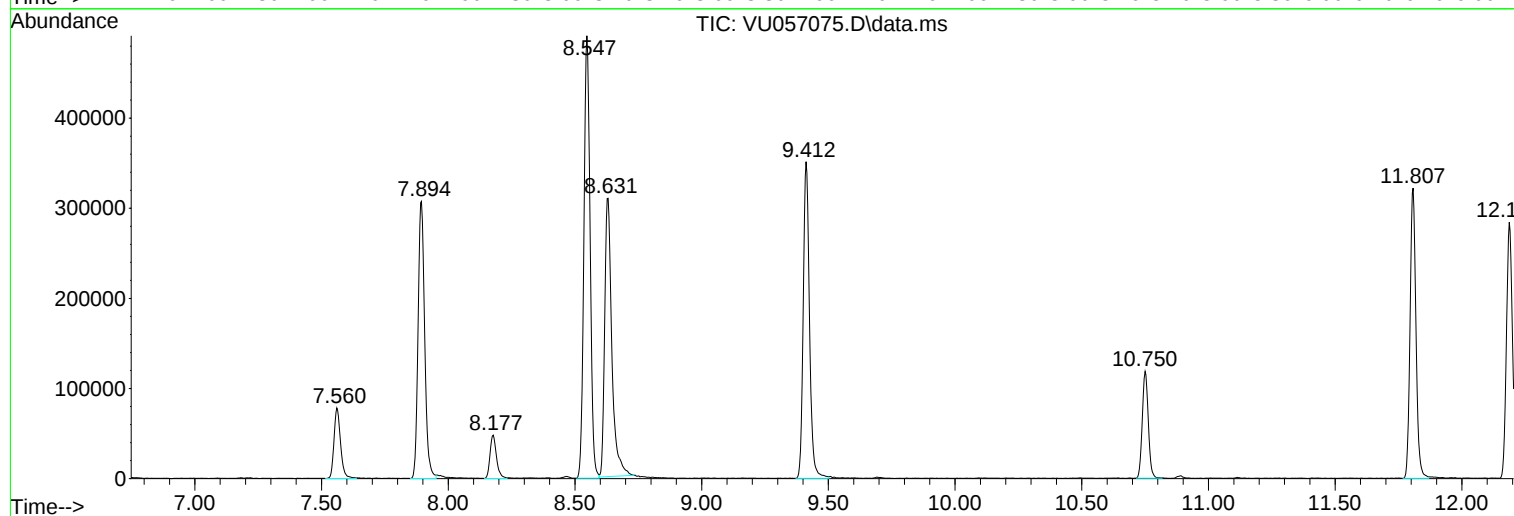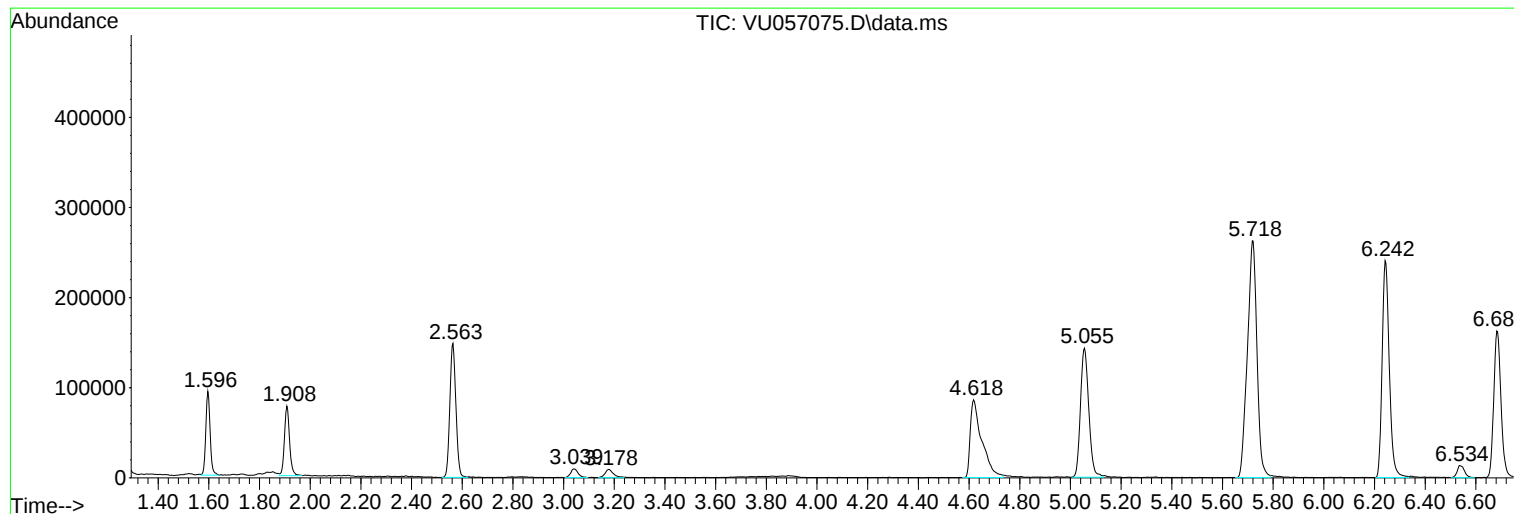

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057075.D
Acq On : 20 Dec 2023 04:04
Operator : MD/SY
Sample : 05890-02DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057075.D
Acq On : 20 Dec 2023 04:04
Operator : MD/SY
Sample : 05890-02DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------