


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121923\
Data File : VU057031.D
Acq On : 19 Dec 2023 08:34
Operator : MD/SY
Sample : BFB097
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB097

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 20 06:35:40 2023

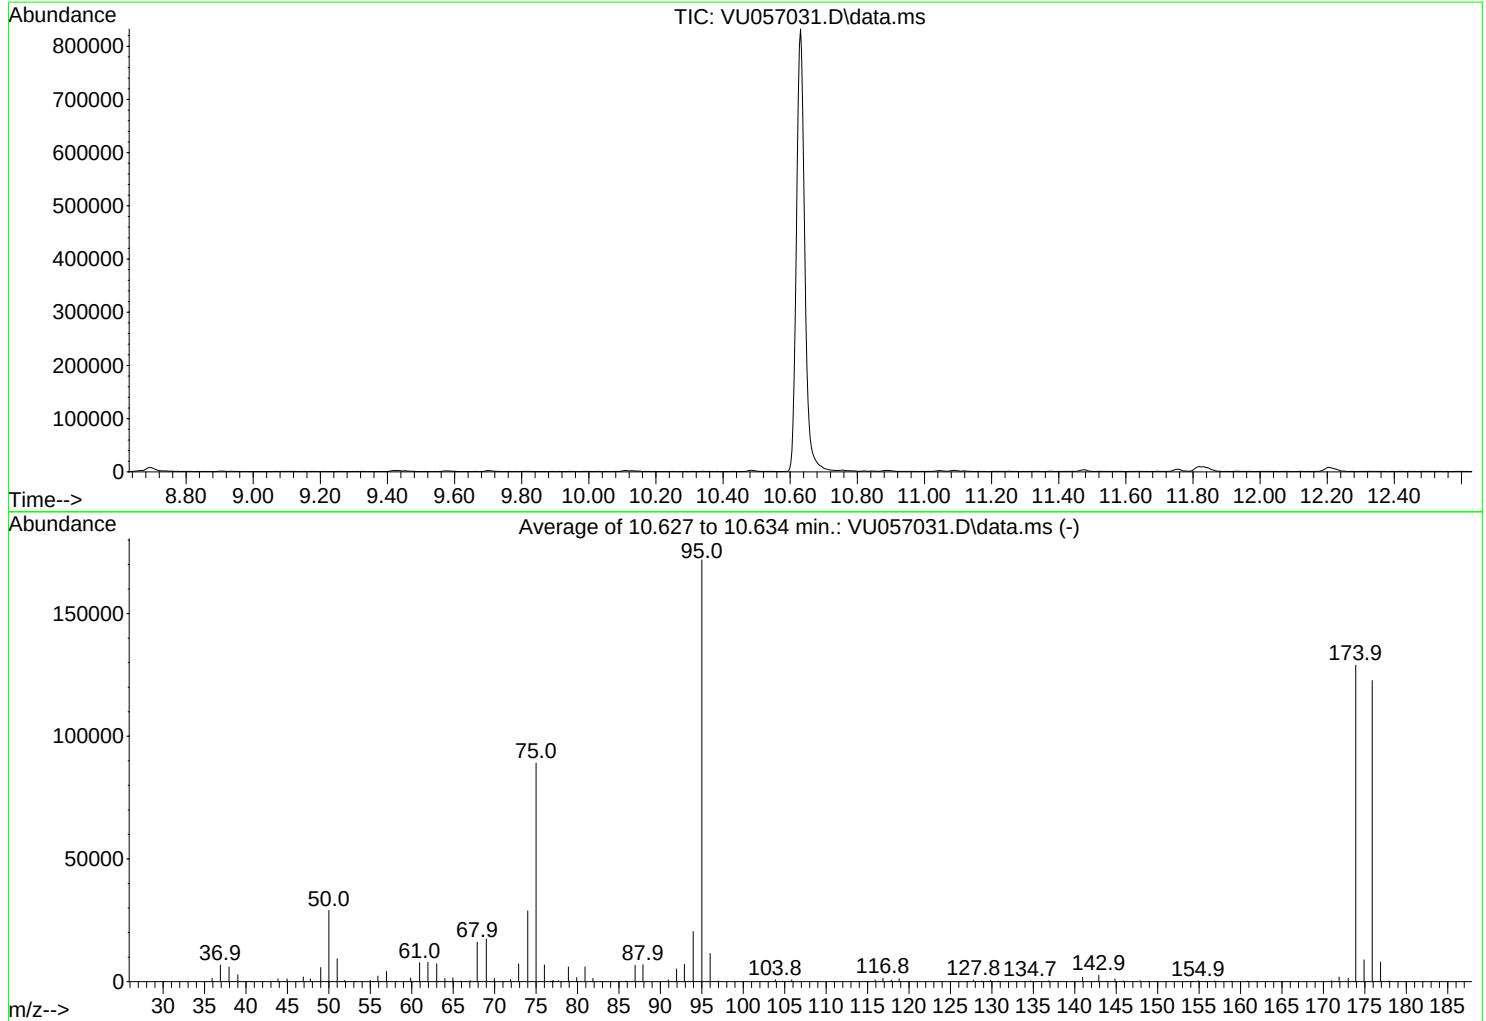

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	28997	PASS
75	95	30	80	51.8	89096	PASS
95	95	100	100	100.0	171904	PASS
96	95	5	9	6.7	11479	PASS
173	174	0.00	2	1.1	1356	PASS
174	95	50	120	75.0	128989	PASS
175	174	5	9	6.9	8858	PASS
176	174	95	101	95.2	122744	PASS
177	176	5	9	6.5	7928	PASS

m/z	Abundance
39.70	274.0
44.10	380.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

m/z	Abundance
35.90	1435.0
36.90	6827.0
37.90	5764.0
39.00	2758.0
39.90	347.0
40.60	106.0
43.90	1242.0
45.00	1041.0
46.10	123.0
46.90	1983.0
47.80	1130.0
49.00	5733.0
50.00	28576.0
51.00	9818.0
51.90	463.0
52.70	111.0
53.10	118.0
53.90	123.0
55.00	454.0
55.90	2137.0
56.90	4125.0
58.10	216.0
59.90	1507.0
60.90	7584.0
61.90	8200.0
63.00	7182.0
64.00	1254.0
64.90	1568.0
65.90	322.0
67.00	409.0
67.90	16392.0
69.00	17096.0
70.00	1338.0
71.90	794.0
72.90	7071.0
74.00	28904.0
75.00	90304.0
76.00	6898.0
77.10	982.0
78.00	627.0
78.90	5958.0
79.90	1662.0
80.90	6126.0
81.80	1380.0
85.90	303.0
87.00	6845.0
87.90	6618.0
90.90	781.0
91.90	4768.0
92.90	7120.0
93.90	19488.0
95.00	173056.0
96.00	11401.0
97.00	234.0
103.90	810.0
104.80	422.0
105.80	811.0
106.80	202.0
111.00	207.0
113.00	132.0
115.90	786.0
116.90	1402.0
117.80	619.0
118.80	1252.0
123.90	133.0
127.80	626.0
128.80	291.0
129.90	597.0
130.80	264.0
134.60	376.0
135.00	246.0
136.80	302.0
141.00	1757.0
141.90	246.0
142.90	2651.0
143.90	201.0
144.90	1160.0
145.90	303.0
147.80	436.0
149.80	115.0
154.90	362.0
156.90	227.0
159.00	183.0
160.90	247.0
171.00	334.0
171.90	1905.0
173.00	1266.0
173.90	124808.0
174.90	9143.0
175.90	119760.0
176.90	8131.0
177.90	294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

m/z	Abundance
35.90	1484.0
36.90	7074.0
37.90	6109.0
39.00	2751.0
39.80	309.0
43.90	1179.0
44.90	1131.0
46.10	125.0
46.90	2016.0
47.80	1163.0
49.00	5933.0
50.00	29864.0
51.00	9666.0
51.90	481.0
52.80	134.0
53.90	116.0
55.00	478.0
55.90	2450.0
57.00	4290.0
58.10	216.0
59.90	1419.0
61.00	7884.0
62.00	8079.0
63.00	7677.0
64.00	1307.0
65.00	1561.0
66.00	246.0
67.10	471.0
67.90	16624.0
69.00	18216.0
70.00	1396.0
71.90	936.0
72.90	7476.0
74.00	29784.0
75.00	91992.0
76.00	7090.0
77.00	818.0
77.70	610.0
78.90	6140.0
79.90	1690.0
80.90	6212.0
81.80	1312.0
82.80	106.0
85.90	347.0
86.90	6767.0
87.90	7221.0
90.90	737.0
92.00	5295.0
92.90	7341.0
93.90	21176.0
95.00	176256.0
96.00	11916.0
97.00	275.0
103.80	858.0
104.70	335.0
105.90	770.0
106.80	151.0
110.90	223.0
113.00	161.0
114.70	202.0
115.90	767.0
116.80	1446.0
117.90	711.0
118.80	1203.0
123.90	160.0
127.80	712.0
128.80	296.0
129.90	606.0
130.80	245.0
134.60	390.0
136.80	337.0
141.00	1885.0
142.00	223.0
142.90	2675.0
143.80	181.0
144.90	1183.0
145.80	341.0
147.90	370.0
148.90	125.0
149.80	113.0
154.90	403.0
155.90	147.0
156.90	319.0
158.90	202.0
160.90	222.0
171.00	387.0
171.90	1983.0
173.00	1401.0
173.90	132928.0
174.90	9165.0
175.90	126712.0
176.90	8019.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

177.90

359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

m/z	Abundance
35.90	1348.0
36.90	6566.0
38.00	5890.0
39.00	2630.0
39.80	357.0
40.10	353.0
43.80	1117.0
44.90	1184.0
46.10	125.0
46.90	1736.0
47.70	1058.0
49.00	5590.0
50.00	28552.0
51.00	8513.0
51.90	373.0
52.80	120.0
53.90	103.0
55.00	528.0
55.90	2348.0
57.00	4018.0
58.10	190.0
59.80	1402.0
61.00	7807.0
61.90	7550.0
63.00	7143.0
64.00	1202.0
65.00	1566.0
66.00	168.0
67.10	455.0
67.90	15364.0
69.00	16888.0
69.90	1343.0
71.00	104.0
71.90	930.0
72.90	7211.0
74.00	27808.0
75.00	84992.0
76.00	6550.0
76.80	797.0
77.70	651.0
78.90	5895.0
79.90	1539.0
80.90	5710.0
81.90	1184.0
82.70	104.0
85.80	345.0
86.90	6274.0
87.90	6898.0
91.00	715.0
92.00	5432.0
92.90	6956.0
94.00	20656.0
95.00	166400.0
96.00	11119.0
97.00	284.0
103.80	782.0
104.70	309.0
105.90	674.0
106.90	126.0
110.90	195.0
113.00	147.0
114.80	286.0
115.90	635.0
116.90	1421.0
117.90	690.0
118.80	1217.0
123.90	174.0
127.80	712.0
128.80	348.0
129.80	545.0
130.80	214.0
134.70	359.0
136.90	364.0
140.90	1887.0
142.90	2494.0
143.70	163.0
144.80	1055.0
145.80	352.0
148.00	310.0
148.80	132.0
154.10	114.0
154.90	421.0
155.80	193.0
156.90	349.0
158.80	269.0
160.80	166.0
170.90	467.0
171.90	1880.0
173.00	1402.0
173.90	129232.0
174.90	8265.0
175.90	121760.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

176.907634.0

177.90331.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097