

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028839.D
 Acq On : 20 Dec 2018 21:07
 Operator : MD/SY
 Sample : J6507-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF030

Quant Time: Dec 21 06:22:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 21 05:57:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	196213	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	181401	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	75330	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	65081	41.37	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.74%
7) Chloroethane-d5	1.67	69	52544	43.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.50%
11) 1,1-Dichloroethene-d2	2.27	63	84803	32.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.12%
21) 2-Butanone-d5	4.18	46	113787	103.25	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.25%
24) Chloroform-d	4.65	84	111099	44.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.82%
26) 1,2-Dichloroethane-d4	5.31	65	72077	47.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.54%
32) Benzene-d6	5.34	84	242340	47.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.58%
36) 1,2-Dichloropropane-d6	6.33	67	86324	49.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.16%
41) Toluene-d8	7.57	98	213059	45.88	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.76%
43) trans-1,3-Dichloropropene-	7.85	79	36473	46.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.50%
47) 2-Hexanone-d5	8.31	63	87570	105.90	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.90%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	116348	48.17	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.34%
64) 1,2-Dichlorobenzene-d4	11.86	152	76687	50.33	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.66%


Target Compounds					Qvalue
13) Acetone	2.32	43	7651	6.812 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028839.D
 Acq On : 20 Dec 2018 21:07
 Operator : MD/SY
 Sample : J6507-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 BF030

Quant Time: Dec 21 06:22:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 21 05:57:29 2018
 Response via : Initial Calibration

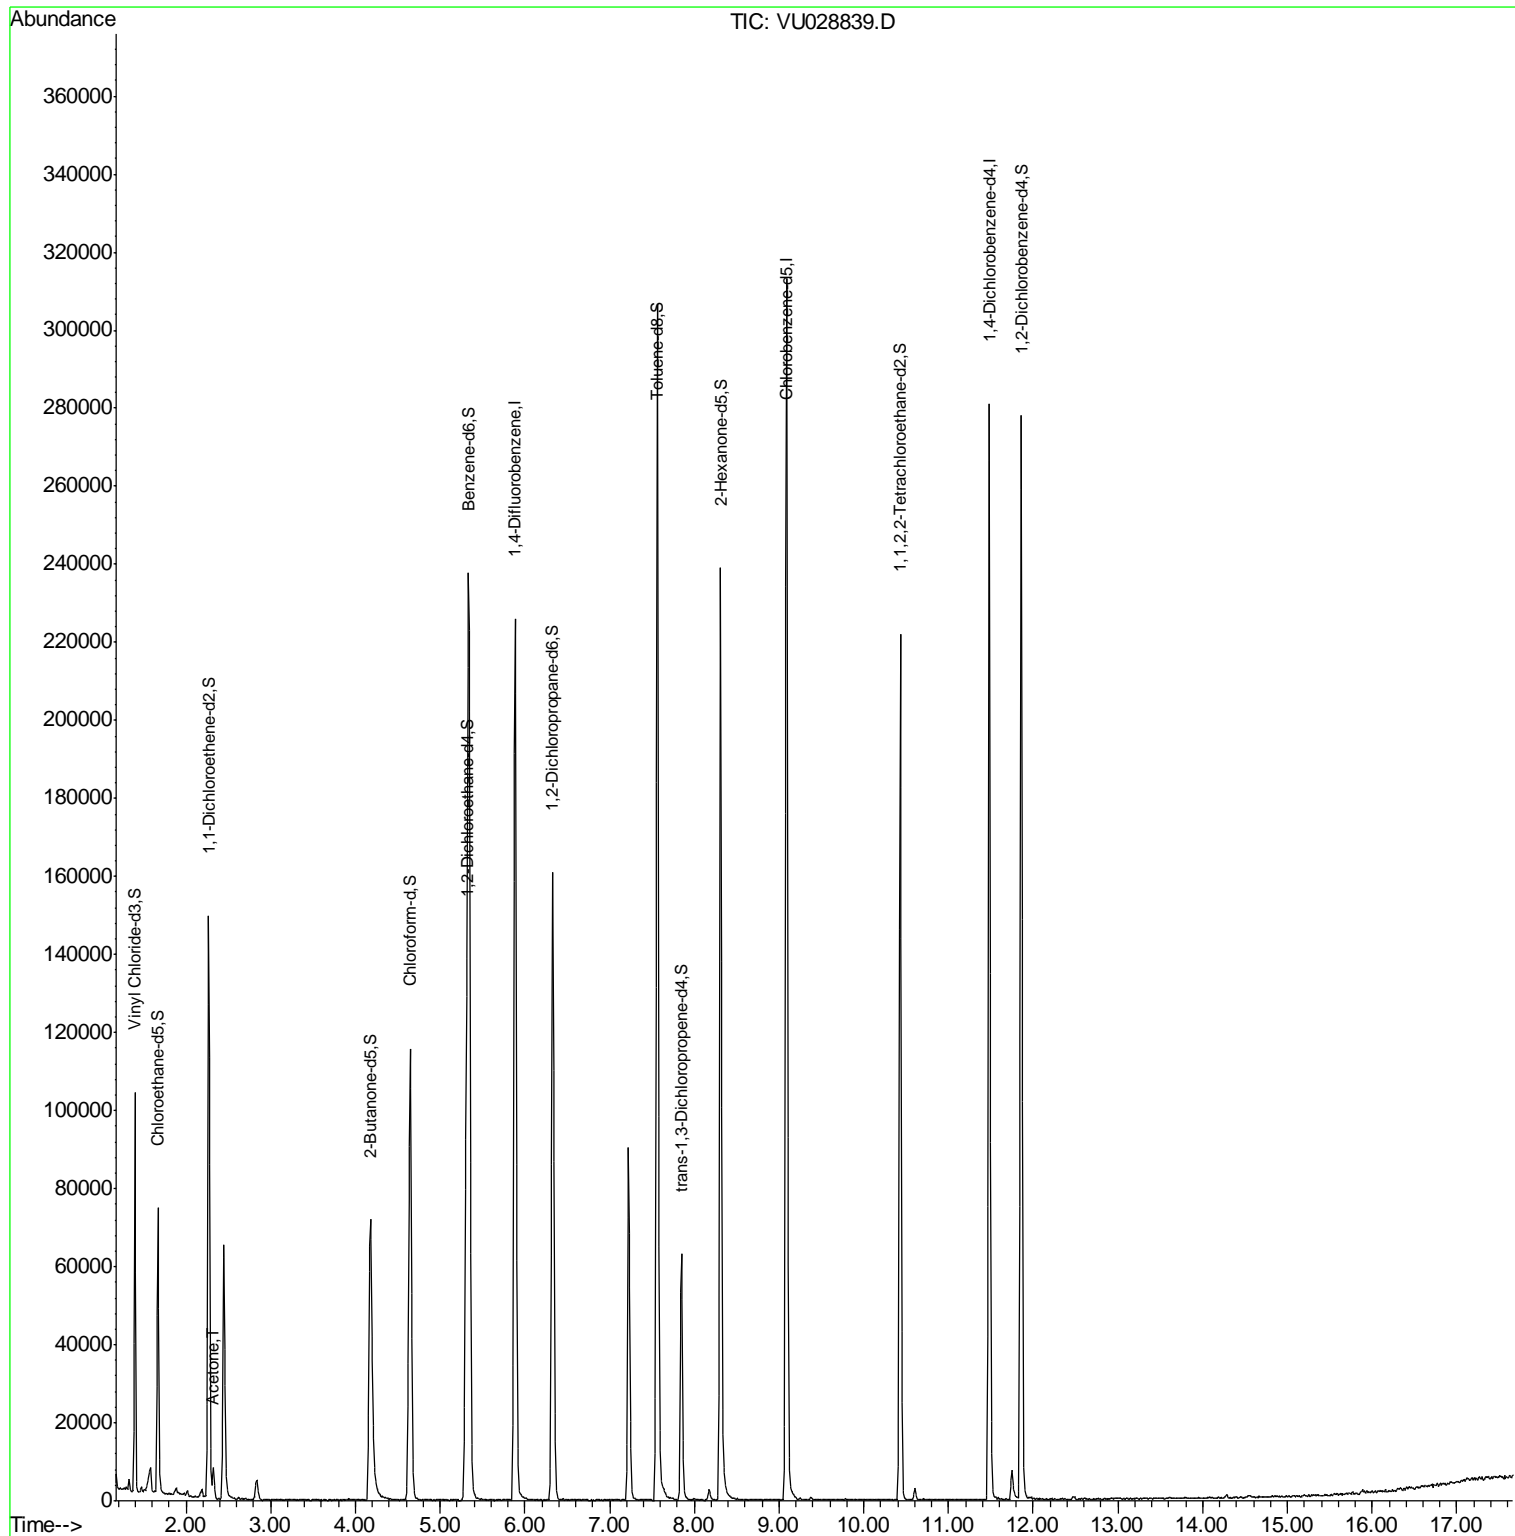

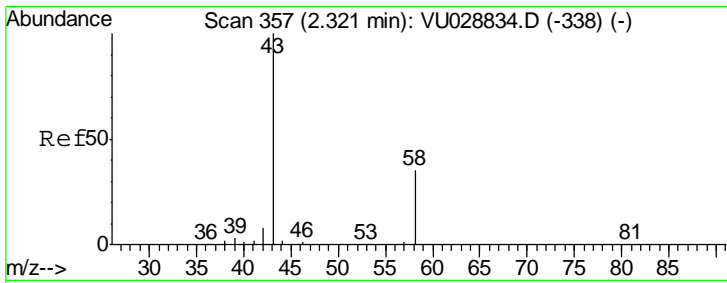

#13
 Acetone
 Concen: 6.812 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VU028839.D
 Acq: 20 Dec 2018 21:07

Instrument :
 MSVOA_U
 ClientSampleId :
 BF030

Tgt Ion: 43 Resp: 7651
 Ion Ratio Lower Upper
 43 100
 58 33.1 0.0 70.2

