

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U122018\
 Data File : VU028842.D
 Acq On : 20 Dec 2018 22:19
 Operator : MD/SY
 Sample : J6506-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF010

Quant Time: Dec 21 06:31:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 21 05:57:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	194813	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	182631	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	74531	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	64743	41.45	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.90%
7) Chloroethane-d5	1.67	69	52625	43.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.24%
11) 1,1-Dichloroethene-d2	2.27	63	85118	32.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.82%
21) 2-Butanone-d5	4.17	46	117469	107.35	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.35%
24) Chloroform-d	4.65	84	113412	46.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.36%
26) 1,2-Dichloroethane-d4	5.31	65	72803	48.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.18%
32) Benzene-d6	5.34	84	244952	47.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.96%
36) 1,2-Dichloropropane-d6	6.33	67	86669	49.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.90%
41) Toluene-d8	7.57	98	215149	46.02	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.04%
43) trans-1,3-Dichloropropene-	7.85	79	36236	46.14	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.28%
47) 2-Hexanone-d5	8.31	63	91172	109.52	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.52%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	118090	48.56	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.12%
64) 1,2-Dichlorobenzene-d4	11.86	152	76660	50.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.72%


Target Compounds					Qvalue
13) Acetone	2.32	43	3608	3.236 ug/L	98
34) Trichloroethene	6.19	95	2388	1.701 ug/L	93
46) Tetrachloroethene	8.22	164	92229	85.311 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
Data File : VU028842.D
Acq On : 20 Dec 2018 22:19
Operator : MD/SY
Sample : J6506-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF010

Quant Time: Dec 21 06:31:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 21 05:57:29 2018
Response via : Initial Calibration

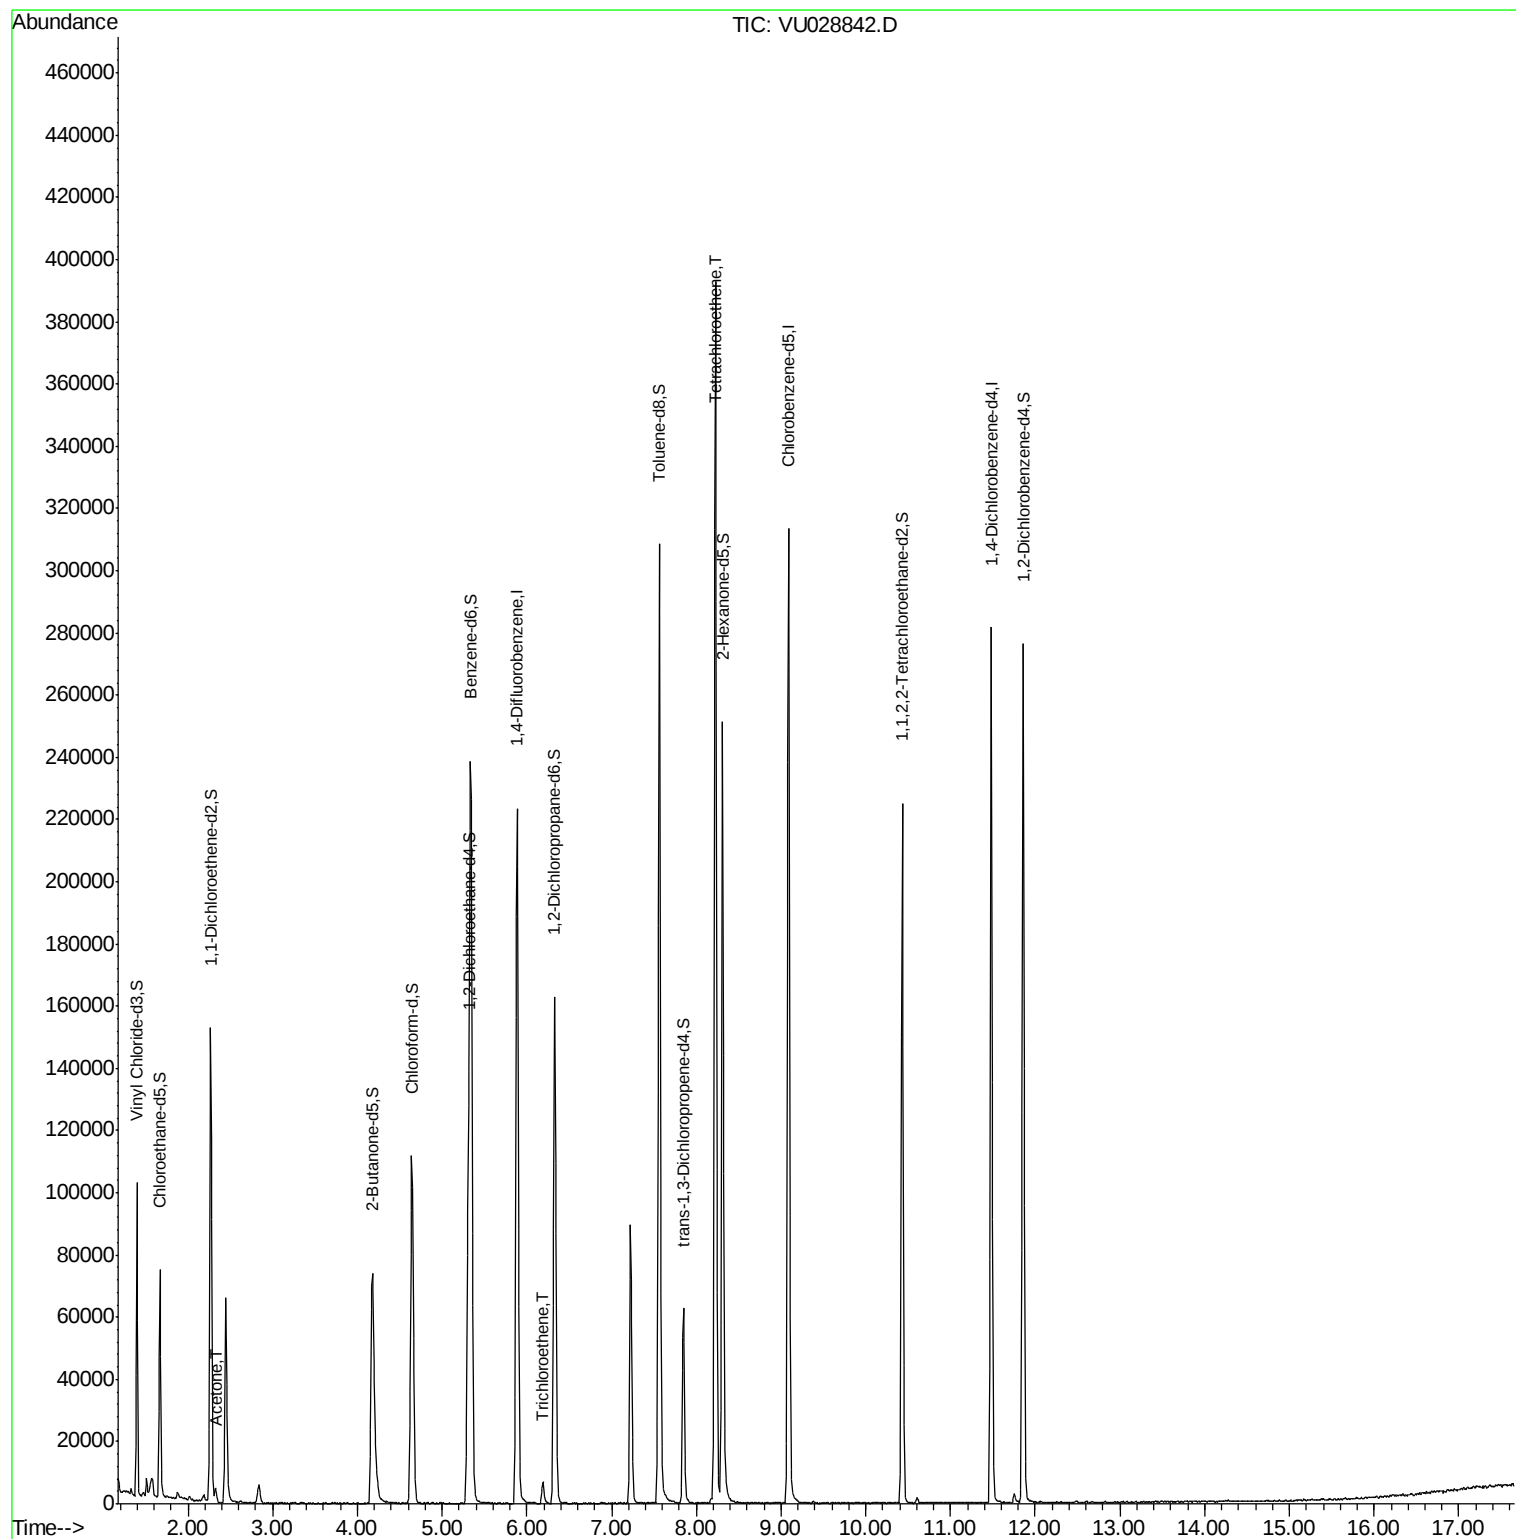

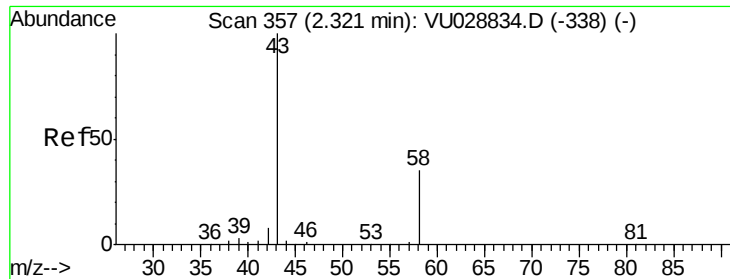

#13

Acetone

Concen: 3.236 ug/L

RT: 2.32 min Scan# 357

Delta R.T. 0.00 min

Lab File: VU028842.D

Acq: 20 Dec 2018 22:19

Instrument :

MSVOA_U

ClientSampled :


BF010

Tgt Ion: 43 Resp: 3608

Ion Ratio Lower Upper




43 100

58 34.0 0.0 70.2

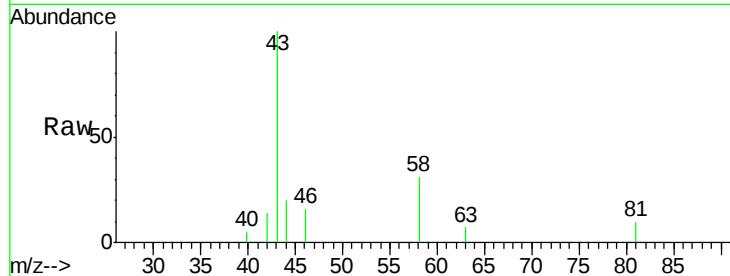

Abundance Ion 43.00 (42.70 to 43.70): VU028834.D (-338) (-)

Ion 58.00 (57.70 to 58.70): VU028834.D (-338) (-)

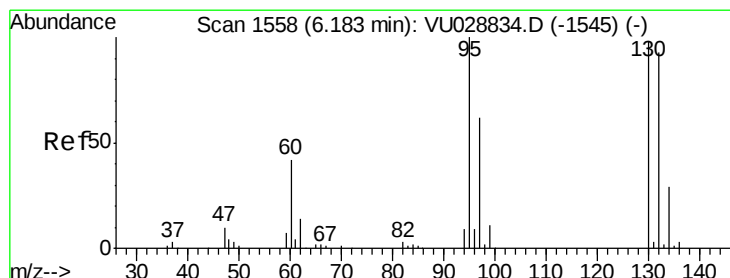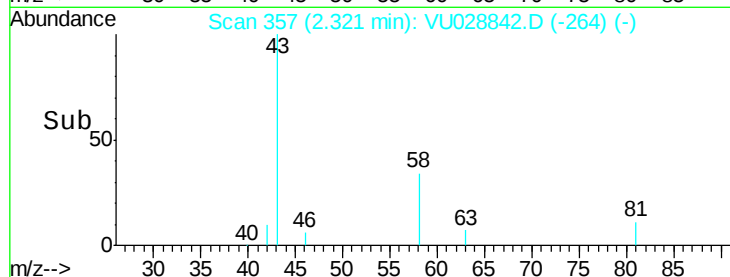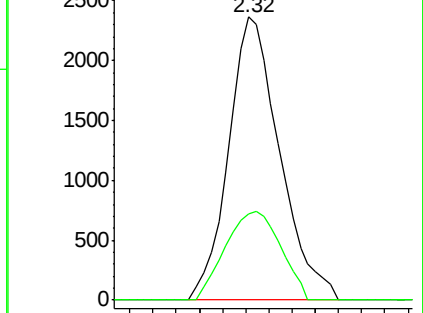

#34

Trichloroethene

Concen: 1.701 ug/L

RT: 6.19 min Scan# 1560

Delta R.T. 0.01 min

Lab File: VU028842.D

Acq: 20 Dec 2018 22:19

Tgt Ion: 95 Resp: 2388


Ion Ratio Lower Upper

95 100

97 61.1 43.3 80.3

132 81.2 64.2 119.2

130 101.9 67.1 124.7


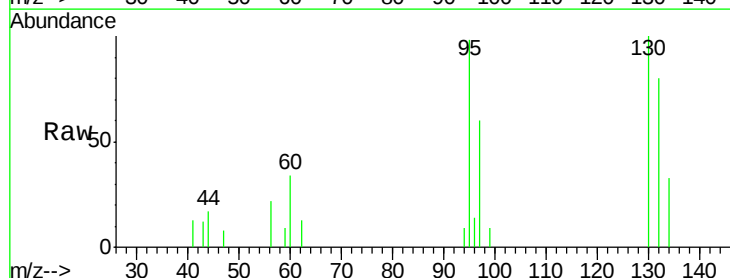



Abundance Ion 95.00 (94.70 to 95.70): VU028834.D (-1545) (-)

Ion 97.00 (96.70 to 97.70): VU028834.D (-1545) (-)

Ion 132.00 (131.70 to 132.70): VU028834.D (-1545) (-)

Ion 130.00 (129.70 to 130.70): VU028834.D (-1545) (-)

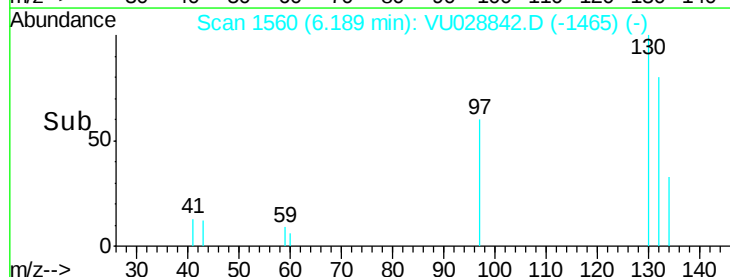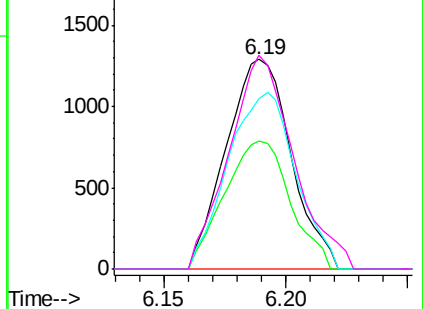

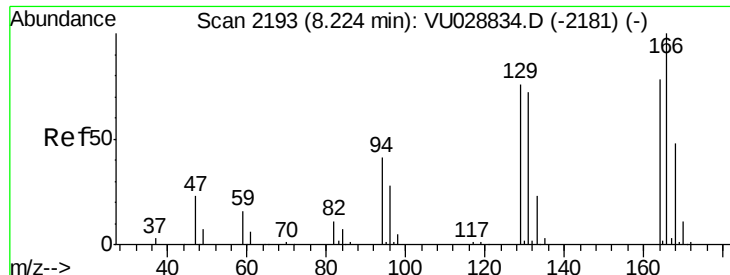

#46

Tetrachloroethene

Concen: 85.311 ug/L

RT: 8.22 min Scan# 2193

Delta R.T. 0.00 min

Lab File: VU028842.D


Acq: 20 Dec 2018 22:19

Instrument :

MSVOA_U

ClientSampleId :

BF010

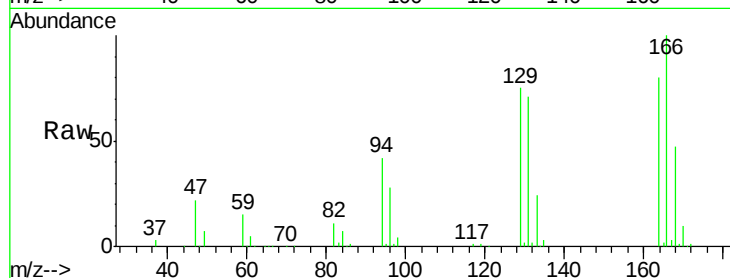

Tgt Ion:164 Resp: 92229

Ion Ratio Lower Upper

164 100

129 93.8 66.8 124.0

131 88.8 64.2 119.2

166 125.7 90.8 168.6

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

