

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028816.D
 Acq On : 20 Dec 2018 11:54
 Operator : MD/SY
 Sample : VU1220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	63	70	81	rBV	122084	122661	15.97%	2.146%
2	1.672	148	155	174	rVB	86597	109459	14.25%	1.915%
3	2.270	330	341	354	rBV	177143	267475	34.81%	4.679%
4	2.472	399	404	416	rVB	2523	3961	0.52%	0.069%
5	2.553	426	429	434	rVB	200	175	0.02%	0.003%
6	2.607	444	446	447	rBV	230	98	0.01%	0.002%
7	2.694	468	473	482	rVB4	1123	1646	0.21%	0.029%
8	2.823	509	513	514	rBV2	455	335	0.04%	0.006%
9	2.984	557	563	572	rBV3	734	1051	0.14%	0.018%
10	3.058	583	586	588	rBV	122	67	0.01%	0.001%
11	3.074	589	591	595	rVB	165	56	0.01%	0.001%
12	3.199	628	630	632	rVB	158	68	0.01%	0.001%
13	3.305	660	663	669	rVB	83	78	0.01%	0.001%
14	3.360	678	680	682	rBV	136	65	0.01%	0.001%
15	3.418	694	698	704	rBV	111	141	0.02%	0.002%
16	3.501	720	724	726	rBV	92	73	0.01%	0.001%
17	3.656	768	772	775	rBV	117	106	0.01%	0.002%
18	3.739	795	798	800	rBV	70	52	0.01%	0.001%
19	3.810	818	820	823	rBV	169	88	0.01%	0.002%
20	3.829	823	826	831	rVV	105	87	0.01%	0.002%
21	3.900	846	848	853	rVB	181	60	0.01%	0.001%
22	3.971	868	870	871	rBV	165	53	0.01%	0.001%
23	4.016	879	884	889	rBV	89	95	0.01%	0.002%
24	4.041	889	892	897	rVB	70	58	0.01%	0.001%
25	4.173	920	933	963	rBV	66332	177072	23.05%	3.097%
26	4.389	998	1000	1007	rVB	345	192	0.02%	0.003%
27	4.469	1023	1025	1027	rBV	135	59	0.01%	0.001%
28	4.537	1042	1046	1050	rVB	170	80	0.01%	0.001%
29	4.562	1050	1054	1059	rBV2	237	192	0.02%	0.003%
30	4.646	1063	1080	1101	rBV	124025	284959	37.09%	4.985%
31	4.874	1148	1151	1153	rBV2	178	105	0.01%	0.002%
32	4.942	1168	1172	1178	rBV2	337	230	0.03%	0.004%
33	4.971	1178	1181	1186	rVB	107	102	0.01%	0.002%
34	5.000	1186	1190	1195	rBV	216	168	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028816.D
 Acq On : 20 Dec 2018 11:54
 Operator : MD/SY
 Sample : VU1220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

35	5.051	1203	1206	1208	rBV	200	130	0.02%	0.002%
36	5.093	1217	1219	1221	rBV	134	82	0.01%	0.001%
37	5.135	1226	1232	1236	rBV2	249	208	0.03%	0.004%
38	5.202	1249	1253	1256	rVB	152	93	0.01%	0.002%
39	5.337	1271	1295	1327	rBV2	267319	768285	100.00%	13.439%
40	5.588	1369	1373	1376	rBV	111	88	0.01%	0.002%
41	5.633	1385	1387	1388	rBV	130	58	0.01%	0.001%
42	5.771	1426	1430	1433	rBV	121	93	0.01%	0.002%
43	5.884	1451	1465	1487	rBV	224300	439417	57.19%	7.686%
44	6.186	1551	1559	1565	rBV5	800	1172	0.15%	0.021%
45	6.228	1570	1572	1578	rVB	93	67	0.01%	0.001%
46	6.328	1589	1603	1625	rBV2	175092	348482	45.36%	6.096%
47	6.450	1638	1641	1646	rBV3	397	338	0.04%	0.006%
48	6.495	1653	1655	1658	rVB	112	58	0.01%	0.001%
49	6.520	1658	1663	1665	rBV	84	74	0.01%	0.001%
50	6.565	1673	1677	1679	rBV	137	99	0.01%	0.002%
51	6.717	1721	1724	1729	rVB2	200	176	0.02%	0.003%
52	6.755	1733	1736	1743	rVB	98	93	0.01%	0.002%
53	6.791	1743	1747	1750	rBV	75	63	0.01%	0.001%
54	6.810	1750	1753	1755	rBV	100	65	0.01%	0.001%
55	6.861	1766	1769	1774	rVB	166	100	0.01%	0.002%
56	6.961	1797	1800	1804	rBV	185	110	0.01%	0.002%
57	7.106	1843	1845	1851	rBV	166	129	0.02%	0.002%
58	7.225	1866	1882	1905	rBV	103792	182832	23.80%	3.198%
59	7.363	1923	1925	1927	rVB	138	58	0.01%	0.001%
60	7.427	1942	1945	1951	rBV2	327	275	0.04%	0.005%
61	7.459	1951	1955	1961	rBV2	264	384	0.05%	0.007%
62	7.562	1974	1987	2007	rBV	351499	617827	80.42%	10.807%
63	7.848	2065	2076	2095	rVV	69878	117575	15.30%	2.057%
64	7.993	2120	2121	2127	rVB	205	100	0.01%	0.002%
65	8.147	2166	2169	2170	rBV	86	51	0.01%	0.001%
66	8.180	2175	2179	2181	rBV2	210	182	0.02%	0.003%
67	8.228	2190	2194	2199	rVB3	440	403	0.05%	0.007%
68	8.308	2208	2219	2247	rBV	237945	400946	52.19%	7.013%
69	8.466	2266	2268	2271	rBV2	184	93	0.01%	0.002%
70	8.556	2293	2296	2303	rVB	236	140	0.02%	0.002%
71	8.594	2306	2308	2311	rBV	166	58	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028816.D
 Acq On : 20 Dec 2018 11:54
 Operator : MD/SY
 Sample : VU1220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

72	8.620	2311	2316	2322	rBV2	675	739	0.10%	0.013%
73	9.086	2449	2461	2496	rBV	317776	532148	69.26%	9.308%
74	9.257	2507	2514	2520	rVB2	652	970	0.13%	0.017%
75	9.340	2538	2540	2542	rBV	179	86	0.01%	0.002%
76	9.382	2545	2553	2554	rBV2	588	691	0.09%	0.012%
77	9.417	2560	2564	2567	rBV	120	106	0.01%	0.002%
78	9.794	2671	2681	2694	rBV6	1174	2424	0.32%	0.042%
79	10.044	2756	2759	2767	rVB	114	100	0.01%	0.002%
80	10.138	2785	2788	2791	rBV	180	150	0.02%	0.003%
81	10.173	2791	2799	2803	rVV	759	983	0.13%	0.017%
82	10.430	2866	2879	2895	rBV	228925	362548	47.19%	6.342%
83	10.646	2943	2946	2950	rBV	270	184	0.02%	0.003%
84	10.665	2950	2952	2954	rVV	146	63	0.01%	0.001%
85	10.954	3040	3042	3044	rBV	169	66	0.01%	0.001%
86	11.417	3179	3186	3195	rBV4	1726	2785	0.36%	0.049%
87	11.482	3195	3206	3235	rVV	289666	456703	59.44%	7.989%
88	11.681	3265	3268	3269	rBV	196	89	0.01%	0.002%
89	11.858	3311	3323	3341	rBV	299279	488264	63.55%	8.541%
90	12.141	3408	3411	3412	rBV2	199	114	0.01%	0.002%
91	12.176	3420	3422	3423	rBV2	148	67	0.01%	0.001%
92	12.212	3431	3433	3436	rBV2	254	144	0.02%	0.003%
93	12.359	3476	3479	3481	rBV2	208	131	0.02%	0.002%
94	12.617	3557	3559	3560	rBV2	248	87	0.01%	0.002%
95	12.710	3585	3588	3590	rBV2	256	195	0.03%	0.003%
96	12.890	3637	3644	3654	rBV4	2270	3332	0.43%	0.058%
97	12.932	3654	3657	3658	rBV	246	115	0.01%	0.002%
98	13.038	3686	3690	3693	rBV	293	295	0.04%	0.005%
99	13.748	3905	3911	3919	rBV	3755	6314	0.82%	0.110%
100	13.996	3981	3988	4003	rVB5	3100	5401	0.70%	0.094%


Sum of corrected areas: 5716865

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
Data File : VU028816.D
Acq On : 20 Dec 2018 11:54
Operator : MD/SY
Sample : VU1220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

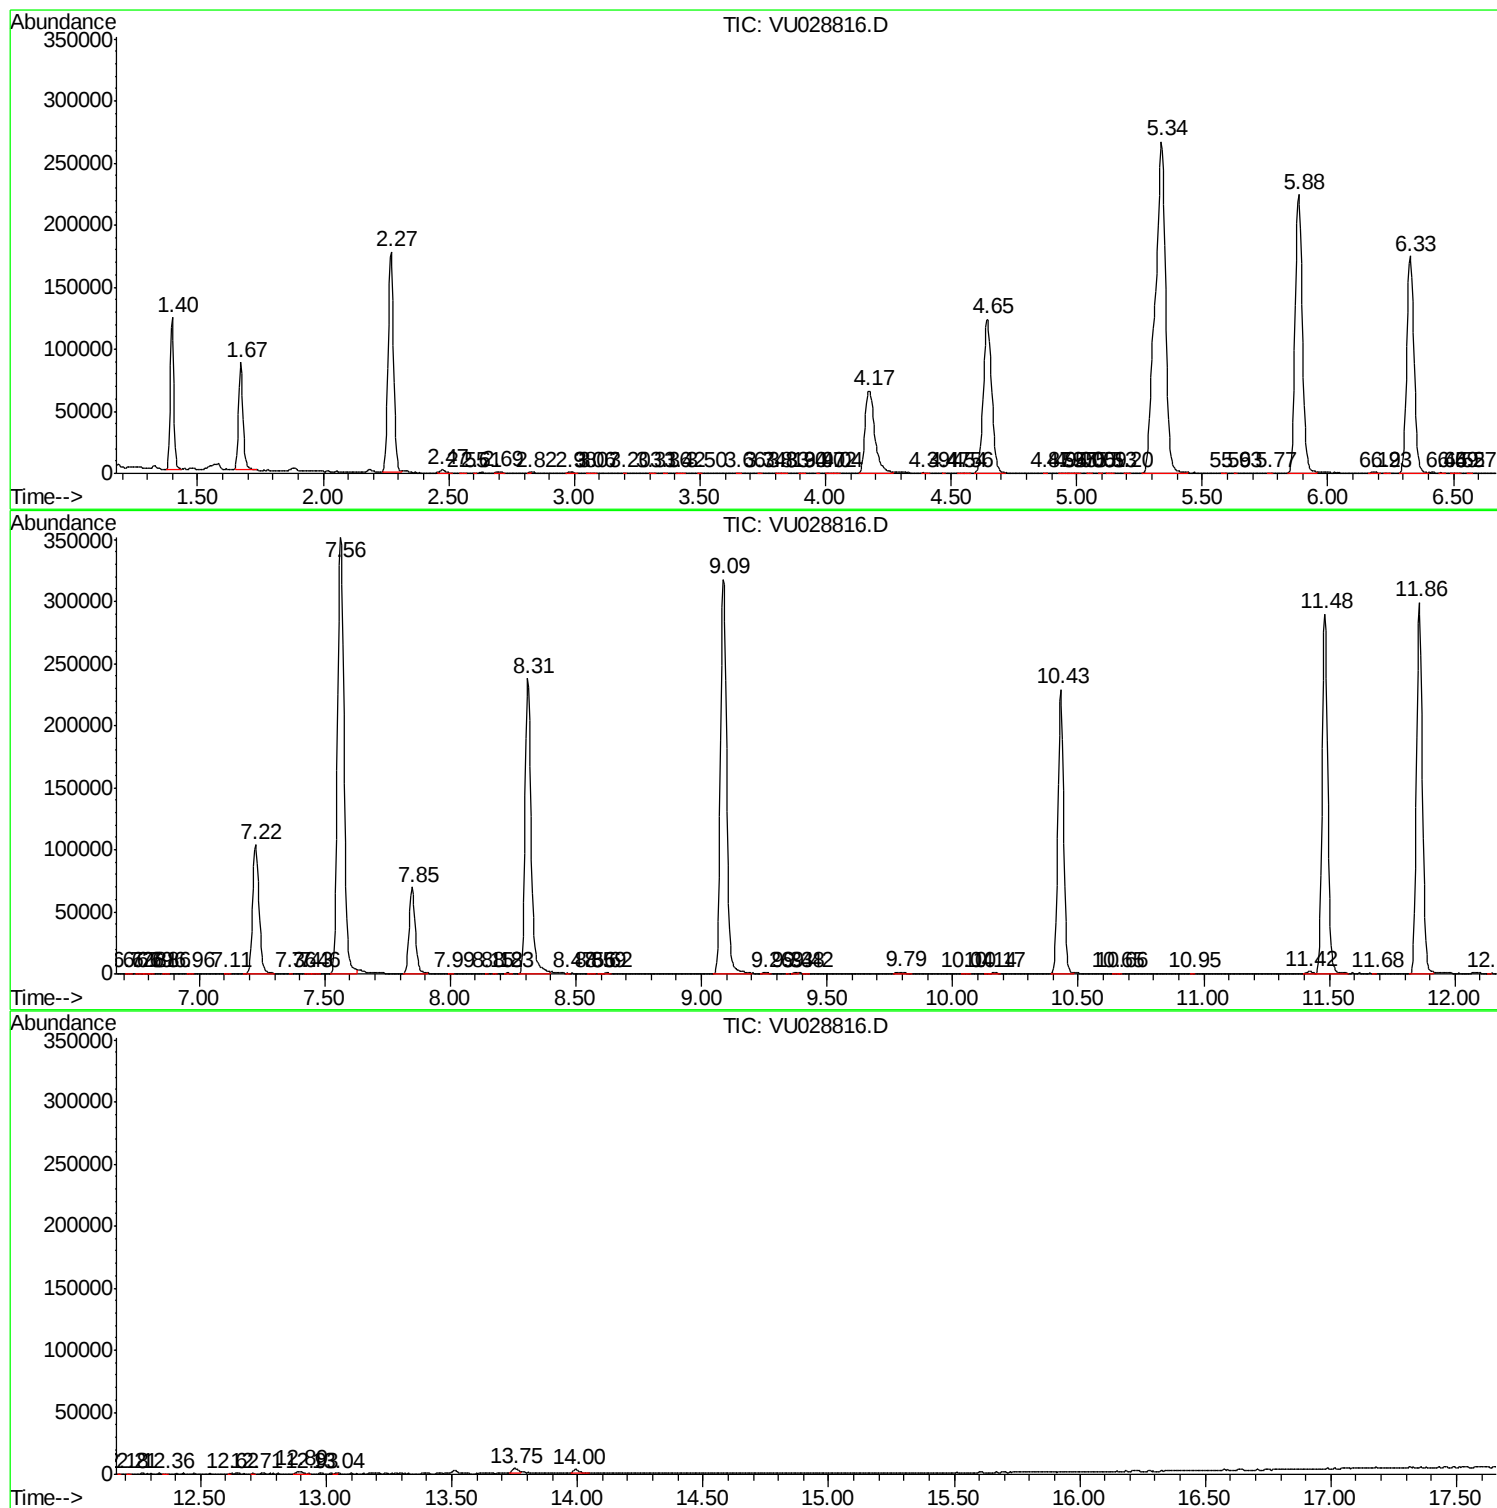

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
Data File : VU028816.D
Acq On : 20 Dec 2018 11:54
Operator : MD/SY
Sample : VU1220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
Data File : VU028816.D
Acq On : 20 Dec 2018 11:54
Operator : MD/SY
Sample : VU1220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc