

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028835.D
 Acq On : 20 Dec 2018 19:31
 Operator : MD/SY
 Sample : VU1220WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	63	70	83	rVB	139912	137794	16.09%	2.159%
2	1.672	148	155	172	rVB	96332	121096	14.14%	1.898%
3	2.270	330	341	355	rBV	196403	298195	34.81%	4.673%
4	2.476	396	405	414	rVB2	1633	2708	0.32%	0.042%
5	2.627	444	452	462	rVB2	512	1015	0.12%	0.016%
6	2.704	469	476	482	rBV3	922	1299	0.15%	0.020%
7	2.832	509	516	518	rBV3	664	795	0.09%	0.012%
8	2.980	557	562	565	rBV3	438	482	0.06%	0.008%
9	3.176	620	623	625	rBV	70	49	0.01%	0.001%
10	3.308	662	664	667	rBV	75	43	0.01%	0.001%
11	3.566	741	744	747	rBV	94	72	0.01%	0.001%
12	3.623	759	762	765	rBV	120	73	0.01%	0.001%
13	3.890	842	845	853	rBV	210	150	0.02%	0.002%
14	3.926	853	856	864	rVB	121	124	0.01%	0.002%
15	4.173	920	933	970	rBV	77519	206286	24.08%	3.233%
16	4.492	1030	1032	1033	rBV	113	44	0.01%	0.001%
17	4.517	1038	1040	1042	rVB	177	62	0.01%	0.001%
18	4.559	1050	1053	1058	rVB2	212	193	0.02%	0.003%
19	4.585	1059	1061	1063	rBV	126	51	0.01%	0.001%
20	4.646	1063	1080	1108	rBV	132670	313096	36.55%	4.907%
21	4.887	1148	1155	1160	rBV3	510	586	0.07%	0.009%
22	4.929	1166	1168	1171	rVB	166	50	0.01%	0.001%
23	4.993	1182	1188	1192	rVB2	521	525	0.06%	0.008%
24	5.029	1196	1199	1201	rBV	104	74	0.01%	0.001%
25	5.099	1215	1221	1223	rBV	200	152	0.02%	0.002%
26	5.202	1249	1253	1254	rBV	54	43	0.01%	0.001%
27	5.337	1272	1295	1323	rBV2	297599	856633	100.00%	13.425%
28	5.556	1361	1363	1367	rVB2	227	172	0.02%	0.003%
29	5.607	1377	1379	1380	rBV2	153	48	0.01%	0.001%
30	5.646	1388	1391	1393	rBV	73	49	0.01%	0.001%
31	5.739	1417	1420	1422	rBV	155	93	0.01%	0.001%
32	5.884	1450	1465	1494	rBV	250211	492230	57.46%	7.714%
33	6.183	1548	1558	1567	rBV7	888	1709	0.20%	0.027%
34	6.237	1572	1575	1578	rVB2	214	161	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028835.D
 Acq On : 20 Dec 2018 19:31
 Operator : MD/SY
 Sample : VU1220WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

35	6.263	1578	1583	1584	rBV2	183	79	0.01%	0.001%
36	6.273	1584	1586	1589	rVB	287	131	0.02%	0.002%
37	6.327	1589	1603	1628	rBV2	193506	385591	45.01%	6.043%
38	6.453	1640	1642	1651	rVB2	304	384	0.04%	0.006%
39	6.495	1652	1655	1659	rBV	284	145	0.02%	0.002%
40	6.581	1678	1682	1686	rVB	104	89	0.01%	0.001%
41	6.604	1686	1689	1692	rBV	126	81	0.01%	0.001%
42	6.649	1698	1703	1706	rBV2	195	185	0.02%	0.003%
43	6.710	1720	1722	1725	rVB	81	40	0.00%	0.001%
44	6.729	1725	1728	1731	rBV	133	109	0.01%	0.002%
45	6.771	1737	1741	1743	rBV	211	108	0.01%	0.002%
46	6.835	1757	1761	1767	rBV	113	134	0.02%	0.002%
47	6.948	1790	1796	1799	rBV	99	106	0.01%	0.002%
48	6.961	1799	1800	1802	rVB	123	46	0.01%	0.001%
49	6.977	1802	1805	1808	rBV	67	51	0.01%	0.001%
50	7.061	1828	1831	1834	rVB2	138	85	0.01%	0.001%
51	7.144	1855	1857	1858	rBV2	141	55	0.01%	0.001%
52	7.225	1871	1882	1903	rBV	111838	197694	23.08%	3.098%
53	7.369	1925	1927	1929	rBV	125	72	0.01%	0.001%
54	7.466	1948	1957	1959	rBV3	627	638	0.07%	0.010%
55	7.562	1972	1987	2019	rBV	389319	693304	80.93%	10.865%
56	7.848	2065	2076	2099	rBV	77160	128253	14.97%	2.010%
57	8.003	2121	2124	2127	rBV2	269	188	0.02%	0.003%
58	8.141	2165	2167	2171	rVV2	197	125	0.01%	0.002%
59	8.157	2171	2172	2175	rBV	213	137	0.02%	0.002%
60	8.228	2188	2194	2202	rVB3	2383	3550	0.41%	0.056%
61	8.308	2206	2219	2252	rBV	270991	469355	54.79%	7.356%
62	8.626	2310	2318	2321	rVB5	802	1069	0.12%	0.017%
63	8.646	2321	2324	2325	rBV	168	115	0.01%	0.002%
64	8.671	2331	2332	2334	rVB	207	41	0.00%	0.001%
65	8.716	2344	2346	2349	rBV	201	104	0.01%	0.002%
66	8.755	2356	2358	2361	rVB	126	72	0.01%	0.001%
67	8.861	2385	2391	2395	rVB2	194	214	0.02%	0.003%
68	8.909	2404	2406	2409	rVB	184	81	0.01%	0.001%
69	9.089	2449	2462	2486	rBV	353591	588225	68.67%	9.219%
70	9.253	2506	2513	2522	rVB2	1337	1815	0.21%	0.028%
71	9.379	2544	2552	2562	rBV2	1662	2582	0.30%	0.040%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028835.D
 Acq On : 20 Dec 2018 19:31
 Operator : MD/SY
 Sample : VU1220WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

72	9.485	2582	2585	2587	rBV	104	58	0.01%	0.001%
73	9.523	2593	2597	2600	rBV	168	155	0.02%	0.002%
74	9.623	2626	2628	2629	rBV	141	38	0.00%	0.001%
75	9.784	2671	2678	2679	rBV	1123	1045	0.12%	0.016%
76	9.880	2706	2708	2712	rVB	214	115	0.01%	0.002%
77	9.970	2734	2736	2739	rVB	210	82	0.01%	0.001%
78	10.331	2846	2848	2850	rVB	214	86	0.01%	0.001%
79	10.430	2866	2879	2894	rBV	257186	411914	48.09%	6.455%
80	10.527	2907	2909	2911	rVB	154	80	0.01%	0.001%
81	10.591	2926	2929	2931	rBV	151	83	0.01%	0.001%
82	10.633	2940	2942	2945	rBV	222	162	0.02%	0.003%
83	10.678	2954	2956	2962	rVB2	347	249	0.03%	0.004%
84	10.700	2962	2963	2964	rBV2	202	65	0.01%	0.001%
85	10.745	2975	2977	2980	rVB	164	72	0.01%	0.001%
86	10.797	2991	2993	2998	rBV	206	136	0.02%	0.002%
87	10.855	3008	3011	3015	rVB	283	149	0.02%	0.002%
88	10.890	3019	3022	3026	rBV	238	171	0.02%	0.003%
89	10.977	3048	3049	3052	rVB	128	51	0.01%	0.001%
90	10.996	3052	3055	3057	rBV	245	144	0.02%	0.002%
91	11.076	3077	3080	3083	rBV	173	127	0.01%	0.002%
92	11.150	3099	3103	3110	rBV3	551	486	0.06%	0.008%
93	11.363	3166	3169	3171	rBV	156	67	0.01%	0.001%
94	11.482	3194	3206	3233	rBV	320031	508739	59.39%	7.973%
95	11.694	3270	3272	3276	rVB	325	111	0.01%	0.002%
96	11.784	3298	3300	3303	rVB	319	130	0.02%	0.002%
97	11.858	3309	3323	3341	rBV	336499	544544	63.57%	8.534%
98	12.144	3410	3412	3413	rBV	306	125	0.01%	0.002%
99	12.382	3483	3486	3491	rBV2	245	301	0.04%	0.005%
100	12.549	3534	3538	3541	rBV	203	191	0.02%	0.003%


Sum of corrected areas: 6380881

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
Data File : VU028835.D
Acq On : 20 Dec 2018 19:31
Operator : MD/SY
Sample : VU1220WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

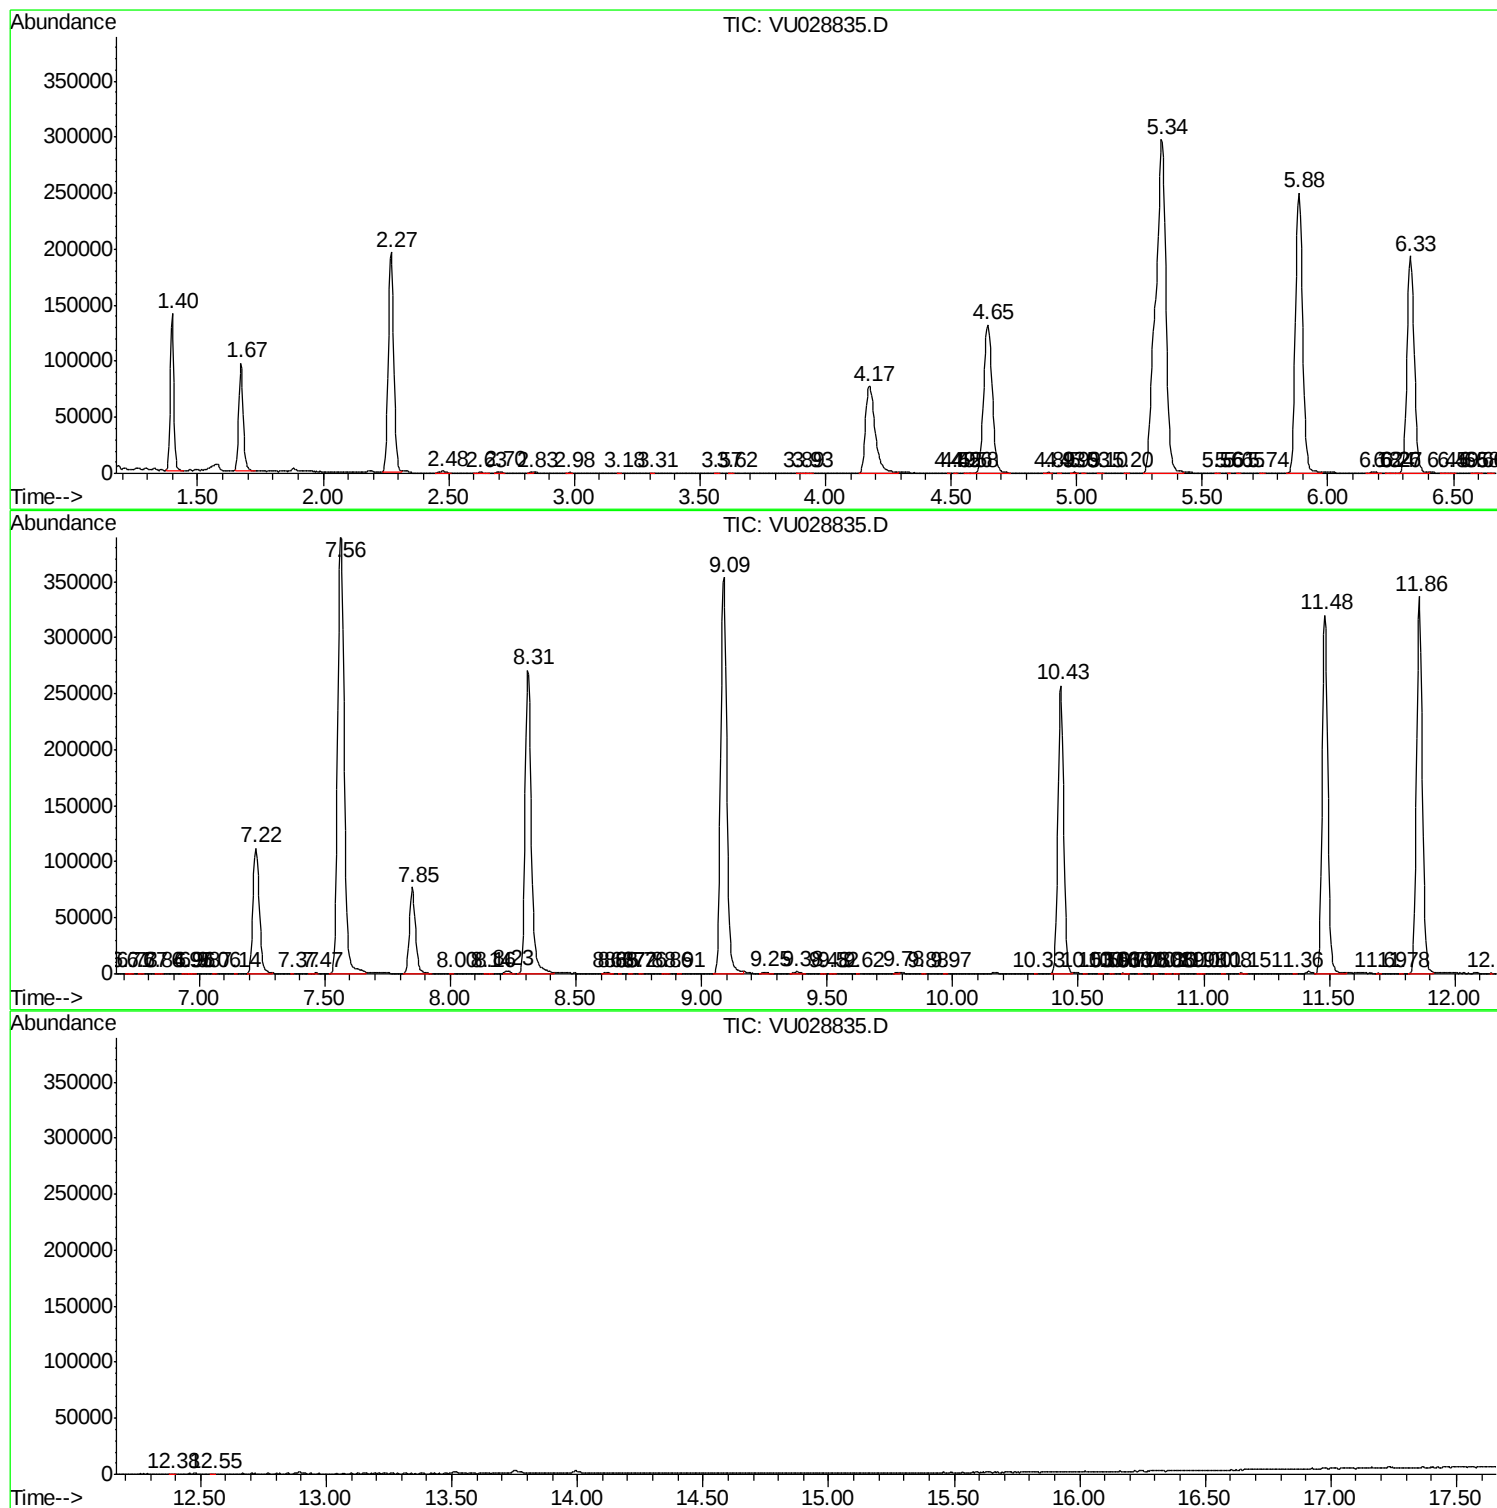

DbaaaPath::ZZ\VOASRVNREBEMM\MSVOA\UNDA\VV1220088\
 DbaaaFile::VV0028855DD
 AcqQ00n ::200Dec2008 199331
 Operator::MDSY
 Sample::VV12200WB002
 Misc::5500mLMSVOA\UNDA\WATER
 ASSVial::227 SampleMultiplier:11

Instrument :
 MSVOA_U
 ClientSampleID :
 VBLK60

QcandMebdd::ZZ\VOASRVNREBEMM\MSVOA\UNDA\WATER
 QcandTitle::VOCAAnalysis

TICLibrary::CC\DATA\BASIS\NIST11LL
 TICIntegrationsParameters:LS6CMTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
