


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122018\
 Data File : VU028809.D
 Acq On : 20 Dec 2018 08:25
 Operator : MD/SY
 Sample : BFB62
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 21 18:12:49 2018

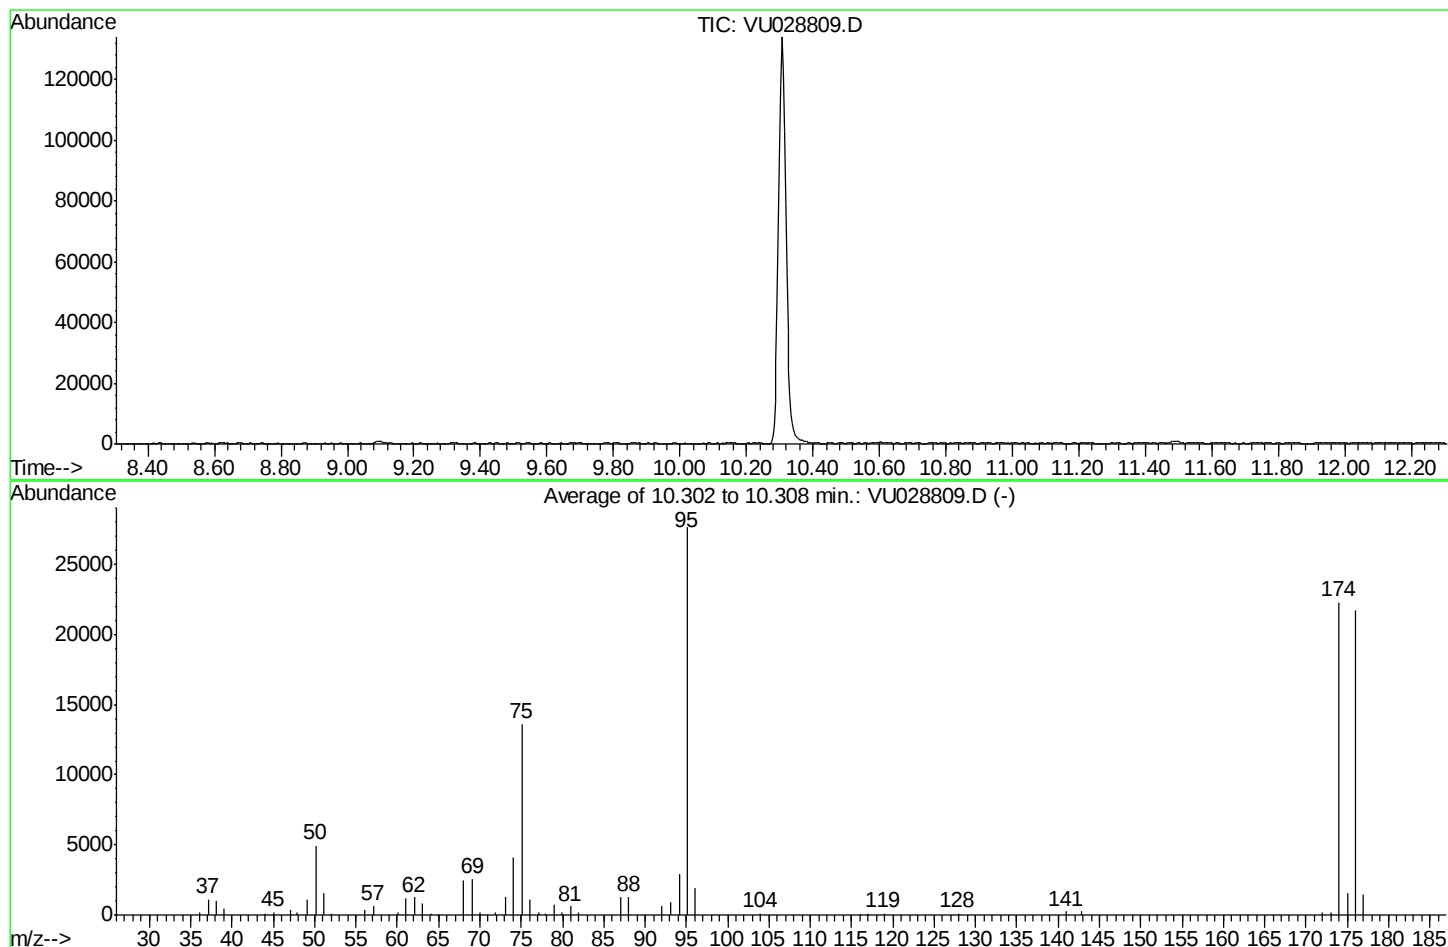

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	4930	PASS
75	95	30	80	49.3	13616	PASS
95	95	100	100	100.0	27640	PASS
96	95	5	9	6.8	1892	PASS
173	174	0.00	2	0.7	154	PASS
174	95	50	120	80.7	22312	PASS
175	174	5	9	7.0	1569	PASS
176	174	95	101	97.2	21688	PASS
177	176	5	9	6.7	1448	PASS

m/z	Abundance
36.00	161.0
37.10	1006.0
38.10	923.0
39.10	411.0
44.00	310.0
45.00	206.0
47.00	312.0
47.80	141.0
49.10	988.0
50.10	4722.0
51.10	1539.0
52.00	100.0
56.00	316.0
57.10	564.0
60.00	210.0
61.00	1025.0
62.10	1133.0
63.00	748.0
64.00	109.0
68.00	2343.0
69.10	2474.0
70.10	204.0
71.90	125.0
73.10	1128.0
74.10	3883.0
75.10	12669.0
76.10	1012.0
77.10	185.0
77.90	111.0
79.00	642.0
80.00	165.0
80.90	573.0
82.00	118.0
87.00	1194.0
88.00	1271.0
92.00	526.0
93.10	943.0
94.10	2629.0
95.10	25968.0
96.10	1779.0
104.00	110.0
116.90	111.0
118.90	125.0
127.90	136.0
141.00	223.0
142.90	207.0
171.90	141.0
174.00	20096.0
175.00	1445.0
176.00	19808.0
177.00	1264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62

m/z	Abundance
36.00	169.0
37.10	1159.0
38.10	1000.0
39.00	424.0
44.00	304.0
45.00	207.0
47.00	387.0
47.80	153.0
49.10	1113.0
50.10	5108.0
51.10	1553.0
52.00	106.0
56.10	341.0
57.10	659.0
60.00	216.0
61.00	1196.0
62.10	1283.0
63.10	842.0
64.10	153.0
68.10	2503.0
69.10	2639.0
70.00	221.0
71.90	154.0
73.10	1306.0
74.10	4185.0
75.10	14125.0
76.10	1151.0
77.10	207.0
78.00	135.0
79.00	732.0
80.00	182.0
81.00	603.0
82.00	159.0
87.00	1277.0
88.00	1348.0
92.00	623.0
93.10	950.0
94.10	2958.0
95.10	28664.0
96.10	1942.0
103.90	119.0
116.90	125.0
118.90	141.0
127.90	145.0
141.00	260.0
142.90	232.0
171.90	175.0
173.10	238.0
174.00	22984.0
175.00	1594.0
176.00	22344.0
177.00	1484.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62

m/z	Abundance
36.00	181.0
37.10	1184.0
38.10	997.0
39.10	456.0
44.10	336.0
45.00	184.0
47.10	394.0
47.90	161.0
49.10	1144.0
50.10	4961.0
51.10	1515.0
56.10	361.0
57.10	699.0
60.10	213.0
61.00	1260.0
62.10	1309.0
63.10	933.0
64.10	155.0
64.90	124.0
68.10	2504.0
69.10	2664.0
70.00	211.0
71.90	150.0
73.10	1282.0
74.10	4229.0
75.10	14054.0
76.10	1244.0
77.10	223.0
78.00	157.0
79.00	718.0
79.90	182.0
81.00	621.0
82.00	160.0
87.00	1240.0
88.00	1299.0
92.00	695.0
93.00	965.0
94.10	3057.0
95.10	28288.0
96.10	1956.0
104.00	100.0
116.00	111.0
117.00	131.0
118.90	143.0
127.90	131.0
141.00	257.0
142.90	258.0
172.00	206.0
173.10	225.0
174.00	23856.0
175.00	1669.0
176.00	22912.0
177.00	1597.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62

m/z	Abundance
44.00	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62