


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122019\
 Data File : VU036305.D
 Acq On : 20 Dec 2019 08:58
 Operator : JC/MD
 Sample : BFB23
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB23

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 20 22:20:21 2019

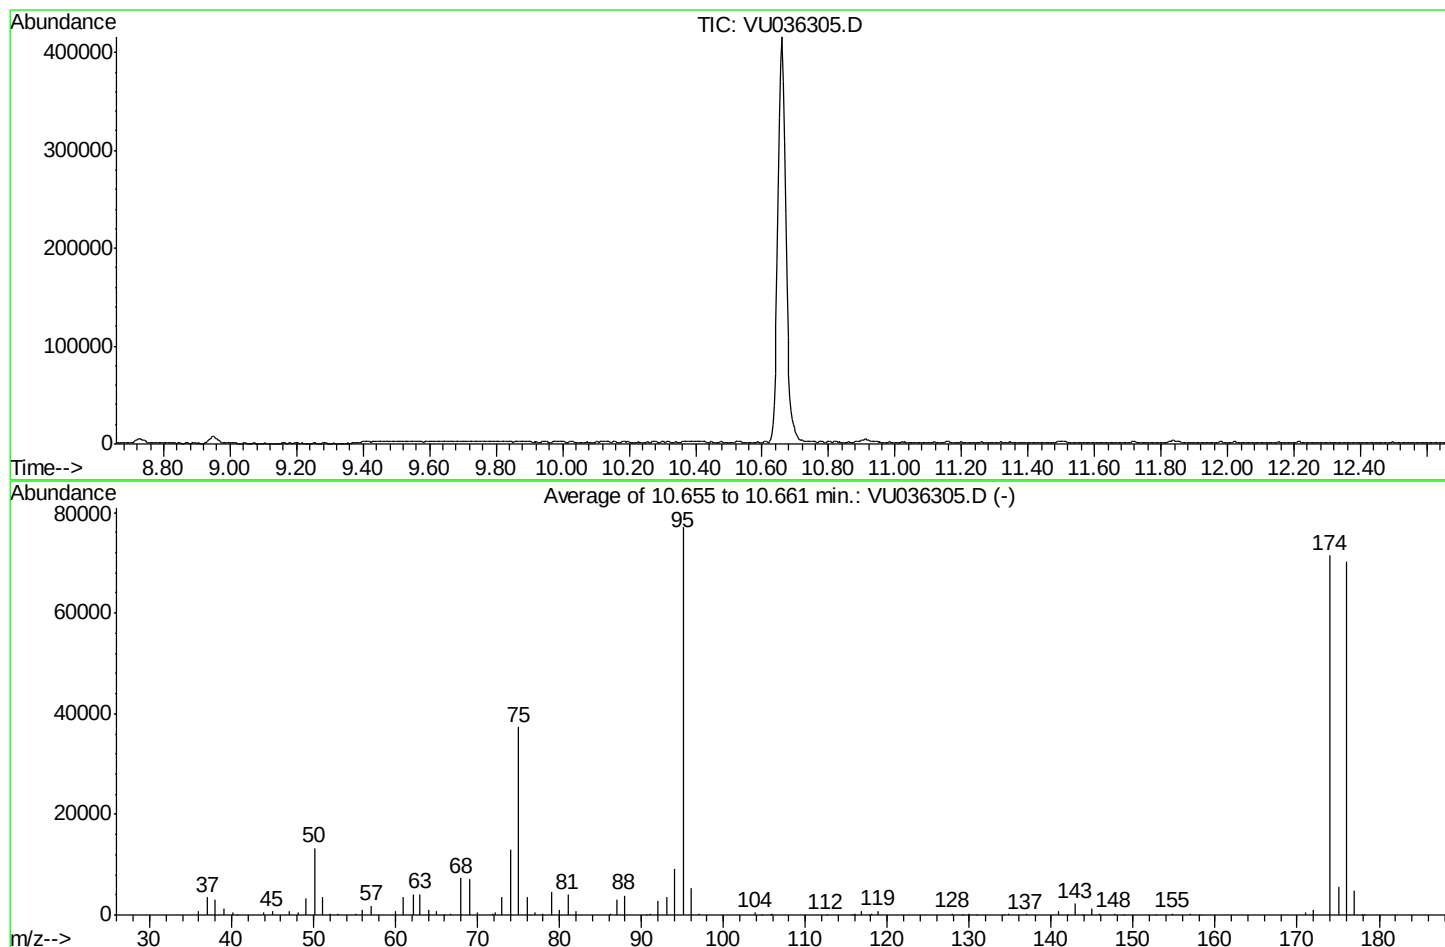

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	13319	PASS
75	95	30	80	48.4	37306	PASS
95	95	100	100	100.0	77042	PASS
96	95	5	9	6.8	5275	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.7	71386	PASS
175	174	5	9	7.9	5622	PASS
176	174	95	101	98.3	70152	PASS
177	176	5	9	6.7	4721	PASS

m/z	Abundance
36.00	1537.0
37.10	3208.0
38.00	3046.0
39.00	1165.0
40.10	425.0
40.70	112.0
44.00	891.0
45.00	685.0
47.00	839.0
48.10	427.0
49.00	3483.0
50.10	12921.0
51.10	3473.0
52.10	115.0
52.90	125.0
55.10	222.0
55.90	884.0
57.10	1654.0
60.00	714.0
61.00	3712.0
62.10	3977.0
63.00	4034.0
64.00	1017.0
65.00	774.0
66.00	154.0
66.70	168.0
68.00	7272.0
69.10	6942.0
70.00	490.0
72.10	508.0
73.00	3523.0
74.00	12700.0
75.10	37024.0
76.10	3440.0
77.00	565.0
78.00	391.0
79.00	4479.0
80.00	1250.0
81.00	3838.0
82.00	896.0
86.20	173.0
87.00	2816.0
87.90	3594.0
91.00	326.0
92.00	2442.0
93.10	3547.0
94.00	9124.0
95.10	73744.0
96.10	5136.0
97.00	131.0
103.90	380.0
105.70	271.0
106.00	300.0
115.70	245.0
116.90	843.0
118.10	460.0
118.90	864.0
127.90	306.0
130.00	211.0
134.10	110.0
134.90	105.0
137.00	171.0
140.90	857.0
143.00	2164.0
144.90	1398.0
145.90	194.0
147.70	276.0
152.80	119.0
154.80	296.0
156.90	171.0
171.00	477.0
172.00	860.0
174.00	67464.0
175.00	5292.0
176.00	66520.0
177.00	4660.0
177.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	1478.0
37.10	3654.0
38.00	3384.0
39.10	1343.0
40.10	419.0
43.90	1024.0
45.00	659.0
47.00	907.0
48.10	472.0
49.00	3437.0
50.10	13673.0
51.10	3609.0
52.10	188.0
52.90	147.0
55.10	294.0
56.00	1027.0
57.00	1813.0
60.00	786.0
61.00	3818.0
62.10	4178.0
63.00	4177.0
64.00	1162.0
65.00	868.0
66.00	144.0
66.80	196.0
68.00	7524.0
69.10	7088.0
70.00	452.0
72.10	384.0
73.00	3701.0
74.10	13434.0
75.00	38240.0
76.10	3757.0
76.90	527.0
78.00	357.0
79.00	4842.0
80.00	1129.0
81.00	4000.0
82.00	911.0
86.10	177.0
87.00	3019.0
87.90	4076.0
91.00	314.0
92.00	2745.0
93.00	3591.0
94.00	9399.0
95.10	79264.0
96.10	5384.0
97.00	183.0
103.90	498.0
104.60	118.0
106.00	419.0
116.00	281.0
116.90	878.0
118.10	391.0
118.90	935.0
127.90	298.0
129.10	108.0
130.00	224.0
130.90	119.0
134.80	165.0
136.90	185.0
140.90	937.0
141.90	108.0
143.00	2290.0
143.90	117.0
144.90	1412.0
145.90	190.0
147.70	266.0
148.90	123.0
152.80	142.0
154.80	319.0
156.90	214.0
171.00	581.0
172.00	933.0
174.00	73192.0
175.00	5928.0
176.00	72304.0
177.00	4908.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	1360.0
37.10	3535.0
38.00	3480.0
39.10	1447.0
40.20	345.0
43.90	1054.0
45.00	627.0
46.90	813.0
48.10	493.0
49.00	3029.0
50.10	13364.0
51.10	3744.0
52.10	197.0
52.90	148.0
55.10	273.0
56.00	1112.0
57.00	1962.0
60.00	851.0
61.00	3503.0
62.10	4039.0
63.00	4191.0
64.00	1198.0
65.00	778.0
66.00	107.0
66.80	200.0
68.00	7123.0
69.10	7143.0
70.00	414.0
71.80	472.0
72.20	383.0
73.00	3695.0
74.10	12939.0
75.00	36656.0
76.10	3777.0
76.90	489.0
78.00	260.0
79.00	4503.0
80.00	1036.0
81.00	4213.0
82.00	837.0
86.10	212.0
87.00	3002.0
87.90	3810.0
90.60	176.0
91.10	281.0
92.00	2894.0
93.00	3566.0
94.00	8712.0
95.10	78120.0
96.10	5306.0
97.10	191.0
103.90	519.0
104.60	120.0
105.90	444.0
112.60	105.0
116.00	356.0
116.90	805.0
117.80	284.0
118.90	829.0
128.00	295.0
129.10	151.0
130.00	244.0
134.80	215.0
136.80	214.0
140.90	859.0
141.90	163.0
142.90	2202.0
143.90	113.0
144.90	1286.0
146.00	155.0
147.80	253.0
148.90	126.0
152.70	114.0
154.80	252.0
156.90	213.0
158.10	105.0
170.90	768.0
172.00	934.0
174.00	73504.0
175.00	5647.0
176.00	71632.0
177.00	4596.0
178.20	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Scan 2884 (10.613 min): VU036305.D
BFB23

m/z	Abundance
35.10	240.0
35.90	722.0
37.90	361.0
39.90	306.0
44.00	559.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23