
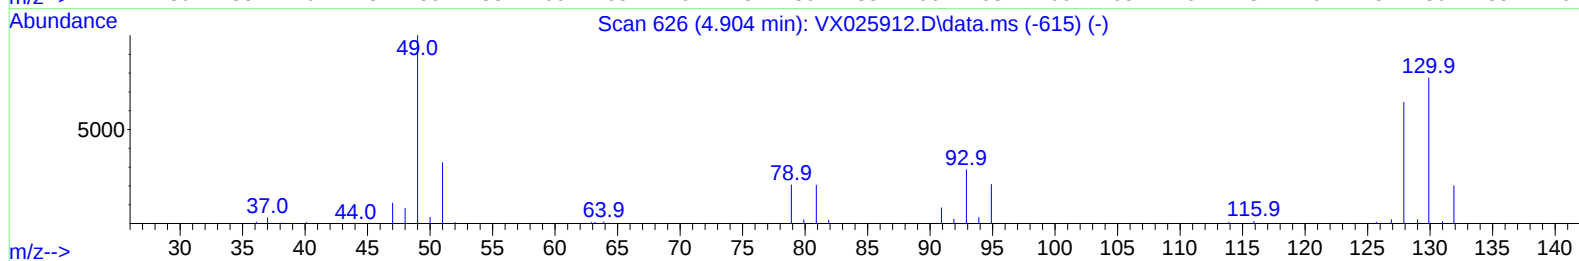
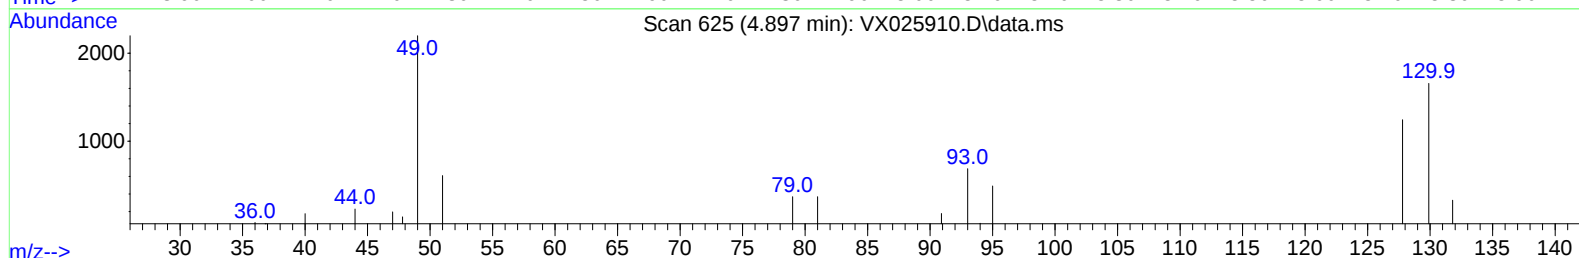


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025910.D
Acq On : 20 Dec 2021 12:35
Operator : JC/MD
Sample : VSTD00543
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 20 14:12:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 20 14:11:27 2021
Response via : Initial Calibration

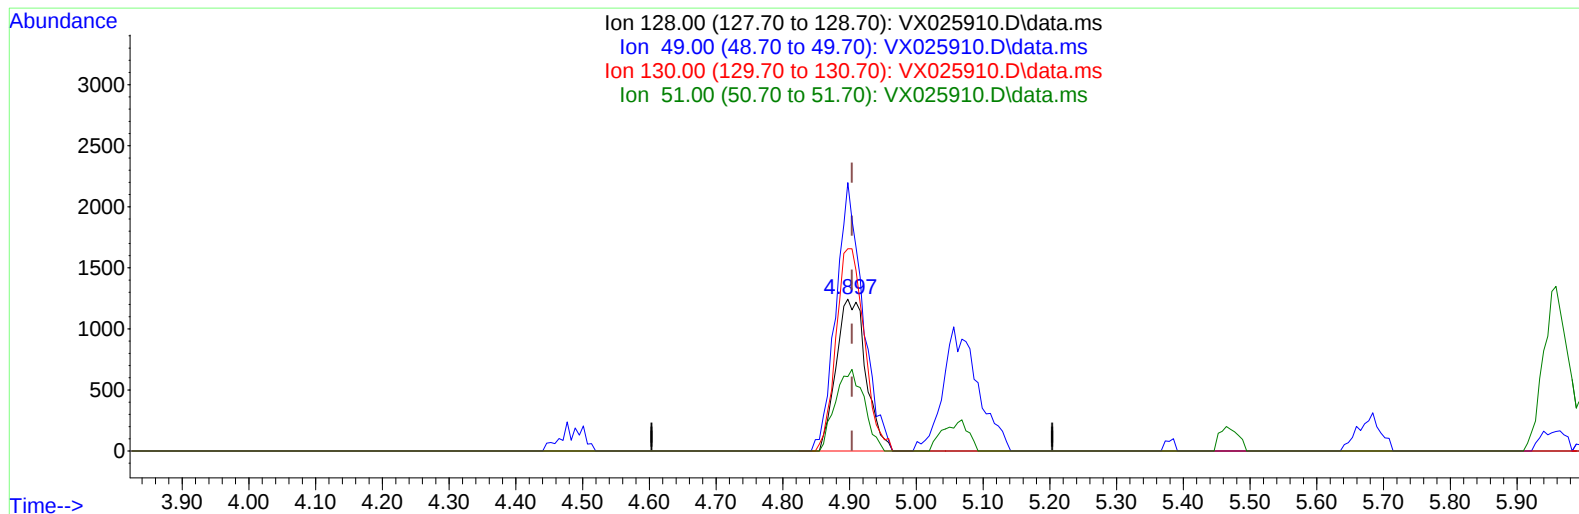

TIC: VX025910.D\data.ms

(23) Bromochloromethane (T)

4.897min (-0.006) 5.90 ug/L m

response 3855

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	139.60	176.69
130.00	126.00	133.20
51.00	45.00	48.95