
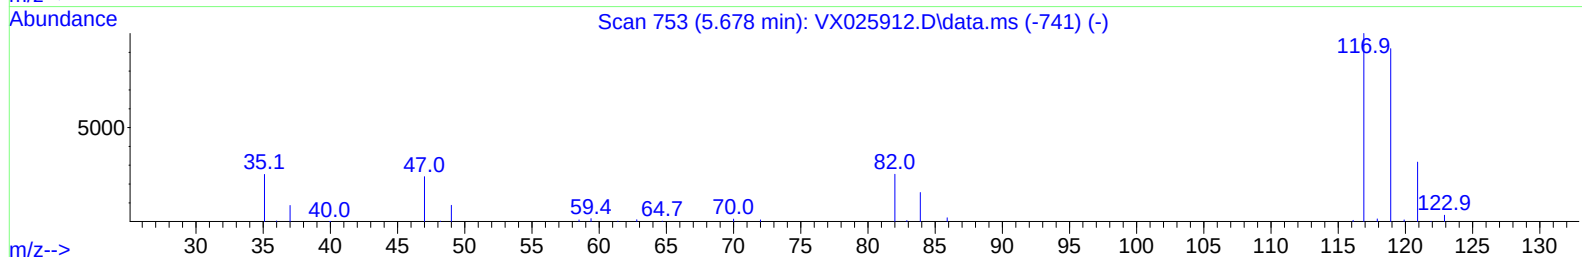
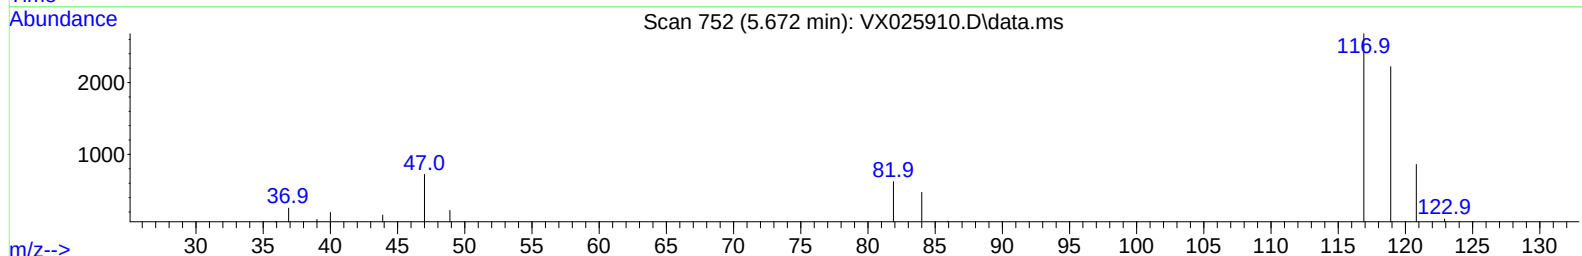


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025910.D
Acq On : 20 Dec 2021 12:35
Operator : JC/MD
Sample : VSTD00543
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 20 14:12:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 20 14:11:27 2021
Response via : Initial Calibration

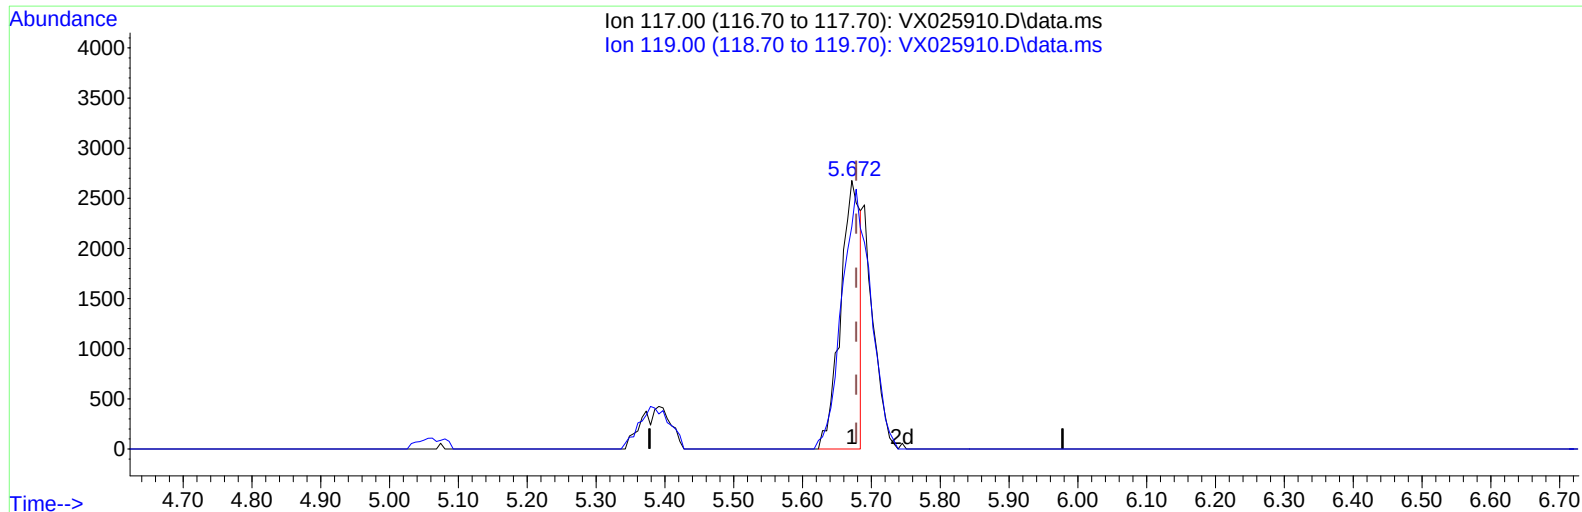

TIC: VX025910.D\data.ms

(31) Carbon tetrachloride (T)

5.672min (-0.006) 3.58 ug/L

response 5334

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	96.00	142.29#
0.00	0.00	0.00
0.00	0.00	0.00