
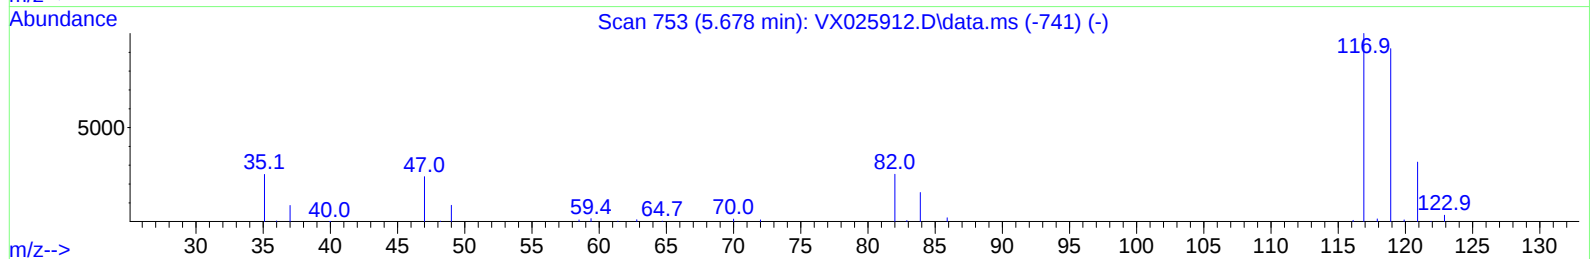
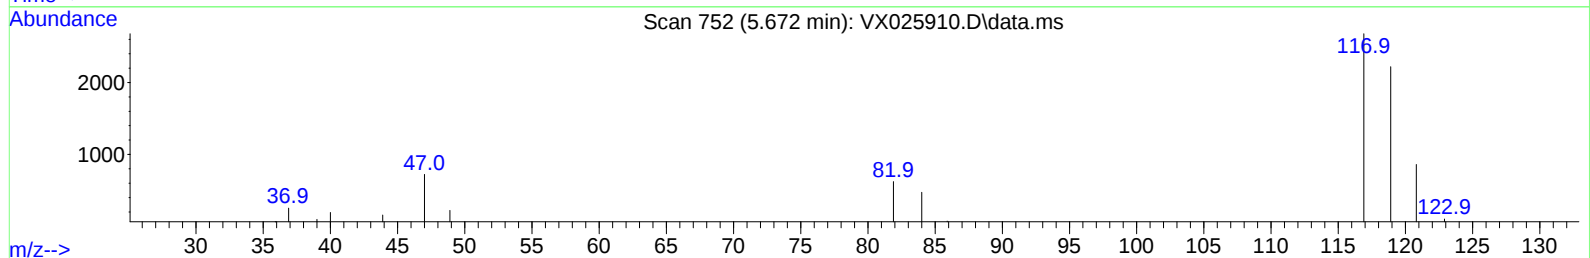


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025910.D
 Acq On : 20 Dec 2021 12:35
 Operator : JC/MD
 Sample : VSTD00543
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 20 14:12:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Dec 20 14:11:27 2021
 Response via : Initial Calibration

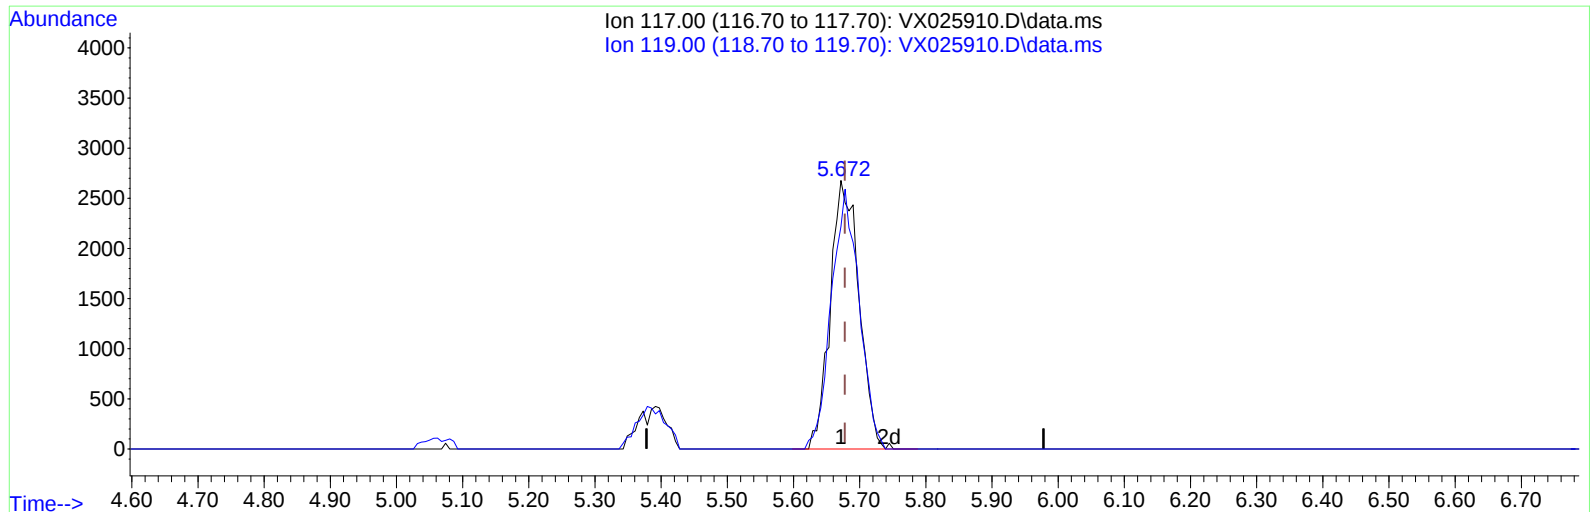

TIC: VX025910.D\data.ms

(31) Carbon tetrachloride (T)

5.672min (-0.006) 5.41 ug/L m

response 8061

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	96.00	94.16
0.00	0.00	0.00
0.00	0.00	0.00