

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046506.D
 Acq On : 20 Dec 2021 12:22
 Operator : SY/MD
 Sample : VU1220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rBV	69534	85198	16.23%	2.052%
2	1.922	172	181	205	rBV	48641	70852	13.49%	1.706%
3	2.086	227	232	233	rBV	267	215	0.04%	0.005%
4	2.211	268	271	273	rBV2	242	154	0.03%	0.004%
5	2.465	347	350	353	rBV2	198	118	0.02%	0.003%
6	2.575	372	384	403	rBV	118057	196627	37.45%	4.736%
7	2.707	423	425	428	rVB2	212	121	0.02%	0.003%
8	2.803	446	455	461	rBB2	513	853	0.16%	0.021%
9	2.851	467	470	473	rBB	142	121	0.02%	0.003%
10	2.945	495	499	501	rBV	138	141	0.03%	0.003%
11	3.054	525	533	540	rBB3	806	1480	0.28%	0.036%
12	3.089	541	544	547	rBB	130	111	0.02%	0.003%
13	3.183	567	573	574	rBV	810	805	0.15%	0.019%
14	4.652	1014	1030	1068	rBV2	33800	125812	23.96%	3.030%
15	4.864	1094	1096	1099	rVV	183	110	0.02%	0.003%
16	5.070	1144	1160	1185	rBV	93740	207249	39.47%	4.992%
17	5.729	1344	1365	1390	rBV2	193930	525041	100.00%	12.646%
18	6.253	1513	1528	1549	rBV	174065	325408	61.98%	7.837%
19	6.366	1561	1563	1566	rVV	220	130	0.02%	0.003%
20	6.382	1566	1568	1570	rVB	234	112	0.02%	0.003%
21	6.623	1641	1643	1648	rBB	157	150	0.03%	0.004%
22	6.694	1651	1665	1688	rBB	117294	228674	43.55%	5.508%
23	6.803	1697	1699	1702	rBB	231	114	0.02%	0.003%
24	7.041	1770	1773	1774	rBV	221	117	0.02%	0.003%
25	7.051	1774	1776	1778	rVB	232	114	0.02%	0.003%
26	7.186	1815	1818	1820	rBV2	219	126	0.02%	0.003%
27	7.568	1925	1937	1953	rBV	66593	114241	21.76%	2.751%
28	7.626	1953	1955	1958	rVB	288	144	0.03%	0.003%
29	7.800	2003	2009	2015	rBB2	330	441	0.08%	0.011%
30	7.899	2027	2040	2055	rBV	240616	413443	78.74%	9.958%
31	7.970	2057	2062	2074	rVV	3402	5723	1.09%	0.138%
32	8.018	2075	2077	2081	rVB	215	149	0.03%	0.004%
33	8.182	2115	2128	2148	rBB	45692	77450	14.75%	1.865%
34	8.468	2215	2217	2220	rBV2	277	214	0.04%	0.005%
35	8.501	2224	2227	2229	rVB2	300	187	0.04%	0.005%
36	8.517	2230	2232	2233	rBV2	292	146	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046506.D
 Acq On : 20 Dec 2021 12:22
 Operator : SY/MD
 Sample : VU1220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.578	2249	2251	2257	rVB2	321	267	0.05%	0.006%
38	8.636	2258	2269	2300	rBV	150061	265951	50.65%	6.405%
39	8.761	2306	2308	2313	rVB	256	194	0.04%	0.005%
40	8.787	2313	2316	2318	rBV	208	138	0.03%	0.003%
41	8.838	2329	2332	2336	rBB	136	138	0.03%	0.003%
42	9.176	2435	2437	2441	rBB	138	123	0.02%	0.003%
43	9.208	2442	2447	2449	rBV	127	135	0.03%	0.003%
44	9.417	2497	2512	2534	rBV	253526	420457	80.08%	10.127%
45	9.520	2541	2544	2546	rVB2	255	167	0.03%	0.004%
46	9.565	2554	2558	2564	rBV2	279	340	0.06%	0.008%
47	9.694	2591	2598	2604	rBV2	470	669	0.13%	0.016%
48	9.774	2619	2623	2625	rBB	132	115	0.02%	0.003%
49	9.825	2636	2639	2642	rBB	137	120	0.02%	0.003%
50	9.848	2643	2646	2650	rBB	166	152	0.03%	0.004%
51	9.883	2654	2657	2661	rBV	152	177	0.03%	0.004%
52	9.996	2688	2692	2694	rBV	169	160	0.03%	0.004%
53	10.102	2721	2725	2728	rBB	279	263	0.05%	0.006%
54	10.131	2729	2734	2736	rBB	150	125	0.02%	0.003%
55	10.198	2753	2755	2760	rVB	168	135	0.03%	0.003%
56	10.349	2798	2802	2804	rBB	129	112	0.02%	0.003%
57	10.375	2807	2810	2813	rBV	163	163	0.03%	0.004%
58	10.475	2837	2841	2842	rBV	143	119	0.02%	0.003%
59	10.488	2842	2845	2849	rVB2	307	295	0.06%	0.007%
60	10.546	2861	2863	2866	rBV	147	120	0.02%	0.003%
61	10.671	2894	2902	2909	rBB4	1365	1780	0.34%	0.043%
62	10.706	2910	2913	2917	rBV	124	154	0.03%	0.004%
63	10.758	2917	2929	2943	rBV	173142	271805	51.77%	6.546%
64	10.841	2951	2955	2957	rBV	166	135	0.03%	0.003%
65	10.857	2958	2960	2964	rVV	265	209	0.04%	0.005%
66	10.877	2964	2966	2969	rVV	295	226	0.04%	0.005%
67	10.893	2970	2971	2974	rVV	319	159	0.03%	0.004%
68	11.005	3003	3006	3010	rBB	183	174	0.03%	0.004%
69	11.044	3014	3018	3020	rBV	143	124	0.02%	0.003%
70	11.089	3029	3032	3036	rVB2	189	170	0.03%	0.004%
71	11.128	3041	3044	3047	rVB	153	127	0.02%	0.003%
72	11.163	3052	3055	3059	rBB	161	161	0.03%	0.004%
73	11.201	3062	3067	3072	rBB	205	268	0.05%	0.006%
74	11.227	3073	3075	3079	rBV	154	163	0.03%	0.004%
75	11.292	3091	3095	3098	rBV	208	223	0.04%	0.005%
76	11.462	3139	3148	3155	rVB4	673	1205	0.23%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046506.D
 Acq On : 20 Dec 2021 12:22
 Operator : SY/MD
 Sample : VU1220WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.552	3173	3176	3179	rBV	159	158	0.03%	0.004%
78	11.603	3188	3192	3193	rBV	161	138	0.03%	0.003%
79	11.693	3215	3220	3223	rBV3	468	461	0.09%	0.011%
80	11.748	3228	3237	3241	rBV3	442	663	0.13%	0.016%
81	11.812	3245	3257	3274	rBV	266039	417558	79.53%	10.057%
82	11.967	3302	3305	3306	rBV	568	288	0.05%	0.007%
83	12.195	3363	3376	3397	rVV	233913	377406	71.88%	9.090%
84	12.568	3489	3492	3496	rVB	192	181	0.03%	0.004%
85	12.590	3496	3499	3507	rBV	196	325	0.06%	0.008%
86	12.639	3510	3514	3516	rBV	244	198	0.04%	0.005%
87	13.221	3688	3695	3701	rBV2	790	1044	0.20%	0.025%
88	13.844	3881	3889	3894	rBV2	711	936	0.18%	0.023%
89	14.095	3959	3967	3974	rVB	623	1039	0.20%	0.025%
90	15.047	4259	4263	4265	rBV	176	132	0.03%	0.003%
91	15.246	4321	4325	4333	rBV2	247	303	0.06%	0.007%
92	15.629	4442	4444	4449	rBV	197	115	0.02%	0.003%
93	15.658	4449	4453	4456	rBV2	257	166	0.03%	0.004%
94	15.693	4461	4464	4466	rBV	181	149	0.03%	0.004%
95	15.803	4496	4498	4503	rVB2	223	120	0.02%	0.003%
96	15.954	4542	4545	4547	rBV	205	152	0.03%	0.004%
97	16.230	4628	4631	4632	rBV	215	124	0.02%	0.003%
98	16.262	4639	4641	4646	rVB	290	161	0.03%	0.004%
99	16.507	4715	4717	4721	rBV2	232	168	0.03%	0.004%
100	16.661	4762	4765	4768	rBV	273	200	0.04%	0.005%




Sum of corrected areas: 4151994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046506.D
Acq On : 20 Dec 2021 12:22
Operator : SY/MD
Sample : VU1220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

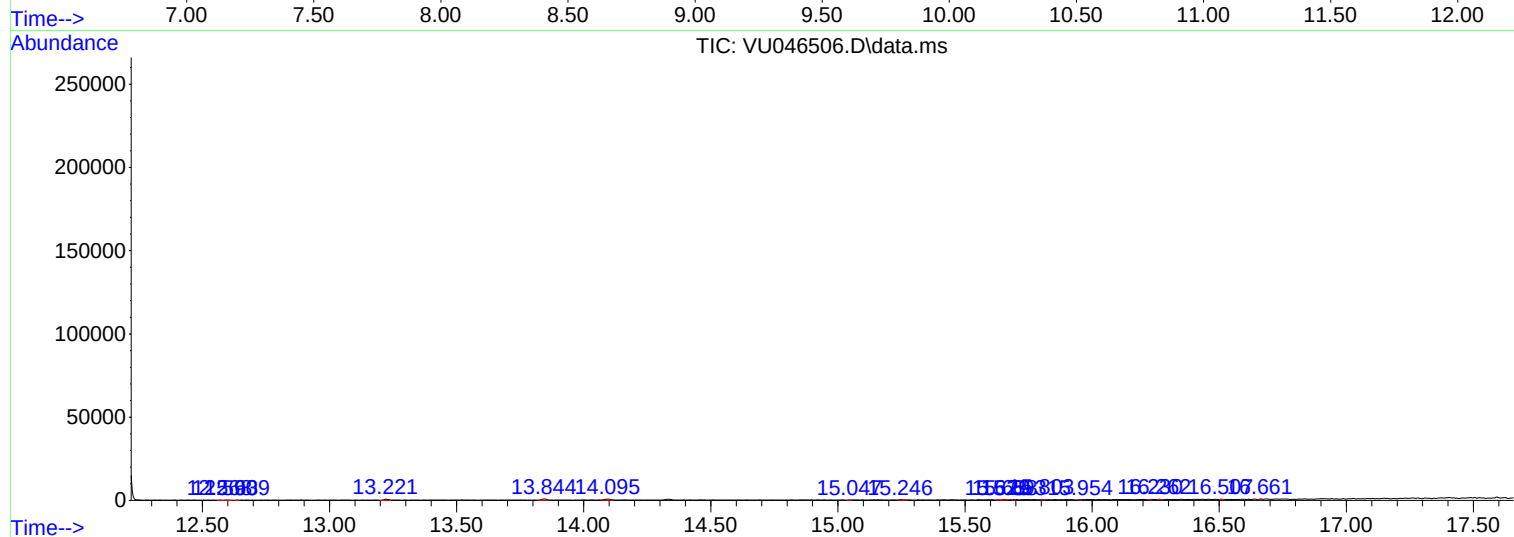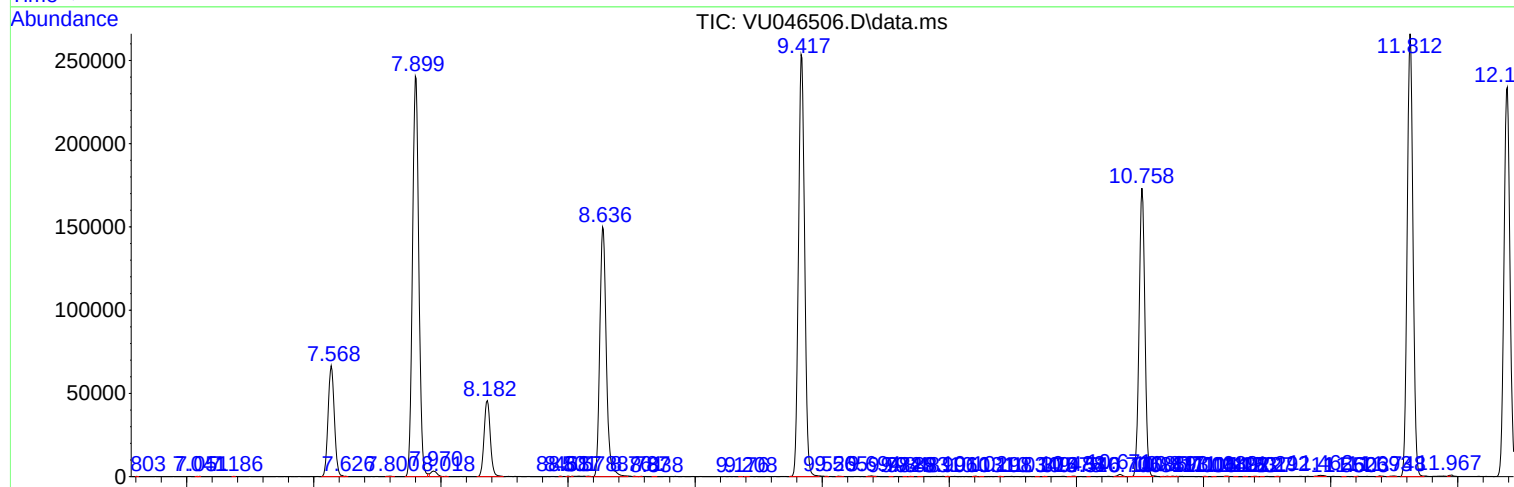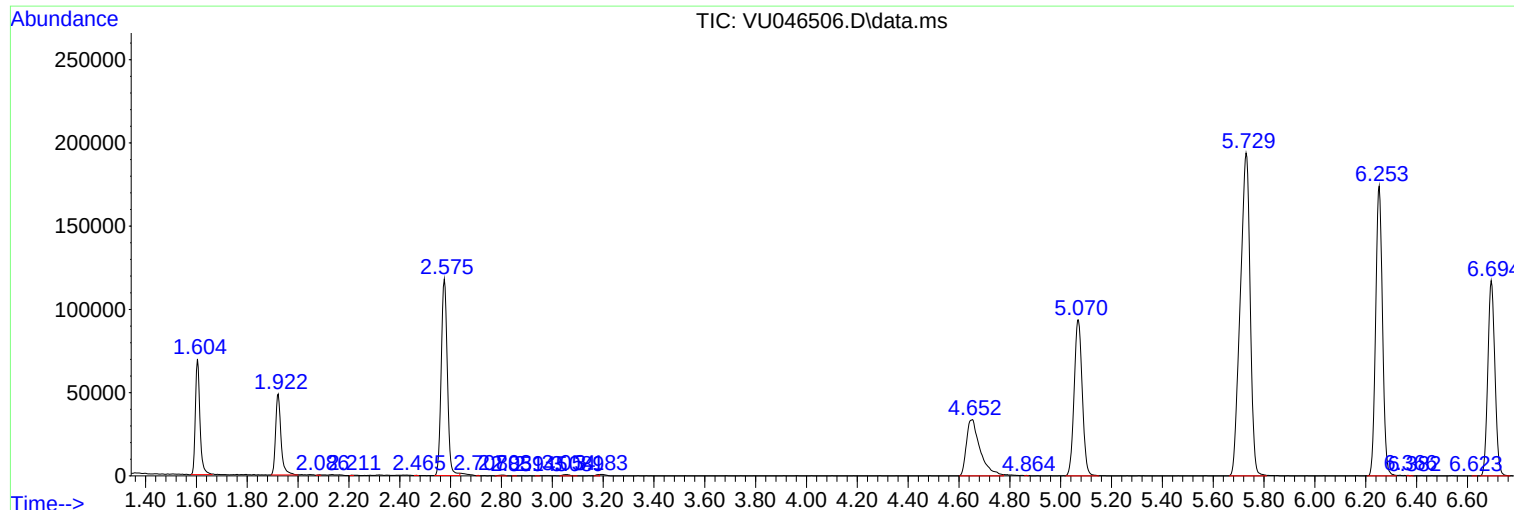

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046506.D
Acq On : 20 Dec 2021 12:22
Operator : SY/MD
Sample : VU1220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046506.D
Acq On : 20 Dec 2021 12:22
Operator : SY/MD
Sample : VU1220WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc