

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046509.D
 Acq On : 20 Dec 2021 14:56
 Operator : SY/MD
 Sample : M5150-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	4	7	11	rBV2	637	445	0.00%	0.002%
2	1.475	37	42	47	rBV2	1871	1953	0.02%	0.007%
3	1.607	73	83	102	rBV2	247741	321617	2.75%	1.230%
4	1.871	162	165	169	rBV2	380	223	0.00%	0.001%
5	1.922	172	181	203	rVV	56803	82385	0.70%	0.315%
6	2.144	247	250	251	rBV	369	218	0.00%	0.001%
7	2.385	320	325	330	rVB2	285	307	0.00%	0.001%
8	2.578	371	385	400	rBV3	164541	308572	2.64%	1.180%
9	2.806	449	456	460	rVB3	561	719	0.01%	0.003%
10	2.964	502	505	513	rVB2	257	354	0.00%	0.001%
11	3.057	530	534	539	rBB2	274	300	0.00%	0.001%
12	3.189	565	575	587	rBB3	1060	2491	0.02%	0.010%
13	3.363	615	629	647	rBV	63711	126420	1.08%	0.483%
14	3.443	651	654	657	rVB2	255	185	0.00%	0.001%
15	3.871	782	787	791	rBV	216	305	0.00%	0.001%
16	4.674	1014	1037	1117	rBV	4024912	9199945	78.59%	35.185%
17	5.070	1145	1160	1185	rVB	112046	244174	2.09%	0.934%
18	5.276	1222	1224	1227	rVB	245	156	0.00%	0.001%
19	5.305	1229	1233	1235	rBV	231	180	0.00%	0.001%
20	5.391	1252	1260	1270	rBB4	2355	4460	0.04%	0.017%
21	5.732	1344	1366	1392	rBV2	225400	612474	5.23%	2.342%
22	5.854	1401	1404	1408	rVV2	246	216	0.00%	0.001%
23	6.253	1514	1528	1548	rBV	209719	393069	3.36%	1.503%
24	6.549	1603	1620	1654	rBV	6308143	11706297	100.00%	44.770%
25	6.697	1655	1666	1688	rVB2	141081	282422	2.41%	1.080%
26	7.047	1772	1775	1779	rBB2	226	171	0.00%	0.001%
27	7.568	1925	1937	1952	rBV	80390	137837	1.18%	0.527%
28	7.800	2004	2009	2010	rBV	172	173	0.00%	0.001%
29	7.903	2028	2041	2056	rBV	281598	482599	4.12%	1.846%
30	7.970	2057	2062	2074	rVB2	5347	8552	0.07%	0.033%
31	8.182	2115	2128	2145	rBV	55273	92747	0.79%	0.355%
32	8.276	2153	2157	2160	rBV	379	261	0.00%	0.001%
33	8.305	2164	2166	2171	rVB2	253	209	0.00%	0.001%
34	8.407	2190	2198	2206	rBB3	2066	2883	0.02%	0.011%
35	8.475	2210	2219	2229	rBV2	2923	5321	0.05%	0.020%
36	8.555	2235	2244	2257	rVB3	16467	27532	0.24%	0.105%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046509.D
 Acq On : 20 Dec 2021 14:56
 Operator : SY/MD
 Sample : M5150-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.639	2258	2270	2296	rBV	174591	299463	2.56%	1.145%
38	8.742	2300	2302	2304	rVV	378	234	0.00%	0.001%
39	8.774	2307	2312	2315	rBV2	315	368	0.00%	0.001%
40	8.809	2318	2323	2326	rBV2	247	208	0.00%	0.001%
41	8.931	2356	2361	2363	rVV2	264	204	0.00%	0.001%
42	9.420	2500	2513	2532	rBV	310160	504101	4.31%	1.928%
43	9.510	2539	2541	2544	rVB	335	199	0.00%	0.001%
44	9.575	2555	2561	2565	rBV2	720	788	0.01%	0.003%
45	9.639	2578	2581	2585	rBB	167	166	0.00%	0.001%
46	9.665	2586	2589	2593	rBB	140	142	0.00%	0.001%
47	9.697	2593	2599	2609	rBB3	898	1424	0.01%	0.005%
48	9.784	2624	2626	2631	rBB	135	141	0.00%	0.001%
49	10.005	2692	2695	2698	rBV	139	140	0.00%	0.001%
50	10.044	2703	2707	2711	rBB	150	180	0.00%	0.001%
51	10.099	2720	2724	2727	rVV2	434	435	0.00%	0.002%
52	10.115	2727	2729	2731	rVV	512	314	0.00%	0.001%
53	10.157	2739	2742	2746	rBB	133	138	0.00%	0.001%
54	10.208	2755	2758	2762	rBB	145	144	0.00%	0.001%
55	10.333	2795	2797	2801	rVV2	308	206	0.00%	0.001%
56	10.401	2815	2818	2820	rBV	171	149	0.00%	0.001%
57	10.481	2840	2843	2844	rBV	288	163	0.00%	0.001%
58	10.584	2871	2875	2879	rVB2	365	368	0.00%	0.001%
59	10.677	2896	2904	2909	rBV4	1310	1806	0.02%	0.007%
60	10.758	2916	2929	2946	rVB	195094	312184	2.67%	1.194%
61	10.835	2950	2953	2955	rBV	169	137	0.00%	0.001%
62	10.896	2963	2972	2981	rVB3	2976	4352	0.04%	0.017%
63	10.983	2996	2999	3002	rBB	164	139	0.00%	0.001%
64	11.089	3027	3032	3036	rVB2	414	330	0.00%	0.001%
65	11.201	3064	3067	3072	rBV	169	225	0.00%	0.001%
66	11.275	3087	3090	3093	rBV	170	164	0.00%	0.001%
67	11.391	3123	3126	3129	rBV	158	153	0.00%	0.001%
68	11.446	3137	3143	3144	rBV	405	374	0.00%	0.001%
69	11.468	3144	3150	3159	rVB6	2090	3128	0.03%	0.012%
70	11.507	3159	3162	3164	rBV	154	134	0.00%	0.001%
71	11.610	3190	3194	3196	rBV	168	162	0.00%	0.001%
72	11.697	3218	3221	3224	rVV2	278	218	0.00%	0.001%
73	11.751	3234	3238	3241	rVB2	499	417	0.00%	0.002%
74	11.816	3246	3258	3277	rBV	333633	516416	4.41%	1.975%
75	11.941	3293	3297	3301	rBV2	371	480	0.00%	0.002%
76	11.980	3302	3309	3312	rVV2	642	730	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046509.D
 Acq On : 20 Dec 2021 14:56
 Operator : SY/MD
 Sample : M5150-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.037	3324	3327	3330	rBV	158	167	0.00%	0.001%
78	12.079	3332	3340	3342	rVV2	304	345	0.00%	0.001%
79	12.195	3363	3376	3395	rVB	282269	442181	3.78%	1.691%
80	12.340	3416	3421	3424	rBV	181	228	0.00%	0.001%
81	12.571	3491	3493	3499	rVB	186	214	0.00%	0.001%
82	12.603	3500	3503	3506	rBV	229	217	0.00%	0.001%
83	12.668	3521	3523	3529	rVB	245	230	0.00%	0.001%
84	12.697	3530	3532	3540	rBV	191	275	0.00%	0.001%
85	12.732	3540	3543	3547	rVV	122	142	0.00%	0.001%
86	12.771	3549	3555	3564	rVV2	864	1324	0.01%	0.005%
87	12.816	3564	3569	3575	rVV	96	132	0.00%	0.001%
88	12.999	3621	3626	3631	rBV3	433	415	0.00%	0.002%
89	13.221	3692	3695	3701	rVB	360	408	0.00%	0.002%
90	14.092	3961	3966	3969	rBV	335	360	0.00%	0.001%
91	14.166	3986	3989	3994	rBV	129	134	0.00%	0.001%
92	14.336	4039	4042	4043	rBV2	254	153	0.00%	0.001%
93	15.253	4324	4327	4331	rVB	229	136	0.00%	0.001%
94	15.317	4343	4347	4350	rBV2	233	193	0.00%	0.001%
95	15.410	4374	4376	4382	rVB2	215	143	0.00%	0.001%
96	15.516	4405	4409	4413	rBV2	193	148	0.00%	0.001%
97	15.600	4431	4435	4436	rBV2	200	148	0.00%	0.001%
98	15.642	4445	4448	4450	rBV	227	185	0.00%	0.001%
99	15.799	4494	4497	4500	rBV	184	168	0.00%	0.001%
100	16.031	4566	4569	4572	rBV2	185	187	0.00%	0.001%




Sum of corrected areas: 26147629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046509.D
Acq On : 20 Dec 2021 14:56
Operator : SY/MD
Sample : M5150-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

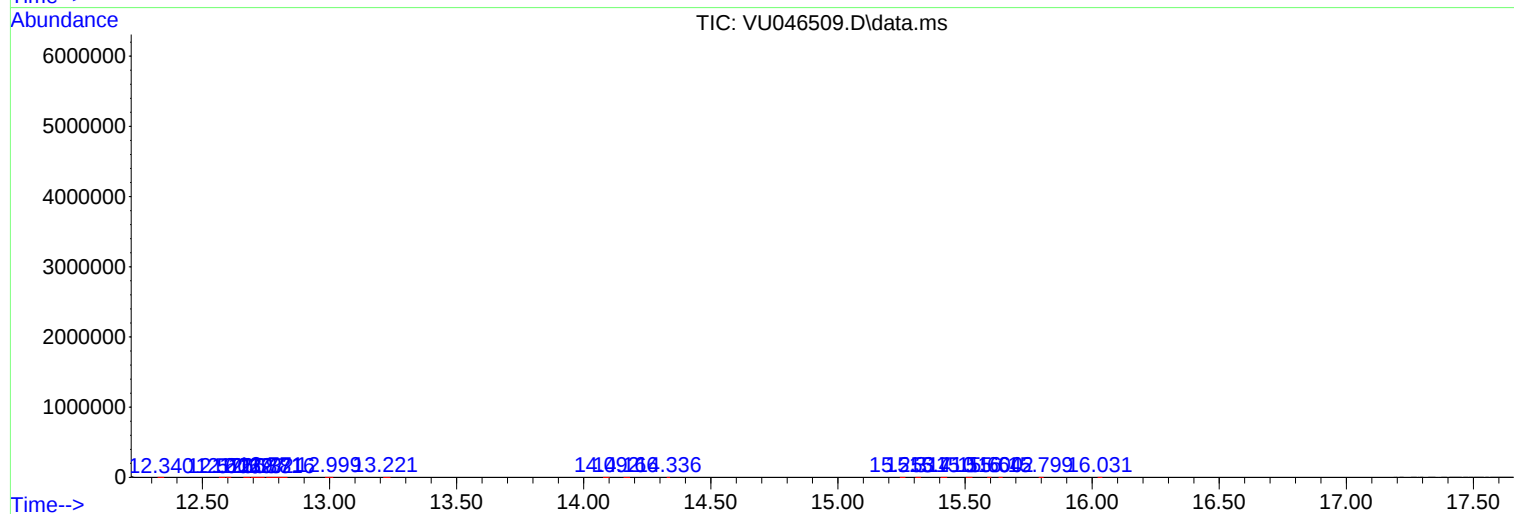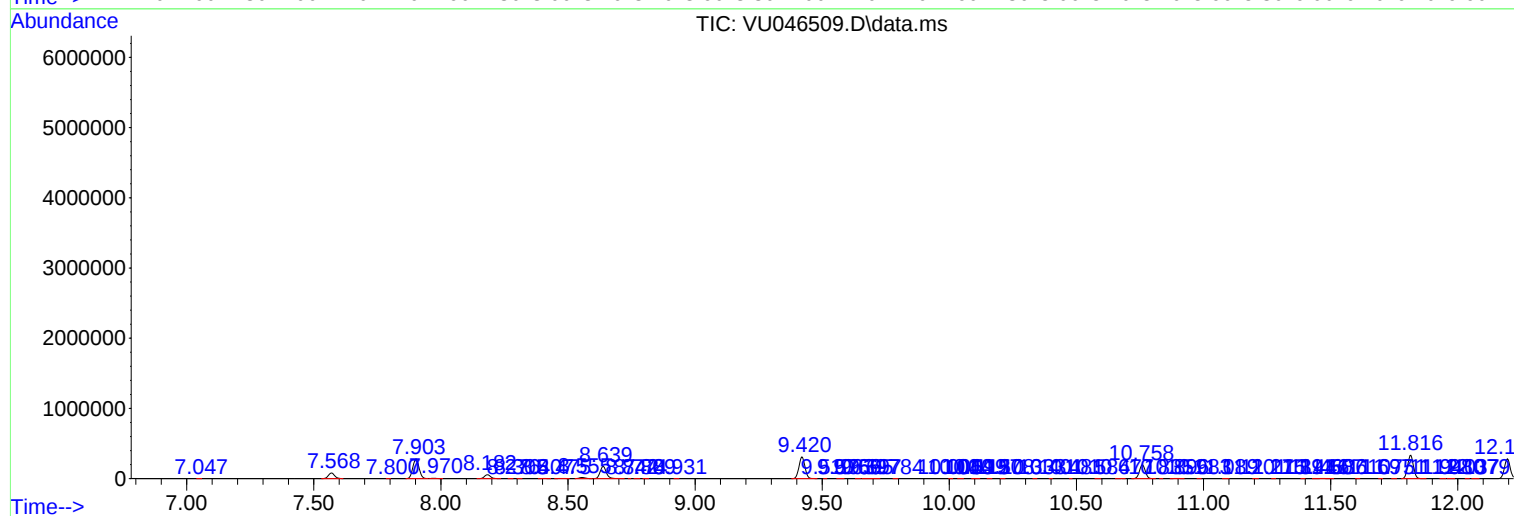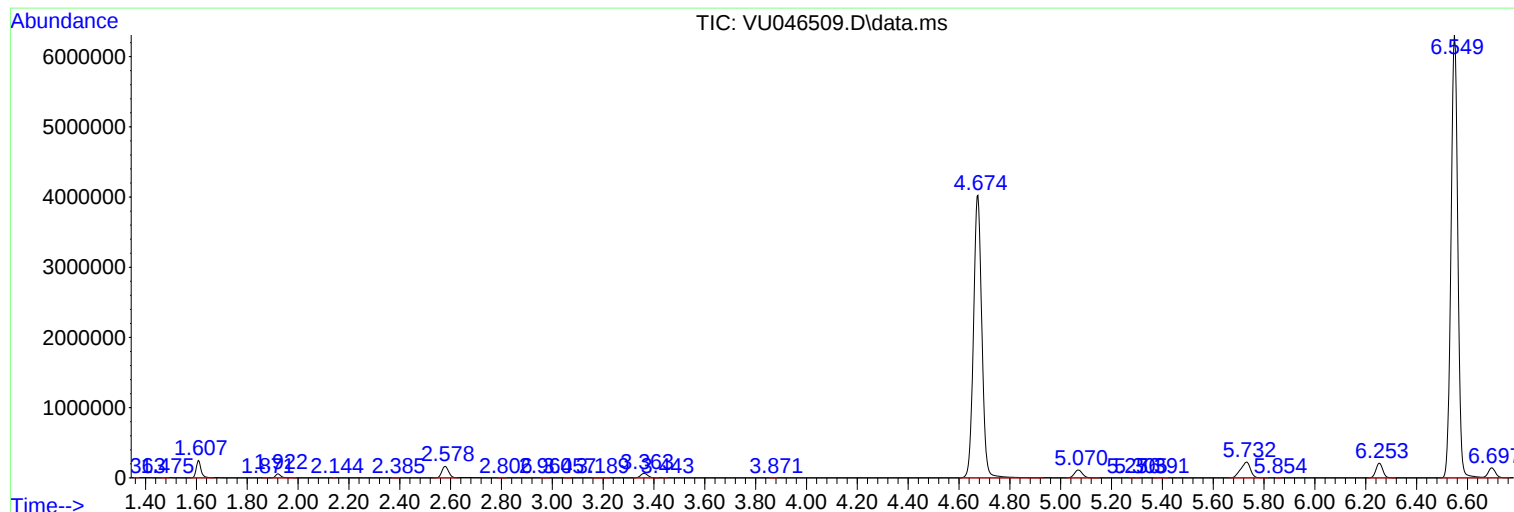

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046509.D
Acq On : 20 Dec 2021 14:56
Operator : SY/MD
Sample : M5150-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046509.D
Acq On : 20 Dec 2021 14:56
Operator : SY/MD
Sample : M5150-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------