

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046510.D
 Acq On : 20 Dec 2021 15:23
 Operator : SY/MD
 Sample : M5150-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	38	42	54	rVB4	1657	1976	0.01%	0.009%
2	1.607	73	83	108	rVB2	69615	92753	0.53%	0.420%
3	1.922	172	181	210	rVB	33677	48585	0.28%	0.220%
4	2.337	306	310	314	rBV	184	205	0.00%	0.001%
5	2.504	359	362	366	rBV2	175	134	0.00%	0.001%
6	2.578	373	385	401	rBV2	98063	184346	1.06%	0.835%
7	2.764	440	443	446	rVB2	163	115	0.00%	0.001%
8	2.800	451	454	455	rBV	170	110	0.00%	0.000%
9	3.002	514	517	521	rBB	130	138	0.00%	0.001%
10	3.054	529	533	537	rBB2	279	281	0.00%	0.001%
11	3.195	566	577	585	rBB3	815	1594	0.01%	0.007%
12	3.362	616	629	643	rBB3	9834	19486	0.11%	0.088%
13	4.671	1014	1036	1076	rBV	710703	1646280	9.45%	7.455%
14	5.070	1145	1160	1177	rBV	64810	143561	0.82%	0.650%
15	5.391	1253	1260	1261	rBV2	1120	1189	0.01%	0.005%
16	5.536	1302	1305	1308	rBB	138	124	0.00%	0.001%
17	5.729	1345	1365	1389	rBV2	128932	352958	2.03%	1.598%
18	5.825	1394	1395	1402	rVB	251	215	0.00%	0.001%
19	6.253	1514	1528	1552	rBV	143626	269136	1.54%	1.219%
20	6.549	1603	1620	1655	rBV	9185698	17427885	100.00%	78.919%
21	6.697	1657	1666	1688	rVB	85022	172346	0.99%	0.780%
22	6.944	1740	1743	1745	rBB	143	98	0.00%	0.000%
23	7.173	1811	1814	1817	rVB	253	197	0.00%	0.001%
24	7.568	1925	1937	1955	rVB2	45163	78188	0.45%	0.354%
25	7.645	1958	1961	1964	rBB2	252	164	0.00%	0.001%
26	7.800	2005	2009	2013	rBB	189	202	0.00%	0.001%
27	7.902	2028	2041	2055	rVV	159298	270844	1.55%	1.226%
28	7.976	2058	2064	2072	rVB4	2204	3627	0.02%	0.016%
29	8.012	2072	2075	2077	rBB	211	107	0.00%	0.000%
30	8.182	2118	2128	2146	rBB2	31505	51886	0.30%	0.235%
31	8.279	2156	2158	2161	rBV	184	154	0.00%	0.001%
32	8.356	2180	2182	2185	rBB	131	94	0.00%	0.000%
33	8.401	2190	2196	2204	rBB5	1935	2982	0.02%	0.014%
34	8.472	2210	2218	2219	rBV2	1853	1618	0.01%	0.007%
35	8.558	2235	2245	2255	rVB3	7647	12294	0.07%	0.056%
36	8.636	2258	2269	2294	rBV	94643	164401	0.94%	0.744%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046510.D
 Acq On : 20 Dec 2021 15:23
 Operator : SY/MD
 Sample : M5150-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.748	2302	2304	2307	rVV	162	95	0.00%	0.000%
38	8.764	2307	2309	2313	rVB2	225	168	0.00%	0.001%
39	9.192	2440	2442	2446	rBV	119	126	0.00%	0.001%
40	9.369	2495	2497	2500	rBB	136	97	0.00%	0.000%
41	9.420	2501	2513	2531	rBV	214433	349834	2.01%	1.584%
42	9.568	2556	2559	2564	rBB	185	194	0.00%	0.001%
43	9.591	2564	2566	2569	rBB	139	95	0.00%	0.000%
44	9.610	2569	2572	2574	rBB	150	100	0.00%	0.000%
45	9.636	2577	2580	2582	rBV	153	129	0.00%	0.001%
46	9.687	2593	2596	2599	rBV2	163	111	0.00%	0.001%
47	9.764	2618	2620	2623	rBB	182	118	0.00%	0.001%
48	9.967	2680	2683	2685	rBV	129	116	0.00%	0.001%
49	10.121	2728	2731	2736	rBB	155	167	0.00%	0.001%
50	10.259	2770	2774	2777	rBV	156	178	0.00%	0.001%
51	10.488	2843	2845	2847	rBV	221	125	0.00%	0.001%
52	10.549	2860	2864	2869	rBV	172	243	0.00%	0.001%
53	10.574	2869	2872	2873	rVV	233	132	0.00%	0.001%
54	10.587	2873	2876	2880	rVV2	252	216	0.00%	0.001%
55	10.674	2895	2903	2909	rVB2	450	576	0.00%	0.003%
56	10.758	2917	2929	2945	rBV	112137	178525	1.02%	0.808%
57	10.890	2963	2970	2981	rBV3	1594	2479	0.01%	0.011%
58	11.086	3028	3031	3034	rVB	192	148	0.00%	0.001%
59	11.198	3062	3066	3069	rBB	154	155	0.00%	0.001%
60	11.256	3078	3084	3089	rBB	170	261	0.00%	0.001%
61	11.291	3089	3095	3101	rBV	151	304	0.00%	0.001%
62	11.375	3117	3121	3127	rBB	191	240	0.00%	0.001%
63	11.433	3136	3139	3141	rBV	144	121	0.00%	0.001%
64	11.468	3143	3150	3156	rVB3	690	864	0.00%	0.004%
65	11.516	3162	3165	3167	rBV	143	120	0.00%	0.001%
66	11.539	3169	3172	3176	rVB	92	102	0.00%	0.000%
67	11.581	3183	3185	3192	rBV	151	231	0.00%	0.001%
68	11.671	3209	3213	3218	rBV	146	225	0.00%	0.001%
69	11.697	3218	3221	3224	rVB2	181	125	0.00%	0.001%
70	11.812	3245	3257	3273	rBV	222240	345457	1.98%	1.564%
71	11.976	3304	3308	3311	rBV2	274	220	0.00%	0.001%
72	12.063	3331	3335	3336	rVV	198	147	0.00%	0.001%
73	12.086	3338	3342	3346	rVB	243	201	0.00%	0.001%
74	12.195	3364	3376	3393	rVB	153696	245931	1.41%	1.114%
75	12.774	3551	3556	3562	rBV	531	546	0.00%	0.002%
76	13.147	3666	3672	3678	rBV	227	400	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046510.D
 Acq On : 20 Dec 2021 15:23
 Operator : SY/MD
 Sample : M5150-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	13.227	3695	3697	3701	rBV2	146	101	0.00%	0.000%
78	13.844	3887	3889	3894	rVB	286	183	0.00%	0.001%
79	13.880	3894	3900	3906	rBV	122	164	0.00%	0.001%
80	14.143	3980	3982	3988	rVB	136	100	0.00%	0.000%
81	14.295	4026	4029	4035	rBV	107	118	0.00%	0.001%
82	14.912	4219	4221	4226	rBV2	159	120	0.00%	0.001%
83	15.413	4374	4377	4380	rVB2	216	121	0.00%	0.001%
84	15.458	4389	4391	4393	rVB	180	99	0.00%	0.000%
85	15.500	4401	4404	4408	rVB	201	121	0.00%	0.001%
86	15.523	4408	4411	4413	rBV2	251	153	0.00%	0.001%
87	15.555	4419	4421	4424	rVB	198	122	0.00%	0.001%
88	15.574	4424	4427	4430	rBV	198	146	0.00%	0.001%
89	15.648	4447	4450	4454	rVB	190	124	0.00%	0.001%
90	15.674	4454	4458	4460	rBV2	183	130	0.00%	0.001%
91	15.719	4470	4472	4476	rVB2	178	132	0.00%	0.001%
92	15.741	4476	4479	4484	rVB2	207	224	0.00%	0.001%
93	15.767	4484	4487	4488	rBV2	169	113	0.00%	0.001%
94	15.793	4492	4495	4498	rBV	164	147	0.00%	0.001%
95	15.867	4515	4518	4520	rBV	145	95	0.00%	0.000%
96	15.886	4520	4524	4525	rBV2	159	112	0.00%	0.001%
97	15.934	4537	4539	4542	rBV2	178	132	0.00%	0.001%
98	16.667	4765	4767	4773	rVB3	297	189	0.00%	0.001%
99	16.925	4845	4847	4849	rBV	289	104	0.00%	0.000%
100	17.082	4892	4896	4897	rBV2	405	311	0.00%	0.001%




Sum of corrected areas: 22083256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046510.D
Acq On : 20 Dec 2021 15:23
Operator : SY/MD
Sample : M5150-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

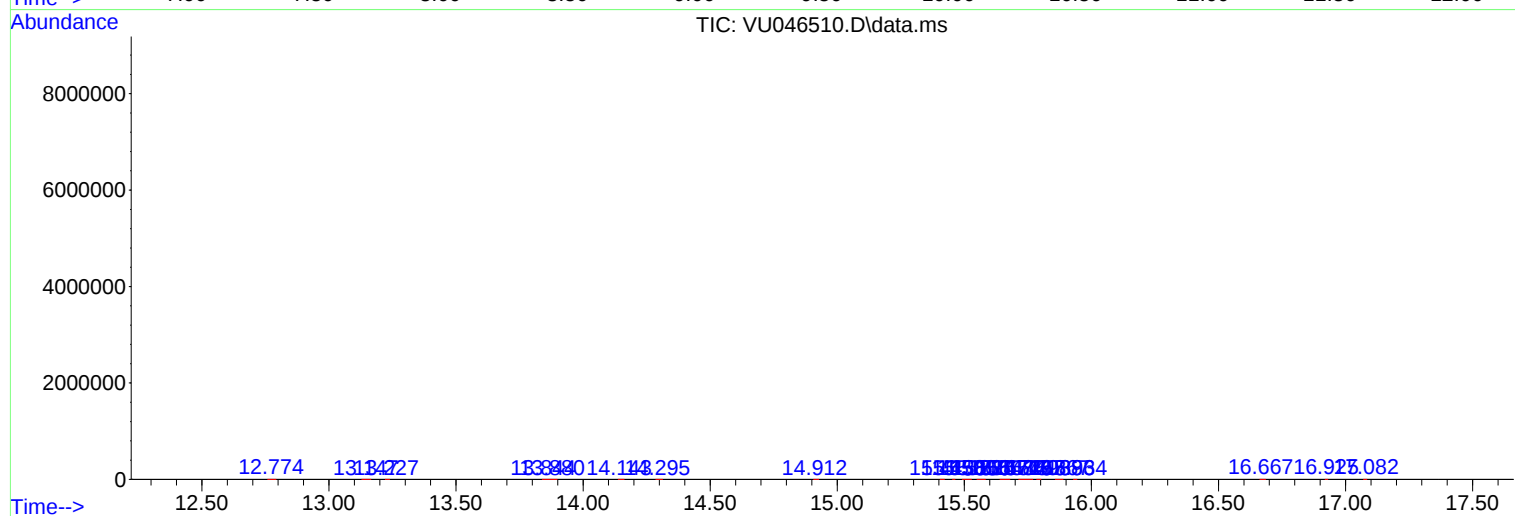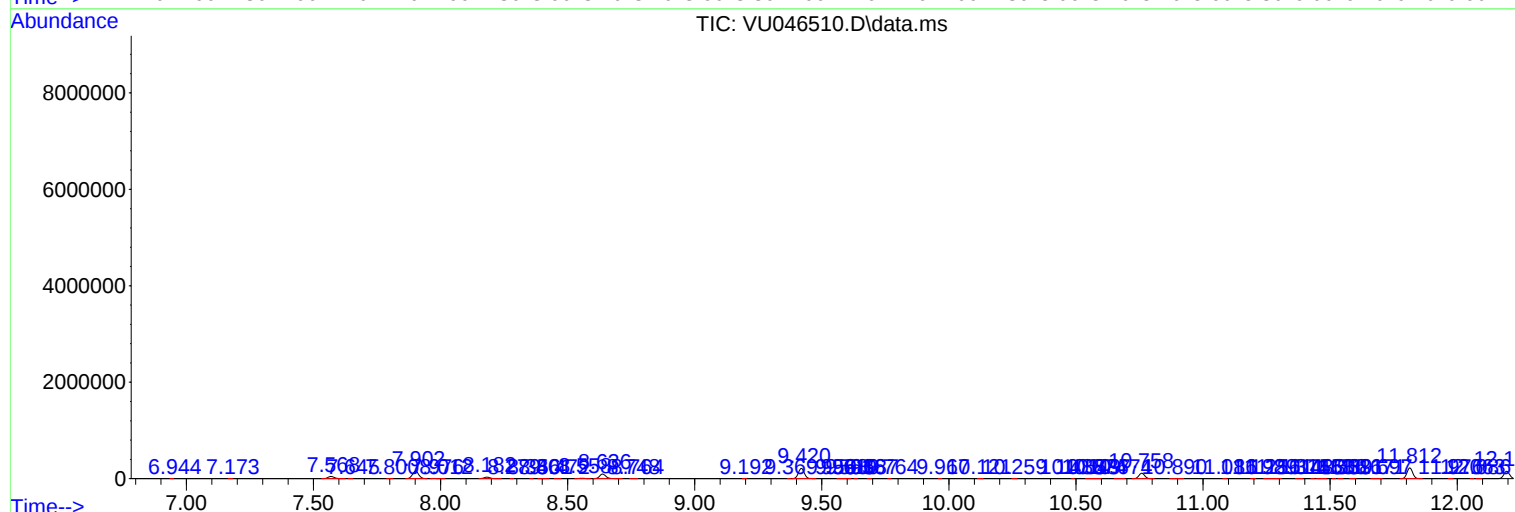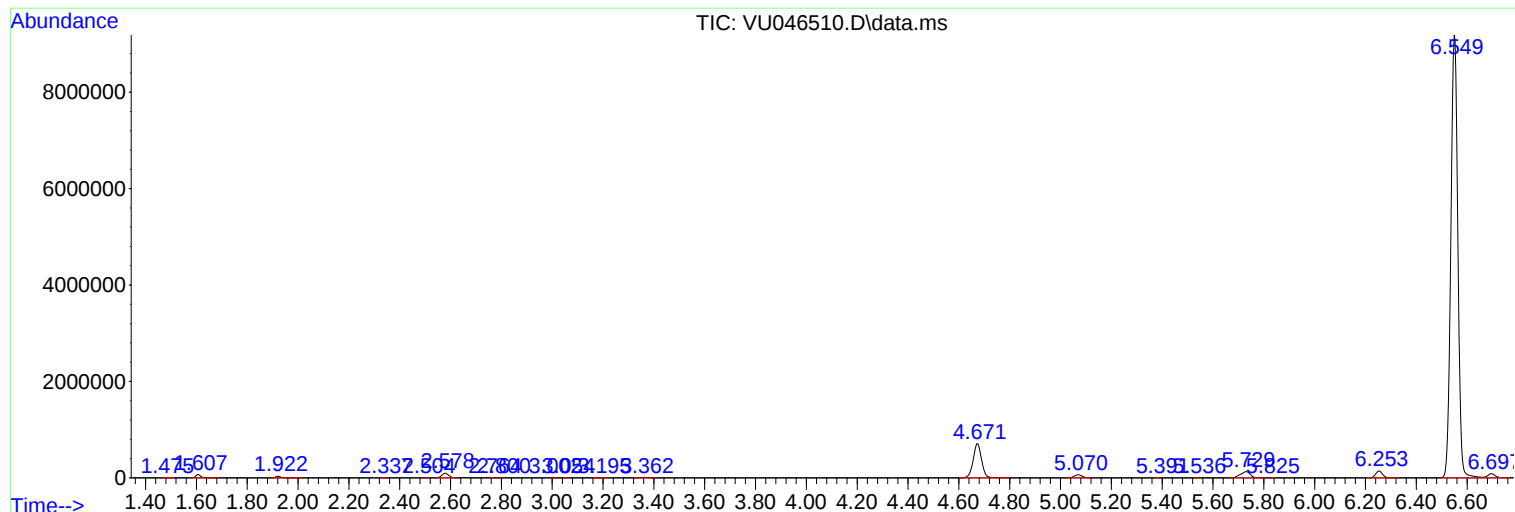

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046510.D
Acq On : 20 Dec 2021 15:23
Operator : SY/MD
Sample : M5150-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046510.D
Acq On : 20 Dec 2021 15:23
Operator : SY/MD
Sample : M5150-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc