

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046514.D
 Acq On : 20 Dec 2021 16:52
 Operator : SY/MD
 Sample : M5121-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	63484	77147	15.70%	1.874%
2	1.919	171	180	201	rBV	44090	63638	12.95%	1.546%
3	2.459	346	348	353	rVB2	173	133	0.03%	0.003%
4	2.530	368	370	372	rBV	153	106	0.02%	0.003%
5	2.575	372	384	404	rBV	106920	178101	36.25%	4.326%
6	2.758	437	441	445	rBB	148	177	0.04%	0.004%
7	2.803	448	455	460	rBB2	492	775	0.16%	0.019%
8	2.916	487	490	494	rBV	136	157	0.03%	0.004%
9	2.970	505	507	509	rBV	133	96	0.02%	0.002%
10	3.054	526	533	540	rBB4	612	1079	0.22%	0.026%
11	3.195	575	577	580	rBB	274	149	0.03%	0.004%
12	3.292	605	607	610	rBB	133	94	0.02%	0.002%
13	3.925	802	804	806	rBB	151	80	0.02%	0.002%
14	4.523	987	990	992	rBB	127	88	0.02%	0.002%
15	4.645	1013	1028	1062	rBV	36788	124203	25.28%	3.017%
16	4.858	1091	1094	1096	rVB2	290	183	0.04%	0.004%
17	4.896	1102	1106	1108	rBB	137	119	0.02%	0.003%
18	5.067	1143	1159	1180	rBV2	91665	199039	40.51%	4.835%
19	5.729	1344	1365	1393	rBV2	181188	491286	100.00%	11.934%
20	6.250	1514	1527	1546	rBV	179709	339478	69.10%	8.246%
21	6.546	1607	1619	1634	rBB2	38445	71087	14.47%	1.727%
22	6.694	1652	1665	1683	rBB	114207	218501	44.48%	5.308%
23	6.761	1684	1686	1688	rBB	232	87	0.02%	0.002%
24	7.568	1925	1937	1951	rBV	63614	108890	22.16%	2.645%
25	7.899	2027	2040	2055	rBV	228862	388453	79.07%	9.436%
26	7.970	2055	2062	2072	rVB	2957	4950	1.01%	0.120%
27	8.179	2116	2127	2140	rBV	44228	73699	15.00%	1.790%
28	8.259	2150	2152	2155	rBB	151	98	0.02%	0.002%
29	8.449	2209	2211	2212	rBV	144	80	0.02%	0.002%
30	8.472	2212	2218	2227	rVV	621	1011	0.21%	0.025%
31	8.533	2235	2237	2241	rVB2	183	107	0.02%	0.003%
32	8.555	2241	2244	2250	rVB3	415	368	0.07%	0.009%
33	8.636	2257	2269	2289	rBV	150062	254671	51.84%	6.186%
34	8.841	2330	2333	2337	rBB	163	158	0.03%	0.004%
35	8.970	2370	2373	2376	rBB	142	97	0.02%	0.002%
36	8.996	2379	2381	2382	rBV	134	74	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046514.D
 Acq On : 20 Dec 2021 16:52
 Operator : SY/MD
 Sample : M5121-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	9.054	2396	2399	2401	rBB	120	87	0.02%	0.002%
38	9.189	2438	2441	2443	rBB	128	91	0.02%	0.002%
39	9.240	2455	2457	2459	rBV	109	79	0.02%	0.002%
40	9.417	2500	2512	2533	rBV	267637	438865	89.33%	10.661%
41	9.533	2546	2548	2550	rBB	142	74	0.02%	0.002%
42	9.549	2551	2553	2555	rBV	121	87	0.02%	0.002%
43	9.568	2555	2559	2562	rVV	218	220	0.04%	0.005%
44	9.581	2562	2563	2569	rVB	282	227	0.05%	0.006%
45	9.613	2570	2573	2578	rBB	137	142	0.03%	0.003%
46	9.697	2594	2599	2604	rBV2	585	698	0.14%	0.017%
47	9.886	2654	2658	2660	rBB	127	88	0.02%	0.002%
48	9.992	2687	2691	2692	rBV	156	108	0.02%	0.003%
49	10.025	2698	2701	2703	rBB	124	89	0.02%	0.002%
50	10.070	2710	2715	2718	rBB	166	176	0.04%	0.004%
51	10.124	2730	2732	2735	rVB2	208	101	0.02%	0.002%
52	10.150	2736	2740	2742	rBV	181	166	0.03%	0.004%
53	10.259	2771	2774	2776	rBV	133	117	0.02%	0.003%
54	10.346	2799	2801	2803	rBB	141	75	0.02%	0.002%
55	10.362	2803	2806	2808	rBB	163	105	0.02%	0.003%
56	10.433	2823	2828	2835	rBV	180	291	0.06%	0.007%
57	10.478	2840	2842	2848	rBB	184	192	0.04%	0.005%
58	10.507	2849	2851	2853	rBV	109	83	0.02%	0.002%
59	10.549	2861	2864	2867	rBV	154	147	0.03%	0.004%
60	10.619	2884	2886	2888	rBV	125	88	0.02%	0.002%
61	10.671	2896	2902	2909	rBV2	1093	1081	0.22%	0.026%
62	10.700	2909	2911	2914	rVB	208	131	0.03%	0.003%
63	10.758	2915	2929	2946	rBV	162400	260327	52.99%	6.324%
64	10.877	2963	2966	2967	rBV	241	142	0.03%	0.003%
65	10.893	2967	2971	2977	rVV2	463	569	0.12%	0.014%
66	11.086	3028	3031	3036	rBB	373	331	0.07%	0.008%
67	11.124	3037	3043	3047	rBV	183	289	0.06%	0.007%
68	11.195	3062	3065	3067	rBB	133	93	0.02%	0.002%
69	11.230	3068	3076	3078	rBV	176	254	0.05%	0.006%
70	11.369	3116	3119	3124	rBV	208	261	0.05%	0.006%
71	11.468	3140	3150	3156	rVB3	681	1044	0.21%	0.025%
72	11.542	3169	3173	3179	rBV	147	235	0.05%	0.006%
73	11.581	3182	3185	3187	rVV	222	138	0.03%	0.003%
74	11.603	3187	3192	3198	rVV	92	116	0.02%	0.003%
75	11.687	3213	3218	3219	rBV	197	184	0.04%	0.004%
76	11.700	3219	3222	3228	rVB2	305	359	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046514.D
 Acq On : 20 Dec 2021 16:52
 Operator : SY/MD
 Sample : M5121-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.732	3229	3232	3233	rBV	194	125	0.03%	0.003%
78	11.742	3233	3235	3237	rBV	286	205	0.04%	0.005%
79	11.812	3244	3257	3273	rBV	282868	441829	89.93%	10.733%
80	11.912	3285	3288	3292	rBV	202	198	0.04%	0.005%
81	11.938	3292	3296	3299	rVV2	323	352	0.07%	0.009%
82	11.970	3303	3306	3316	rVB2	541	579	0.12%	0.014%
83	12.192	3364	3375	3392	rBV	223385	361583	73.60%	8.783%
84	12.385	3432	3435	3441	rBV	206	278	0.06%	0.007%
85	12.770	3551	3555	3558	rBV2	203	190	0.04%	0.005%
86	13.221	3690	3695	3704	rBV3	415	557	0.11%	0.014%
87	13.494	3776	3780	3784	rBV	82	85	0.02%	0.002%
88	13.841	3884	3888	3895	rBV3	616	768	0.16%	0.019%
89	14.095	3959	3967	3975	rBV	595	1009	0.21%	0.025%
90	14.333	4035	4041	4048	rBB3	552	702	0.14%	0.017%
91	14.655	4138	4141	4146	rBV	121	102	0.02%	0.002%
92	14.719	4159	4161	4169	rBV	92	121	0.02%	0.003%
93	14.780	4177	4180	4183	rBV	117	94	0.02%	0.002%
94	14.841	4194	4199	4204	rBV	205	245	0.05%	0.006%
95	15.298	4339	4341	4344	rBV	143	104	0.02%	0.003%
96	15.571	4424	4426	4430	rBV2	192	154	0.03%	0.004%
97	15.741	4477	4479	4485	rVB	319	236	0.05%	0.006%
98	15.774	4485	4489	4492	rBV2	232	217	0.04%	0.005%
99	16.301	4650	4653	4654	rBV	227	110	0.02%	0.003%
100	17.388	4988	4991	4993	rBV3	574	429	0.09%	0.010%




Sum of corrected areas: 4116681

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046514.D
Acq On : 20 Dec 2021 16:52
Operator : SY/MD
Sample : M5121-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

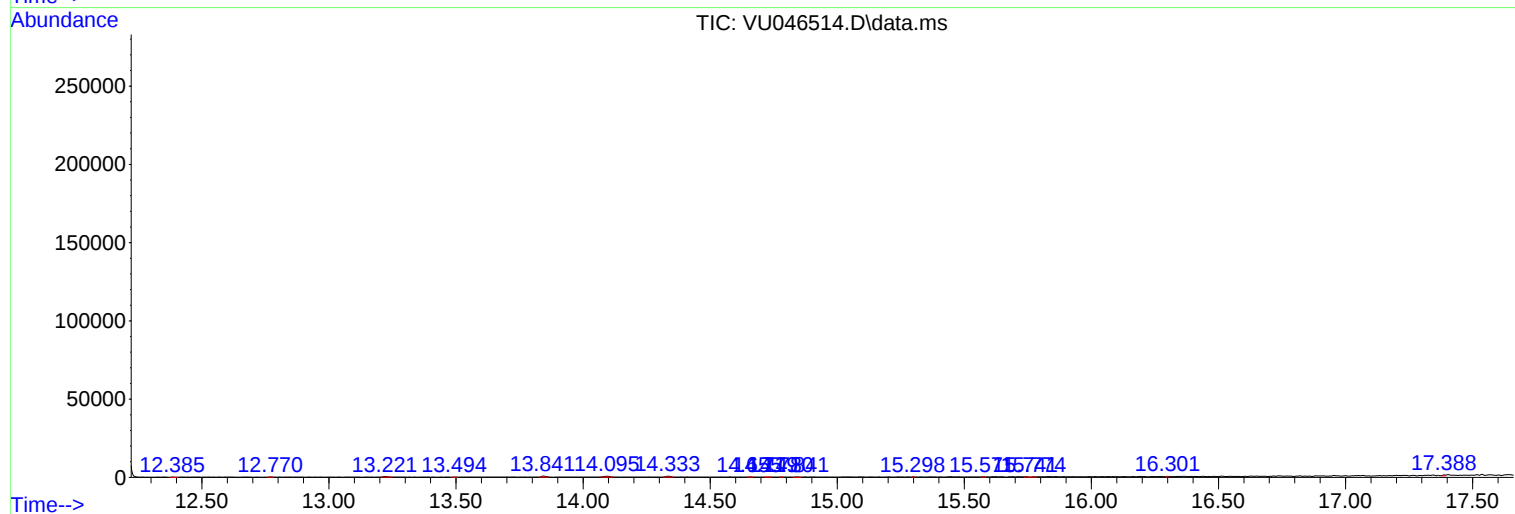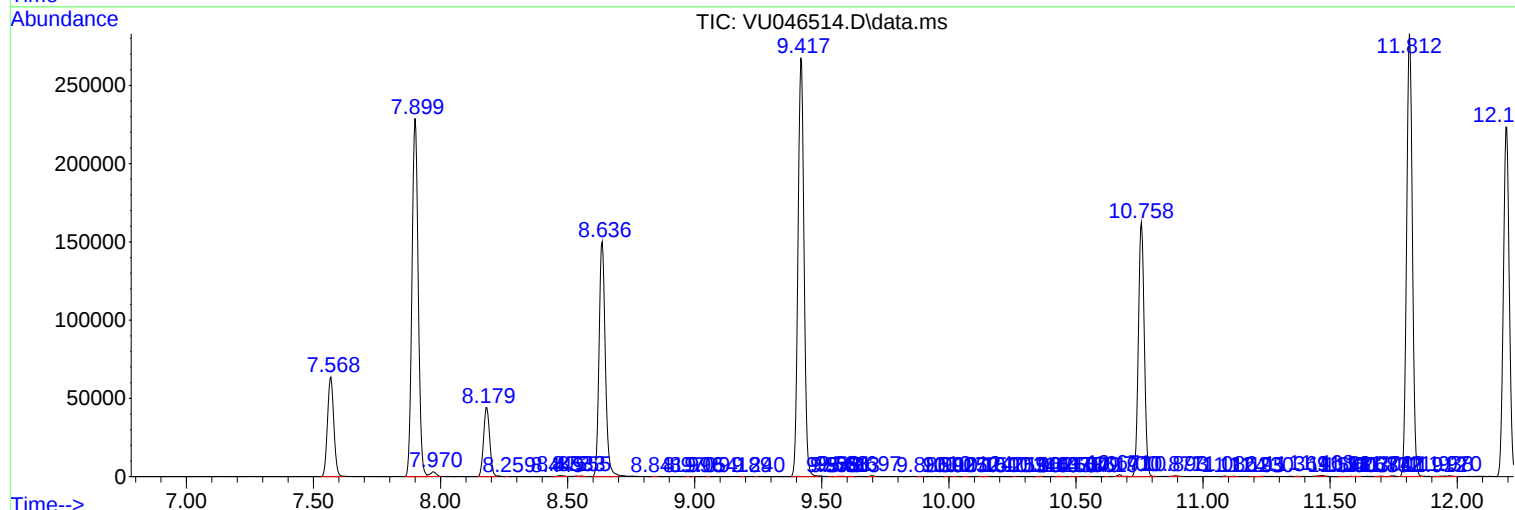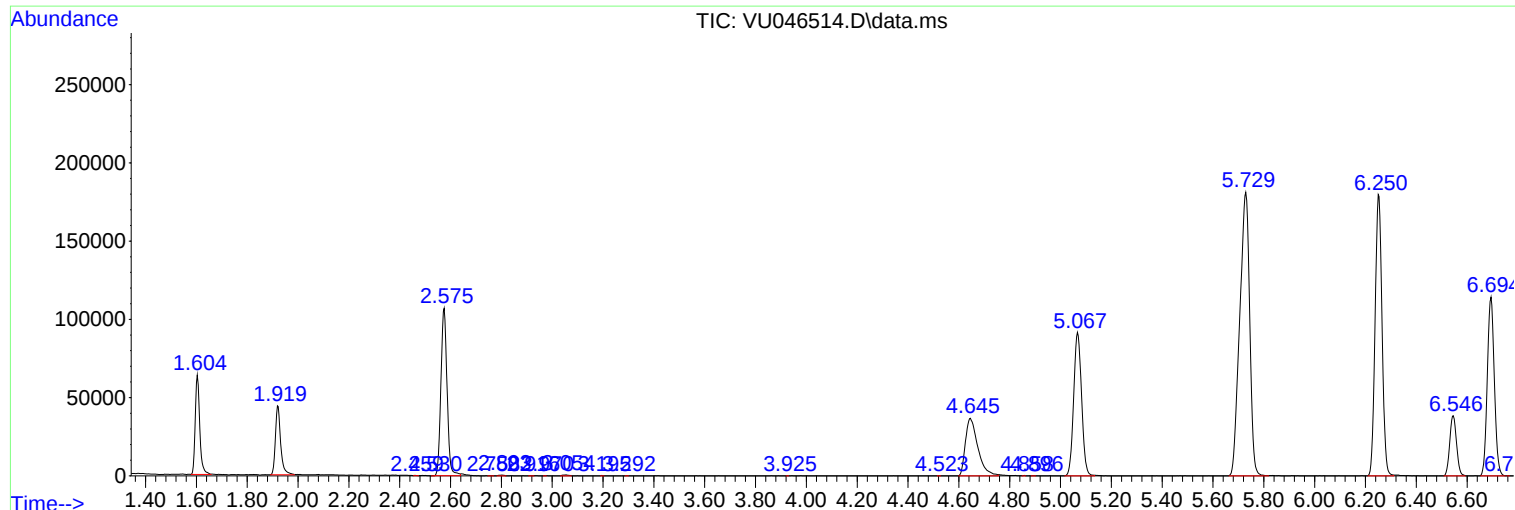

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046514.D
Acq On : 20 Dec 2021 16:52
Operator : SY/MD
Sample : M5121-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046514.D
Acq On : 20 Dec 2021 16:52
Operator : SY/MD
Sample : M5121-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
