

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046516.D
 Acq On : 20 Dec 2021 17:37
 Operator : SY/MD
 Sample : M5150-27
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	37	42	48	rVB2	3239	3327	0.59%	0.073%
2	1.604	74	82	100	rBV	73442	89210	15.77%	1.950%
3	1.739	119	124	129	rBV2	611	658	0.12%	0.014%
4	1.922	171	181	203	rVB	50501	73432	12.98%	1.606%
5	2.347	310	313	318	rVB2	181	147	0.03%	0.003%
6	2.369	318	320	322	rBV	225	153	0.03%	0.003%
7	2.575	372	384	397	rBV	121288	198261	35.05%	4.335%
8	2.713	426	427	431	rVB	268	127	0.02%	0.003%
9	2.810	454	457	460	rBB	299	206	0.04%	0.005%
10	3.054	531	533	537	rBB	355	222	0.04%	0.005%
11	3.189	563	575	589	rVB2	6245	13640	2.41%	0.298%
12	4.642	1011	1027	1066	rBV2	46383	152351	26.93%	3.331%
13	4.777	1066	1069	1072	rVB3	292	159	0.03%	0.003%
14	5.067	1144	1159	1180	rBV	104001	224699	39.72%	4.913%
15	5.729	1344	1365	1385	rBV2	210514	565717	100.00%	12.369%
16	6.250	1513	1527	1546	rBV	195036	364394	64.41%	7.967%
17	6.546	1608	1619	1631	rBB3	11980	21426	3.79%	0.468%
18	6.694	1651	1665	1689	rBB	128680	249265	44.06%	5.450%
19	7.186	1816	1818	1821	rBB	250	117	0.02%	0.003%
20	7.568	1925	1937	1953	rBV	72572	125060	22.11%	2.734%
21	7.623	1953	1954	1960	rVB	370	297	0.05%	0.006%
22	7.899	2026	2040	2056	rBV	259299	443233	78.35%	9.691%
23	7.970	2057	2062	2073	rVB2	3734	6022	1.06%	0.132%
24	8.015	2073	2076	2082	rBB	166	200	0.04%	0.004%
25	8.128	2108	2111	2114	rBV	158	157	0.03%	0.003%
26	8.179	2116	2127	2144	rBV	49784	83146	14.70%	1.818%
27	8.240	2144	2146	2150	rVB2	377	252	0.04%	0.006%
28	8.388	2190	2192	2196	rBB	137	118	0.02%	0.003%
29	8.452	2210	2212	2213	rBV	281	141	0.02%	0.003%
30	8.472	2213	2218	2223	rVV2	790	1032	0.18%	0.023%
31	8.539	2236	2239	2242	rVB	228	139	0.02%	0.003%
32	8.565	2242	2247	2251	rVB2	227	259	0.05%	0.006%
33	8.636	2257	2269	2296	rBV	170226	287886	50.89%	6.294%
34	8.796	2314	2319	2322	rBV	178	215	0.04%	0.005%
35	8.816	2322	2325	2327	rVV	157	126	0.02%	0.003%
36	8.874	2340	2343	2347	rVB	177	165	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046516.D
 Acq On : 20 Dec 2021 17:37
 Operator : SY/MD
 Sample : M5150-27
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.931	2358	2361	2365	rBV	155	186	0.03%	0.004%
38	8.980	2373	2376	2380	rBV	166	175	0.03%	0.004%
39	9.005	2381	2384	2387	rVB	175	141	0.02%	0.003%
40	9.308	2474	2478	2482	rBB	151	169	0.03%	0.004%
41	9.417	2500	2512	2534	rBV	285618	467851	82.70%	10.229%
42	9.510	2538	2541	2544	rVB	432	342	0.06%	0.007%
43	9.558	2552	2556	2557	rBV	132	116	0.02%	0.003%
44	9.565	2557	2558	2562	rVB	246	130	0.02%	0.003%
45	9.610	2568	2572	2575	rBV	150	173	0.03%	0.004%
46	9.665	2586	2589	2591	rBB	160	111	0.02%	0.002%
47	9.700	2596	2600	2604	rVB2	379	349	0.06%	0.008%
48	9.829	2638	2640	2643	rBV	141	126	0.02%	0.003%
49	9.861	2647	2650	2653	rBV	142	145	0.03%	0.003%
50	9.951	2675	2678	2682	rBV	127	158	0.03%	0.003%
51	10.047	2704	2708	2711	rBB	141	142	0.03%	0.003%
52	10.121	2727	2731	2734	rBV	153	178	0.03%	0.004%
53	10.195	2751	2754	2756	rBV	154	124	0.02%	0.003%
54	10.253	2769	2772	2774	rBV	176	134	0.02%	0.003%
55	10.304	2785	2788	2790	rBV	146	118	0.02%	0.003%
56	10.366	2805	2807	2813	rBB	133	164	0.03%	0.004%
57	10.423	2819	2825	2828	rBV	155	217	0.04%	0.005%
58	10.472	2836	2840	2844	rBB	174	207	0.04%	0.005%
59	10.562	2865	2868	2871	rBV	156	142	0.03%	0.003%
60	10.587	2873	2876	2880	rVV	165	180	0.03%	0.004%
61	10.620	2883	2886	2890	rVB	173	142	0.03%	0.003%
62	10.671	2895	2902	2909	rVB3	1100	1343	0.24%	0.029%
63	10.758	2917	2929	2946	rBV	186780	296148	52.35%	6.475%
64	10.857	2956	2960	2964	rBB	217	225	0.04%	0.005%
65	10.893	2964	2971	2974	rBV3	934	1212	0.21%	0.026%
66	11.041	3013	3017	3019	rBV	143	146	0.03%	0.003%
67	11.111	3035	3039	3040	rBV	154	137	0.02%	0.003%
68	11.330	3102	3107	3110	rBV	169	219	0.04%	0.005%
69	11.378	3119	3122	3124	rBV	129	117	0.02%	0.003%
70	11.411	3126	3132	3136	rBB	177	247	0.04%	0.005%
71	11.456	3140	3146	3147	rVV	420	336	0.06%	0.007%
72	11.468	3147	3150	3156	rVB2	595	567	0.10%	0.012%
73	11.533	3165	3170	3173	rBV	162	220	0.04%	0.005%
74	11.581	3183	3185	3187	rBV	229	117	0.02%	0.003%
75	11.693	3214	3220	3224	rBV2	199	220	0.04%	0.005%
76	11.812	3245	3257	3272	rBV	307830	476062	84.15%	10.409%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046516.D
 Acq On : 20 Dec 2021 17:37
 Operator : SY/MD
 Sample : M5150-27
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.947	3293	3299	3301	rBV	188	242	0.04%	0.005%
78	11.973	3303	3307	3309	rVV3	373	220	0.04%	0.005%
79	12.076	3334	3339	3340	rBV2	156	149	0.03%	0.003%
80	12.134	3353	3357	3361	rBV	118	116	0.02%	0.003%
81	12.192	3361	3375	3390	rBV	259860	413863	73.16%	9.049%
82	12.771	3551	3555	3561	rBV2	291	326	0.06%	0.007%
83	13.224	3693	3696	3700	rVV3	277	218	0.04%	0.005%
84	13.346	3731	3734	3741	rVB	132	126	0.02%	0.003%
85	13.472	3768	3773	3778	rBV	107	138	0.02%	0.003%
86	13.780	3863	3869	3874	rBV	127	171	0.03%	0.004%
87	13.841	3885	3888	3894	rVB2	321	320	0.06%	0.007%
88	14.089	3962	3965	3967	rBV2	260	204	0.04%	0.004%
89	14.336	4039	4042	4044	rVB	185	126	0.02%	0.003%
90	15.266	4328	4331	4335	rBV	146	150	0.03%	0.003%
91	15.311	4343	4345	4348	rVV	235	131	0.02%	0.003%
92	15.330	4348	4351	4359	rVB2	203	286	0.05%	0.006%
93	15.468	4391	4394	4397	rBV2	136	140	0.02%	0.003%
94	15.529	4409	4413	4419	rVB	258	211	0.04%	0.005%
95	15.780	4487	4491	4494	rBV2	247	262	0.05%	0.006%
96	15.957	4543	4546	4549	rBV2	204	186	0.03%	0.004%
97	16.468	4703	4705	4707	rBV	319	158	0.03%	0.003%
98	16.999	4868	4870	4872	rBV	277	165	0.03%	0.004%
99	17.217	4936	4938	4940	rBV	423	249	0.04%	0.005%
100	17.349	4976	4979	4982	rBV3	547	365	0.06%	0.008%




Sum of corrected areas: 4573717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046516.D
Acq On : 20 Dec 2021 17:37
Operator : SY/MD
Sample : M5150-27
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

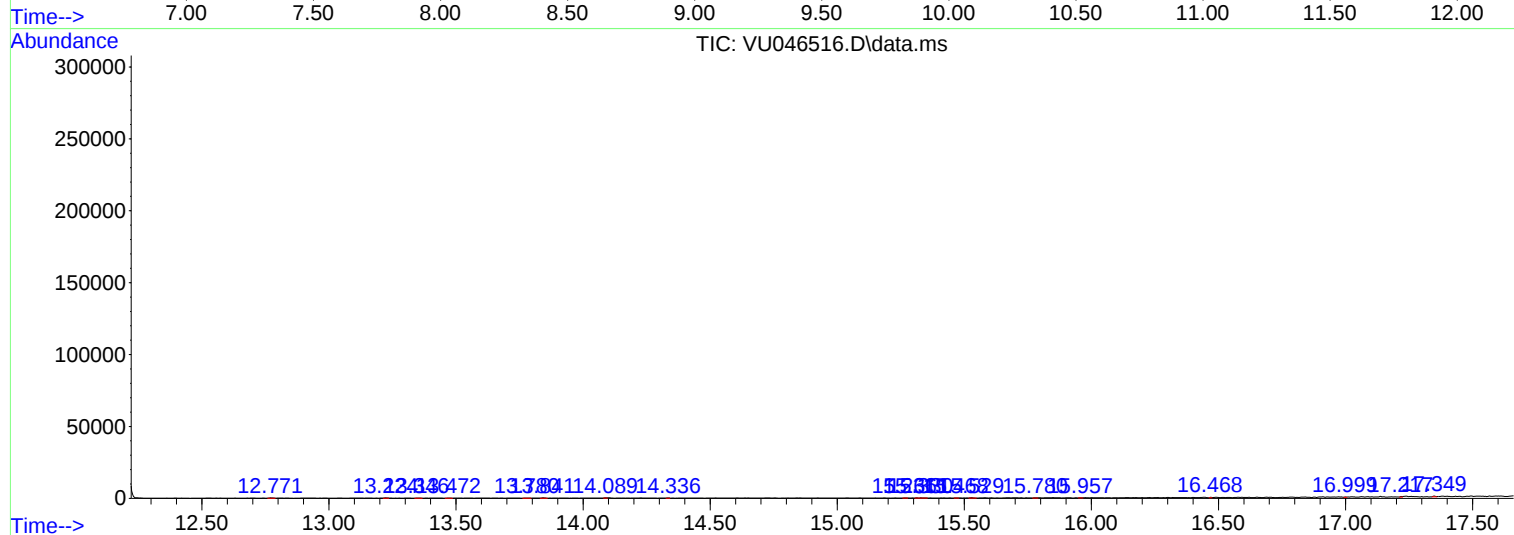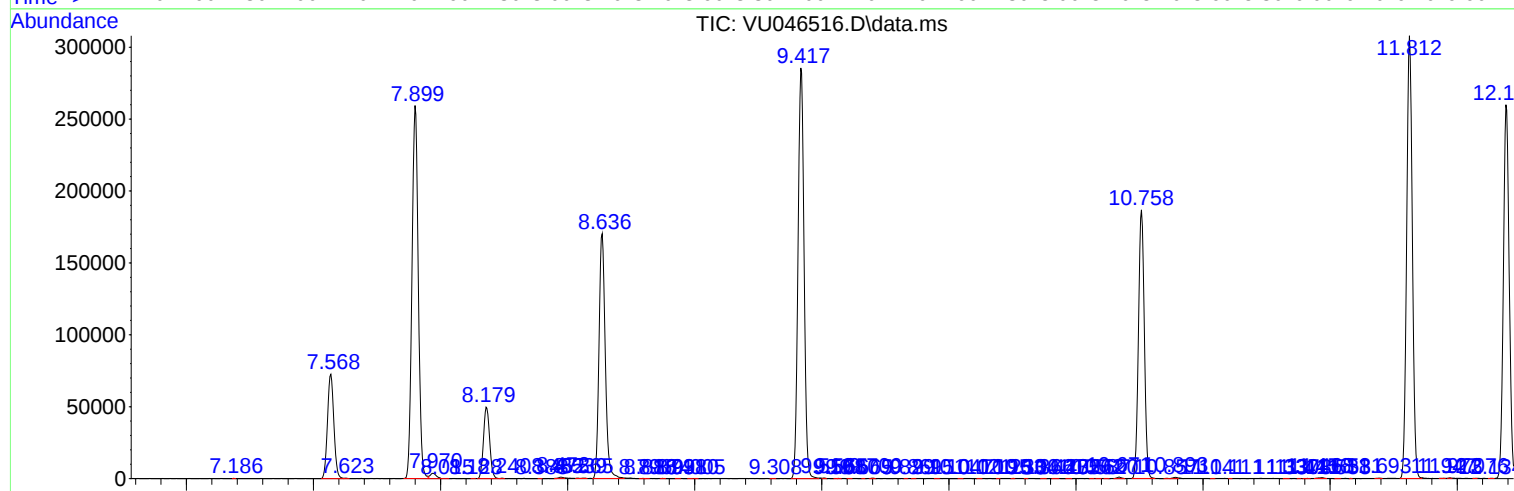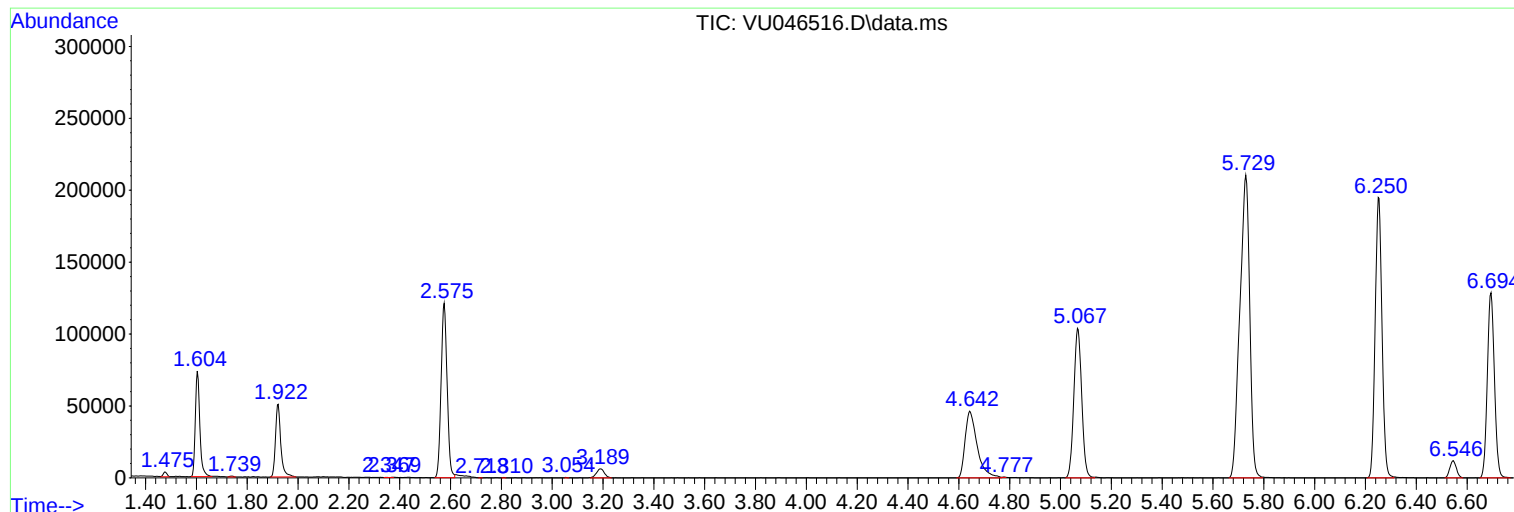

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046516.D
Acq On : 20 Dec 2021 17:37
Operator : SY/MD
Sample : M5150-27
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046516.D
Acq On : 20 Dec 2021 17:37
Operator : SY/MD
Sample : M5150-27
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------