

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046517.D
 Acq On : 20 Dec 2021 18:00
 Operator : SY/MD
 Sample : M5153-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	37	42	48	rVB	2524	2422	0.52%	0.063%
2	1.604	74	82	103	rVB	62071	75904	16.15%	1.975%
3	1.681	104	106	112	rVB2	344	251	0.05%	0.007%
4	1.919	171	180	203	rVV	43222	61770	13.15%	1.607%
5	2.015	207	210	214	rBV2	219	183	0.04%	0.005%
6	2.237	277	279	283	rBV2	176	145	0.03%	0.004%
7	2.385	321	325	328	rVB	219	185	0.04%	0.005%
8	2.404	328	331	333	rBV2	212	172	0.04%	0.004%
9	2.575	371	384	400	rBV	100006	166596	35.46%	4.334%
10	2.771	443	445	447	rBV	271	159	0.03%	0.004%
11	2.800	451	454	460	rVB2	209	216	0.05%	0.006%
12	2.851	468	470	473	rBV	138	115	0.02%	0.003%
13	2.906	481	487	488	rBV2	266	274	0.06%	0.007%
14	2.941	494	498	500	rBV2	207	171	0.04%	0.004%
15	2.957	500	503	505	rVV2	273	206	0.04%	0.005%
16	2.970	505	507	511	rVV	255	156	0.03%	0.004%
17	3.054	529	533	541	rVB3	416	328	0.07%	0.009%
18	3.179	566	572	573	rBV	396	329	0.07%	0.009%
19	4.645	1013	1028	1058	rBV2	33705	115813	24.65%	3.013%
20	4.813	1069	1080	1095	rVB2	4026	9830	2.09%	0.256%
21	4.903	1105	1108	1110	rVB	344	174	0.04%	0.005%
22	5.067	1143	1159	1184	rBB	85989	188905	40.21%	4.914%
23	5.729	1344	1365	1391	rBV2	172709	469853	100.00%	12.223%
24	5.832	1395	1397	1402	rBV	181	113	0.02%	0.003%
25	6.250	1513	1527	1546	rBV	167782	315369	67.12%	8.204%
26	6.362	1560	1562	1565	rBB2	272	153	0.03%	0.004%
27	6.542	1609	1618	1632	rBB2	7960	14618	3.11%	0.380%
28	6.693	1651	1665	1683	rBV	106422	205671	43.77%	5.350%
29	6.864	1715	1718	1722	rBB	148	157	0.03%	0.004%
30	6.893	1723	1727	1730	rBV	133	135	0.03%	0.004%
31	7.568	1925	1937	1950	rBV	59147	102321	21.78%	2.662%
32	7.677	1968	1971	1972	rBV	223	117	0.02%	0.003%
33	7.899	2027	2040	2054	rBV	215208	365675	77.83%	9.513%
34	7.970	2057	2062	2073	rVV2	3453	5343	1.14%	0.139%
35	8.012	2073	2075	2079	rVB	273	151	0.03%	0.004%
36	8.179	2117	2127	2140	rVV	41570	70149	14.93%	1.825%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046517.D
 Acq On : 20 Dec 2021 18:00
 Operator : SY/MD
 Sample : M5153-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.227	2140	2142	2147	rVV	540	430	0.09%	0.011%
38	8.266	2151	2154	2155	rVV	230	131	0.03%	0.003%
39	8.314	2168	2169	2172	rBV	218	117	0.02%	0.003%
40	8.478	2210	2220	2225	rBV3	1249	2069	0.44%	0.054%
41	8.636	2257	2269	2292	rBV	141413	242394	51.59%	6.306%
42	8.751	2300	2305	2309	rVB2	298	361	0.08%	0.009%
43	8.787	2309	2316	2323	rBV2	1239	1641	0.35%	0.043%
44	8.854	2334	2337	2340	rBV	153	144	0.03%	0.004%
45	8.915	2352	2356	2359	rBV	148	167	0.04%	0.004%
46	9.099	2410	2413	2416	rBV	130	135	0.03%	0.004%
47	9.179	2435	2438	2441	rBV	146	146	0.03%	0.004%
48	9.417	2500	2512	2532	rBV	251024	408547	86.95%	10.628%
49	9.565	2556	2558	2563	rVB	255	215	0.05%	0.006%
50	9.697	2593	2599	2602	rVV2	451	437	0.09%	0.011%
51	9.758	2615	2618	2621	rBB	142	121	0.03%	0.003%
52	9.918	2664	2668	2670	rBV	180	178	0.04%	0.005%
53	9.999	2689	2693	2697	rBB	128	134	0.03%	0.003%
54	10.031	2698	2703	2706	rBB	149	177	0.04%	0.005%
55	10.102	2722	2725	2728	rVB2	244	195	0.04%	0.005%
56	10.140	2734	2737	2739	rBV	158	128	0.03%	0.003%
57	10.195	2751	2754	2761	rVB	136	156	0.03%	0.004%
58	10.565	2865	2869	2872	rBV	159	184	0.04%	0.005%
59	10.674	2897	2903	2908	rBV2	522	561	0.12%	0.015%
60	10.758	2917	2929	2945	rBV	155515	247846	52.75%	6.448%
61	10.893	2963	2971	2982	rVB3	1125	2058	0.44%	0.054%
62	10.941	2982	2986	2987	rBV	143	129	0.03%	0.003%
63	11.015	3006	3009	3013	rVB	170	158	0.03%	0.004%
64	11.037	3014	3016	3019	rBV	171	141	0.03%	0.004%
65	11.121	3039	3042	3047	rBV	155	214	0.05%	0.006%
66	11.188	3060	3063	3066	rBV	168	163	0.03%	0.004%
67	11.291	3091	3095	3097	rBV	179	173	0.04%	0.005%
68	11.349	3109	3113	3115	rBV	147	146	0.03%	0.004%
69	11.365	3116	3118	3121	rVB	175	112	0.02%	0.003%
70	11.401	3126	3129	3131	rBV	146	126	0.03%	0.003%
71	11.468	3143	3150	3157	rVB3	541	724	0.15%	0.019%
72	11.594	3184	3189	3192	rBV	160	182	0.04%	0.005%
73	11.693	3215	3220	3223	rBV	385	295	0.06%	0.008%
74	11.812	3245	3257	3278	rBV	266094	408277	86.89%	10.621%
75	11.909	3284	3287	3290	rBV	182	183	0.04%	0.005%
76	11.970	3303	3306	3313	rVB	440	427	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046517.D
 Acq On : 20 Dec 2021 18:00
 Operator : SY/MD
 Sample : M5153-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.063	3328	3335	3345	rBV3	2263	3538	0.75%	0.092%
78	12.192	3363	3375	3396	rBB	213238	339310	72.22%	8.827%
79	12.491	3465	3468	3471	rBV	184	185	0.04%	0.005%
80	12.552	3484	3487	3493	rBV	112	129	0.03%	0.003%
81	12.600	3498	3502	3504	rBV	235	197	0.04%	0.005%
82	12.770	3550	3555	3561	rBV	409	484	0.10%	0.013%
83	12.848	3576	3579	3584	rBV	135	130	0.03%	0.003%
84	12.889	3586	3592	3598	rVB3	1733	1947	0.41%	0.051%
85	13.214	3687	3693	3697	rVB3	624	653	0.14%	0.017%
86	14.079	3957	3962	3963	rBV	263	199	0.04%	0.005%
87	14.857	4200	4204	4206	rBV	151	115	0.02%	0.003%
88	15.246	4319	4325	4327	rBV	135	152	0.03%	0.004%
89	15.359	4356	4360	4363	rBV	229	152	0.03%	0.004%
90	15.391	4366	4370	4374	rBV	177	173	0.04%	0.005%
91	15.465	4390	4393	4397	rBV	151	139	0.03%	0.004%
92	15.545	4412	4418	4423	rBV2	210	284	0.06%	0.007%
93	15.587	4426	4431	4434	rBV	244	237	0.05%	0.006%
94	15.667	4453	4456	4461	rBV	174	202	0.04%	0.005%
95	15.819	4496	4503	4504	rBV	211	250	0.05%	0.007%
96	15.876	4518	4521	4524	rBV2	256	230	0.05%	0.006%
97	15.905	4527	4530	4534	rBV	226	255	0.05%	0.007%
98	15.966	4547	4549	4552	rBV	191	161	0.03%	0.004%
99	16.417	4687	4689	4692	rBV2	213	147	0.03%	0.004%
100	16.892	4831	4837	4840	rBV2	530	527	0.11%	0.014%




Sum of corrected areas: 3844047

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046517.D
Acq On : 20 Dec 2021 18:00
Operator : SY/MD
Sample : M5153-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

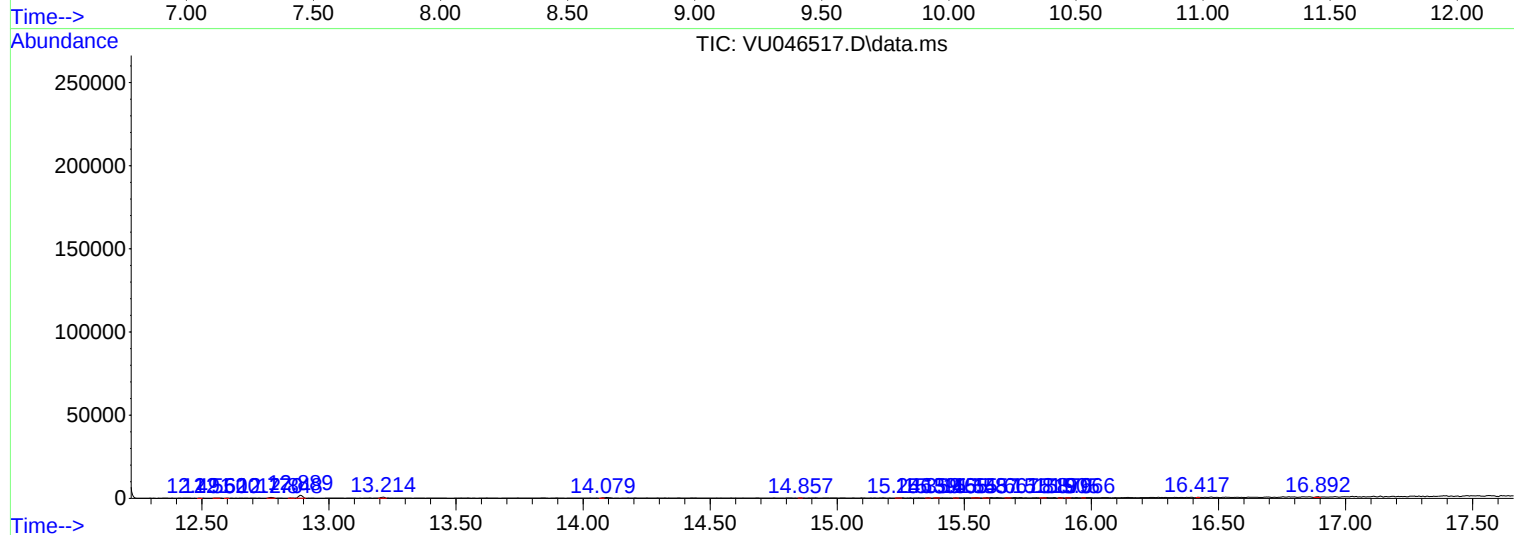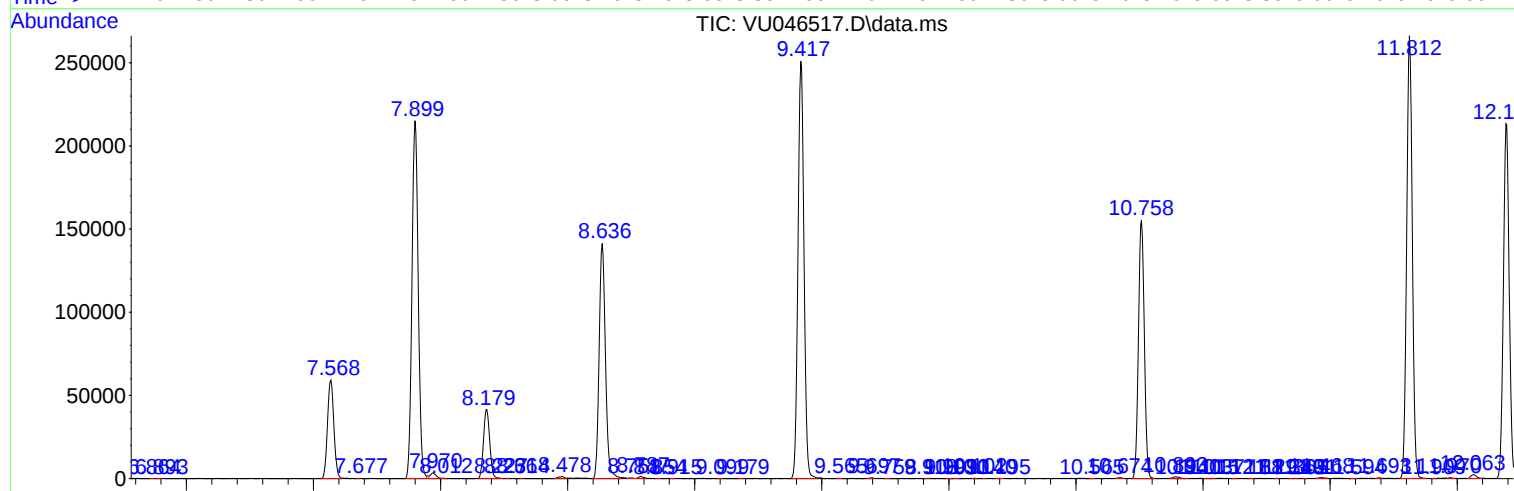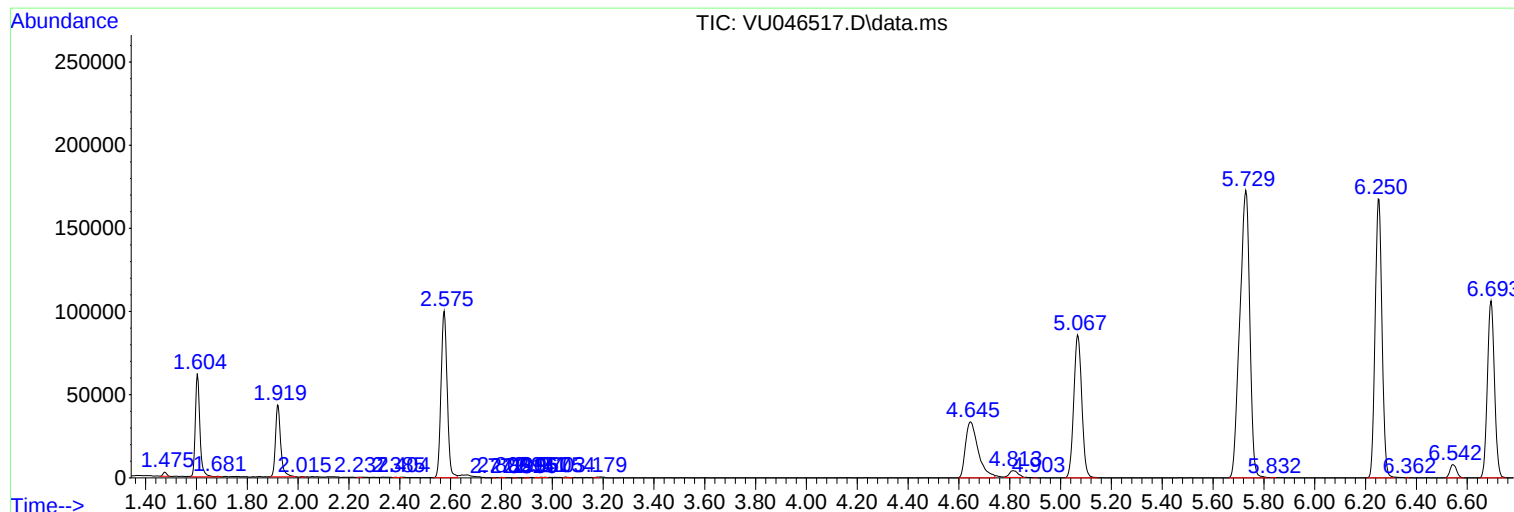

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046517.D
Acq On : 20 Dec 2021 18:00
Operator : SY/MD
Sample : M5153-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046517.D
Acq On : 20 Dec 2021 18:00
Operator : SY/MD
Sample : M5153-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------