

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046518.D
 Acq On : 20 Dec 2021 18:22
 Operator : SY/MD
 Sample : M5154-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	37	42	52	rVB2	2251	2440	0.51%	0.063%
2	1.604	74	82	102	rVB	62110	74390	15.68%	1.926%
3	1.919	171	180	201	rBV	43406	62963	13.28%	1.630%
4	2.073	226	228	231	rBV	232	117	0.02%	0.003%
5	2.240	276	280	284	rBV2	239	203	0.04%	0.005%
6	2.369	316	320	322	rBV	185	125	0.03%	0.003%
7	2.424	329	337	340	rBV2	218	354	0.07%	0.009%
8	2.575	371	384	402	rBV	102028	168407	35.51%	4.361%
9	2.793	450	452	454	rBB	226	106	0.02%	0.003%
10	2.864	471	474	476	rBV	182	121	0.03%	0.003%
11	2.970	498	507	510	rBV2	377	552	0.12%	0.014%
12	3.044	529	530	535	rVB2	295	175	0.04%	0.005%
13	3.099	543	547	549	rBV	141	123	0.03%	0.003%
14	3.125	553	555	559	rVB	255	138	0.03%	0.004%
15	3.192	566	576	588	rVB4	1872	4271	0.90%	0.111%
16	4.642	1013	1027	1069	rBV2	34377	118160	24.91%	3.060%
17	4.816	1072	1081	1097	rVB2	4359	10005	2.11%	0.259%
18	5.067	1144	1159	1189	rBB	87316	190773	40.22%	4.940%
19	5.729	1343	1365	1386	rBV2	177655	474293	100.00%	12.282%
20	5.877	1408	1411	1412	rBV	206	102	0.02%	0.003%
21	6.250	1513	1527	1550	rBV	166761	313270	66.05%	8.112%
22	6.546	1609	1619	1629	rBB3	5891	9846	2.08%	0.255%
23	6.694	1652	1665	1684	rBB	109004	210077	44.29%	5.440%
24	6.761	1684	1686	1689	rBB	136	98	0.02%	0.003%
25	7.041	1770	1773	1775	rBB	245	126	0.03%	0.003%
26	7.108	1791	1794	1797	rBV	119	105	0.02%	0.003%
27	7.189	1816	1819	1821	rBB	232	132	0.03%	0.003%
28	7.568	1925	1937	1957	rBB	59776	104318	21.99%	2.701%
29	7.899	2027	2040	2055	rBV	217117	370993	78.22%	9.607%
30	7.970	2058	2062	2071	rVB3	3113	4595	0.97%	0.119%
31	8.179	2117	2127	2142	rBV	42853	69906	14.74%	1.810%
32	8.250	2146	2149	2151	rBV	155	128	0.03%	0.003%
33	8.472	2210	2218	2223	rBV	1313	1727	0.36%	0.045%
34	8.552	2241	2243	2247	rVB2	219	137	0.03%	0.004%
35	8.636	2257	2269	2295	rBV	139197	238827	50.35%	6.185%
36	8.787	2310	2316	2323	rBV	985	1246	0.26%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046518.D
 Acq On : 20 Dec 2021 18:22
 Operator : SY/MD
 Sample : M5154-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.864	2337	2340	2342	rBV	128	111	0.02%	0.003%
38	8.944	2362	2365	2368	rBV	129	137	0.03%	0.004%
39	9.038	2390	2394	2399	rBV	161	232	0.05%	0.006%
40	9.141	2423	2426	2428	rBV	135	114	0.02%	0.003%
41	9.224	2448	2452	2454	rBV	149	149	0.03%	0.004%
42	9.327	2480	2484	2485	rBV	120	107	0.02%	0.003%
43	9.417	2500	2512	2530	rBV	249816	409292	86.30%	10.599%
44	9.546	2549	2552	2557	rBB	142	143	0.03%	0.004%
45	9.575	2558	2561	2563	rBB2	220	146	0.03%	0.004%
46	9.694	2593	2598	2604	rVB2	456	556	0.12%	0.014%
47	9.806	2630	2633	2637	rBB	133	140	0.03%	0.004%
48	9.854	2646	2648	2650	rBV	146	99	0.02%	0.003%
49	9.906	2661	2664	2668	rBB	173	172	0.04%	0.004%
50	9.938	2672	2674	2676	rBV	164	113	0.02%	0.003%
51	9.980	2684	2687	2690	rBB	172	134	0.03%	0.003%
52	10.083	2715	2719	2722	rBB	144	125	0.03%	0.003%
53	10.099	2722	2724	2727	rBB	254	141	0.03%	0.004%
54	10.131	2728	2734	2736	rBV	176	192	0.04%	0.005%
55	10.169	2744	2746	2749	rBV	146	127	0.03%	0.003%
56	10.221	2758	2762	2764	rBB	146	121	0.03%	0.003%
57	10.276	2777	2779	2782	rBB	153	99	0.02%	0.003%
58	10.330	2794	2796	2801	rBV	145	175	0.04%	0.005%
59	10.404	2815	2819	2821	rBV	167	162	0.03%	0.004%
60	10.671	2896	2902	2908	rBB3	737	903	0.19%	0.023%
61	10.758	2917	2929	2946	rBV	159887	248413	52.38%	6.433%
62	10.890	2962	2970	2972	rBV3	1299	1309	0.28%	0.034%
63	11.205	3065	3068	3072	rBV	170	194	0.04%	0.005%
64	11.295	3093	3096	3098	rBV	138	114	0.02%	0.003%
65	11.372	3115	3120	3123	rBV	169	230	0.05%	0.006%
66	11.456	3141	3146	3148	rBV2	662	589	0.12%	0.015%
67	11.629	3197	3200	3203	rBV	147	154	0.03%	0.004%
68	11.684	3214	3217	3219	rBV	195	131	0.03%	0.003%
69	11.697	3219	3221	3224	rVB	268	151	0.03%	0.004%
70	11.732	3230	3232	3236	rVB	181	124	0.03%	0.003%
71	11.755	3237	3239	3240	rBV	219	106	0.02%	0.003%
72	11.812	3245	3257	3271	rBV	261401	408505	86.13%	10.579%
73	11.906	3281	3286	3290	rBV	153	199	0.04%	0.005%
74	11.947	3295	3299	3301	rBV	166	145	0.03%	0.004%
75	12.063	3326	3335	3346	rBV3	2236	3599	0.76%	0.093%
76	12.192	3358	3375	3395	rBV	216357	344898	72.72%	8.931%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046518.D
 Acq On : 20 Dec 2021 18:22
 Operator : SY/MD
 Sample : M5154-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.343	3414	3422	3427	rBV	182	370	0.08%	0.010%
78	12.391	3434	3437	3439	rBV	198	165	0.03%	0.004%
79	12.771	3551	3555	3561	rVB	365	402	0.08%	0.010%
80	12.890	3587	3592	3601	rVB4	873	986	0.21%	0.026%
81	13.124	3661	3665	3670	rBV	128	119	0.03%	0.003%
82	13.218	3688	3694	3696	rVB2	450	432	0.09%	0.011%
83	13.552	3795	3798	3807	rVB	123	156	0.03%	0.004%
84	14.092	3961	3966	3972	rVB	315	378	0.08%	0.010%
85	14.722	4159	4162	4168	rVB	228	155	0.03%	0.004%
86	14.796	4182	4185	4190	rBV	131	104	0.02%	0.003%
87	15.272	4330	4333	4338	rVB	165	131	0.03%	0.003%
88	15.298	4338	4341	4345	rBV	169	128	0.03%	0.003%
89	15.375	4362	4365	4368	rBV	144	98	0.02%	0.003%
90	15.471	4391	4395	4397	rBV2	241	169	0.04%	0.004%
91	15.529	4411	4413	4418	rVB2	241	172	0.04%	0.004%
92	15.561	4419	4423	4428	rBV2	266	350	0.07%	0.009%
93	15.610	4436	4438	4441	rBV2	188	119	0.03%	0.003%
94	15.684	4458	4461	4463	rBV	170	123	0.03%	0.003%
95	15.700	4463	4466	4468	rBV	139	111	0.02%	0.003%
96	15.713	4468	4470	4473	rBV2	176	104	0.02%	0.003%
97	16.504	4713	4716	4717	rBV	220	113	0.02%	0.003%
98	16.536	4724	4726	4730	rBV2	252	182	0.04%	0.005%
99	16.787	4803	4804	4808	rVB2	323	204	0.04%	0.005%
100	16.944	4850	4853	4860	rVB3	417	446	0.09%	0.012%




Sum of corrected areas: 3861617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046518.D
Acq On : 20 Dec 2021 18:22
Operator : SY/MD
Sample : M5154-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

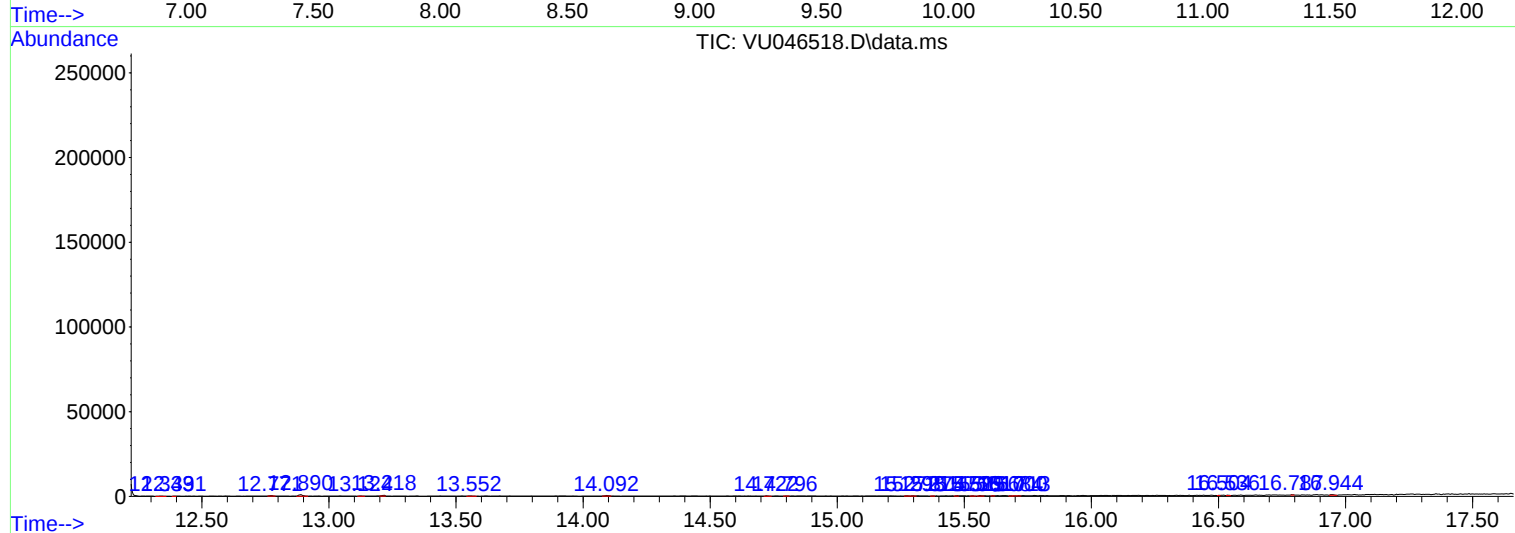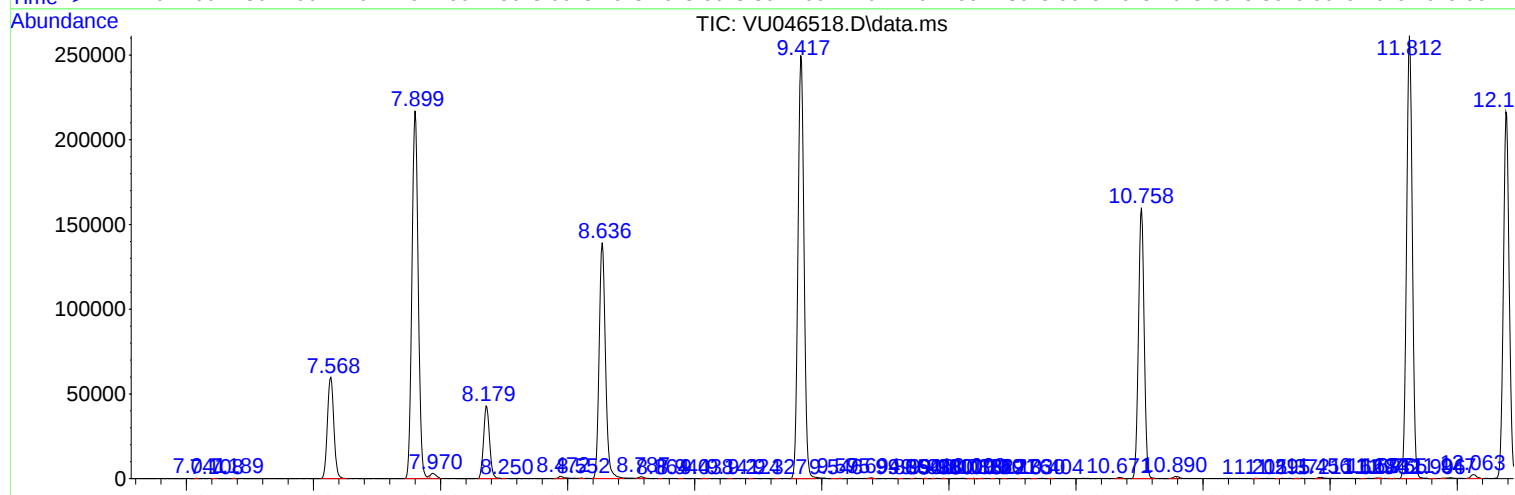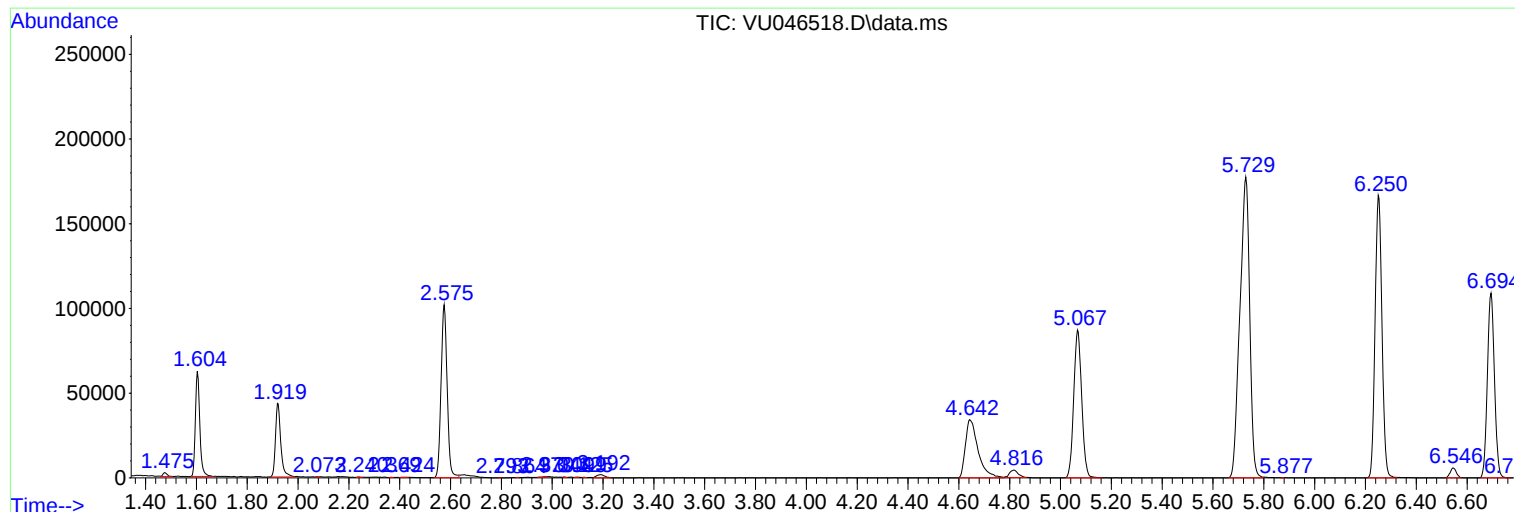

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046518.D
Acq On : 20 Dec 2021 18:22
Operator : SY/MD
Sample : M5154-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046518.D
Acq On : 20 Dec 2021 18:22
Operator : SY/MD
Sample : M5154-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------