

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046519.D
 Acq On : 20 Dec 2021 18:45
 Operator : SY/MD
 Sample : M5121-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	104	rBV	58348	70758	13.88%	1.739%
2	1.871	160	165	169	rBV2	337	396	0.08%	0.010%
3	1.919	172	180	201	rVV	44098	64332	12.62%	1.581%
4	2.041	215	218	222	rBV	286	263	0.05%	0.006%
5	2.311	299	302	303	rBV	187	108	0.02%	0.003%
6	2.369	317	320	322	rBV	213	105	0.02%	0.003%
7	2.417	334	335	342	rVB	214	111	0.02%	0.003%
8	2.575	369	384	420	rVV	104501	174525	34.24%	4.288%
9	2.723	426	430	431	rBV	238	147	0.03%	0.004%
10	2.761	440	442	445	rBB	134	96	0.02%	0.002%
11	2.803	452	455	457	rBB	250	117	0.02%	0.003%
12	2.858	471	472	475	rBV	251	129	0.03%	0.003%
13	2.890	480	482	484	rVB	246	117	0.02%	0.003%
14	2.916	487	490	493	rBB	144	120	0.02%	0.003%
15	3.054	527	533	541	rBB	816	1234	0.24%	0.030%
16	3.198	575	578	581	rBB	136	113	0.02%	0.003%
17	4.642	1013	1027	1062	rBV	38001	126910	24.90%	3.118%
18	4.867	1095	1097	1100	rBB	168	113	0.02%	0.003%
19	4.903	1104	1108	1112	rBB2	253	207	0.04%	0.005%
20	5.067	1144	1159	1180	rBV	94433	205585	40.33%	5.052%
21	5.729	1344	1365	1390	rBV2	188193	509763	100.00%	12.526%
22	5.861	1403	1406	1410	rBB	153	148	0.03%	0.004%
23	6.250	1514	1527	1545	rBV	168899	317952	62.37%	7.813%
24	6.546	1610	1619	1630	rBB4	5077	8523	1.67%	0.209%
25	6.694	1652	1665	1681	rBV	116648	226211	44.38%	5.558%
26	6.806	1697	1700	1703	rBV	252	229	0.04%	0.006%
27	7.189	1815	1819	1820	rBB	210	117	0.02%	0.003%
28	7.510	1917	1919	1922	rBB	169	111	0.02%	0.003%
29	7.568	1923	1937	1953	rBV	64161	113344	22.23%	2.785%
30	7.726	1984	1986	1989	rBV	142	116	0.02%	0.003%
31	7.899	2026	2040	2056	rBV	231746	396810	77.84%	9.750%
32	8.179	2117	2127	2142	rVV2	45213	75857	14.88%	1.864%
33	8.266	2151	2154	2156	rBB2	257	142	0.03%	0.003%
34	8.362	2181	2184	2186	rBB	143	99	0.02%	0.002%
35	8.391	2190	2193	2195	rBB	139	97	0.02%	0.002%
36	8.462	2211	2215	2216	rBV	355	257	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046519.D
 Acq On : 20 Dec 2021 18:45
 Operator : SY/MD
 Sample : M5121-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.636	2256	2269	2298	rBV	157799	274002	53.75%	6.733%
38	8.822	2324	2327	2331	rVB	187	184	0.04%	0.005%
39	8.883	2344	2346	2349	rBV	124	115	0.02%	0.003%
40	8.915	2352	2356	2359	rBV	119	130	0.03%	0.003%
41	9.025	2387	2390	2392	rBB	158	108	0.02%	0.003%
42	9.160	2429	2432	2434	rBV	143	125	0.02%	0.003%
43	9.243	2453	2458	2461	rBB	139	169	0.03%	0.004%
44	9.417	2500	2512	2532	rBV	251481	417056	81.81%	10.248%
45	9.684	2592	2595	2597	rBV2	315	249	0.05%	0.006%
46	9.745	2612	2614	2617	rBB	148	101	0.02%	0.002%
47	9.886	2655	2658	2661	rBB	133	113	0.02%	0.003%
48	9.931	2670	2672	2674	rBV	151	103	0.02%	0.003%
49	9.957	2677	2680	2681	rVV	156	112	0.02%	0.003%
50	9.989	2685	2690	2693	rBB	152	153	0.03%	0.004%
51	10.172	2745	2747	2750	rBB	183	120	0.02%	0.003%
52	10.250	2769	2771	2774	rBB	155	101	0.02%	0.002%
53	10.407	2816	2820	2823	rBB	131	115	0.02%	0.003%
54	10.426	2823	2826	2829	rBB	144	124	0.02%	0.003%
55	10.462	2834	2837	2839	rBV	154	126	0.02%	0.003%
56	10.478	2840	2842	2845	rVB2	255	151	0.03%	0.004%
57	10.526	2854	2857	2860	rBB	143	120	0.02%	0.003%
58	10.613	2880	2884	2888	rBV	168	217	0.04%	0.005%
59	10.671	2894	2902	2906	rBV3	551	733	0.14%	0.018%
60	10.758	2916	2929	2944	rBB	174753	280028	54.93%	6.881%
61	10.819	2945	2948	2950	rBV	150	132	0.03%	0.003%
62	10.864	2960	2962	2966	rVB	247	161	0.03%	0.004%
63	10.896	2967	2972	2978	rBV2	496	534	0.10%	0.013%
64	11.025	3010	3012	3016	rBB	141	97	0.02%	0.002%
65	11.166	3053	3056	3059	rBB	172	134	0.03%	0.003%
66	11.259	3083	3085	3086	rBV	172	93	0.02%	0.002%
67	11.311	3099	3101	3105	rBB	149	125	0.02%	0.003%
68	11.340	3106	3110	3114	rBV	144	196	0.04%	0.005%
69	11.417	3131	3134	3136	rBV	188	147	0.03%	0.004%
70	11.433	3136	3139	3142	rVV	150	142	0.03%	0.003%
71	11.452	3142	3145	3146	rVV	288	170	0.03%	0.004%
72	11.468	3148	3150	3158	rVB2	638	577	0.11%	0.014%
73	11.507	3159	3162	3164	rBV	157	136	0.03%	0.003%
74	11.549	3173	3175	3177	rBV	127	92	0.02%	0.002%
75	11.812	3245	3257	3276	rVB	270202	417274	81.86%	10.253%
76	11.883	3276	3279	3280	rBV	241	137	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
 Data File : VU046519.D
 Acq On : 20 Dec 2021 18:45
 Operator : SY/MD
 Sample : M5121-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.893	3280	3282	3286	rVB2	151	94	0.02%	0.002%
78	11.938	3292	3296	3301	rBV2	249	317	0.06%	0.008%
79	12.063	3329	3335	3339	rBV	79	105	0.02%	0.003%
80	12.192	3363	3375	3396	rBV	237228	375970	73.75%	9.238%
81	12.385	3429	3435	3440	rBV	149	270	0.05%	0.007%
82	12.436	3447	3451	3454	rBV	228	229	0.04%	0.006%
83	12.507	3469	3473	3481	rBV	91	113	0.02%	0.003%
84	13.060	3639	3645	3648	rBV	108	127	0.02%	0.003%
85	13.639	3820	3825	3827	rBV	90	96	0.02%	0.002%
86	13.922	3910	3913	3915	rBV	187	120	0.02%	0.003%
87	14.610	4123	4127	4128	rBV	168	122	0.02%	0.003%
88	14.706	4152	4157	4164	rBV	182	230	0.05%	0.006%
89	15.082	4272	4274	4278	rBV	145	138	0.03%	0.003%
90	15.397	4369	4372	4377	rVB	210	132	0.03%	0.003%
91	15.497	4400	4403	4406	rBV2	182	122	0.02%	0.003%
92	15.555	4415	4421	4424	rVB2	208	232	0.05%	0.006%
93	15.574	4424	4427	4429	rBV2	138	110	0.02%	0.003%
94	15.648	4448	4450	4453	rVB	173	115	0.02%	0.003%
95	15.783	4490	4492	4495	rBV	158	126	0.02%	0.003%
96	15.844	4508	4511	4514	rVB2	200	166	0.03%	0.004%
97	15.860	4514	4516	4519	rBV	199	143	0.03%	0.004%
98	15.896	4524	4527	4530	rBV2	239	210	0.04%	0.005%
99	16.847	4820	4823	4824	rBV	288	166	0.03%	0.004%
100	17.439	5005	5007	5010	rBV	482	326	0.06%	0.008%




Sum of corrected areas: 4069743

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046519.D
Acq On : 20 Dec 2021 18:45
Operator : SY/MD
Sample : M5121-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

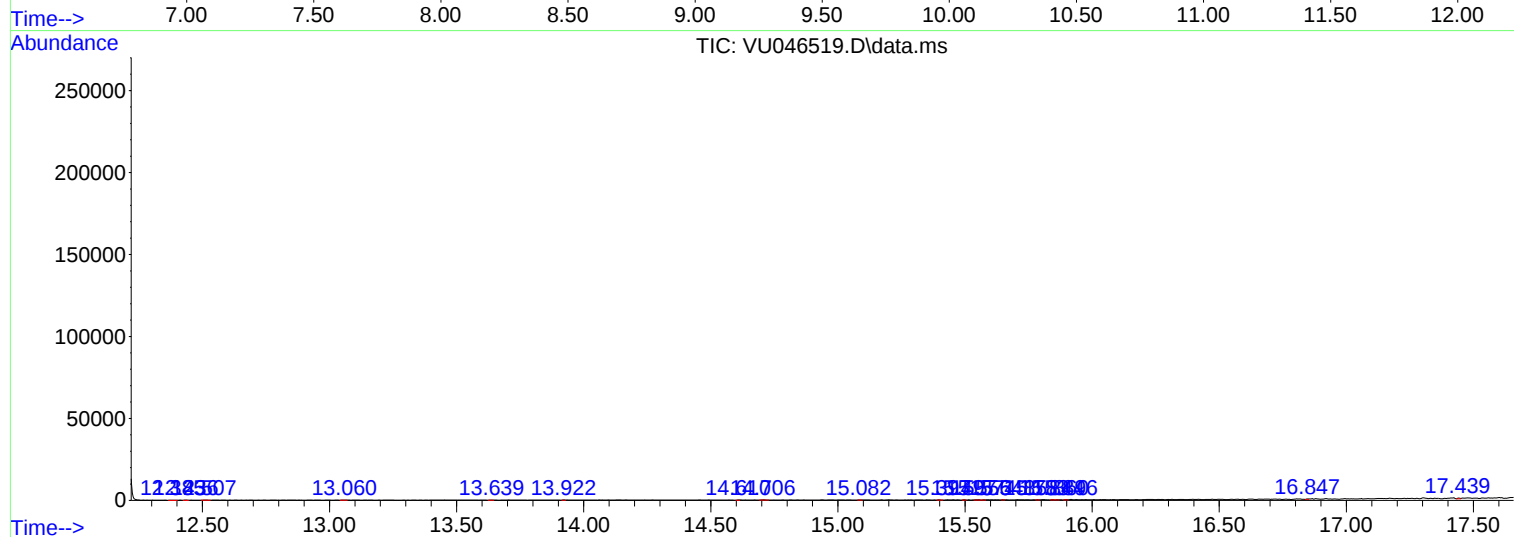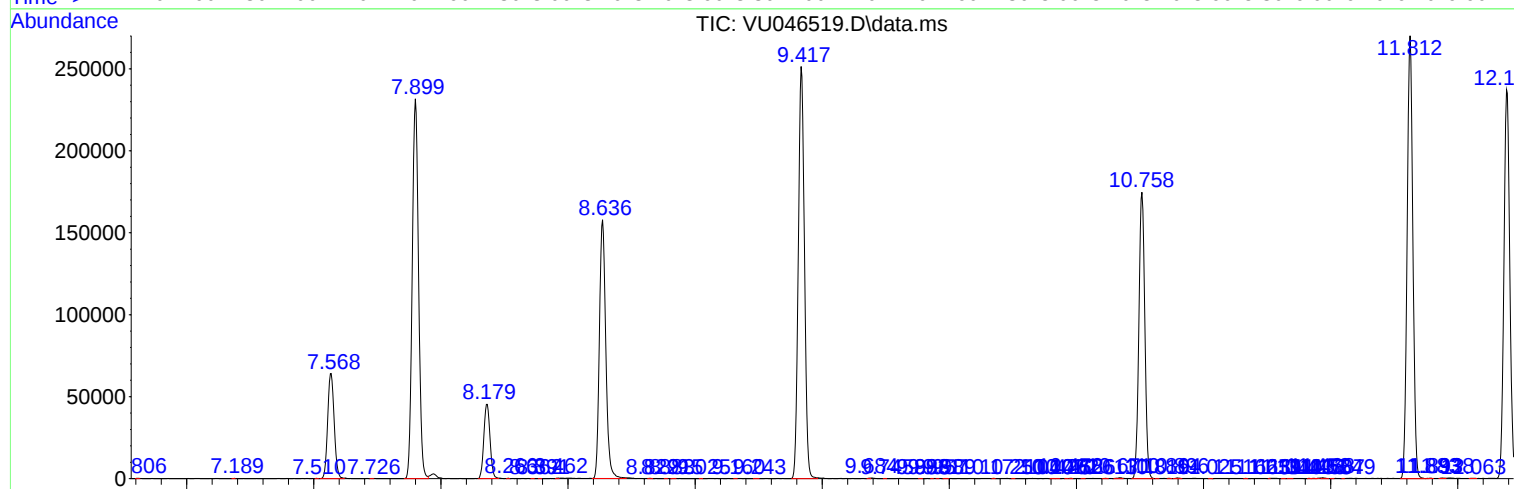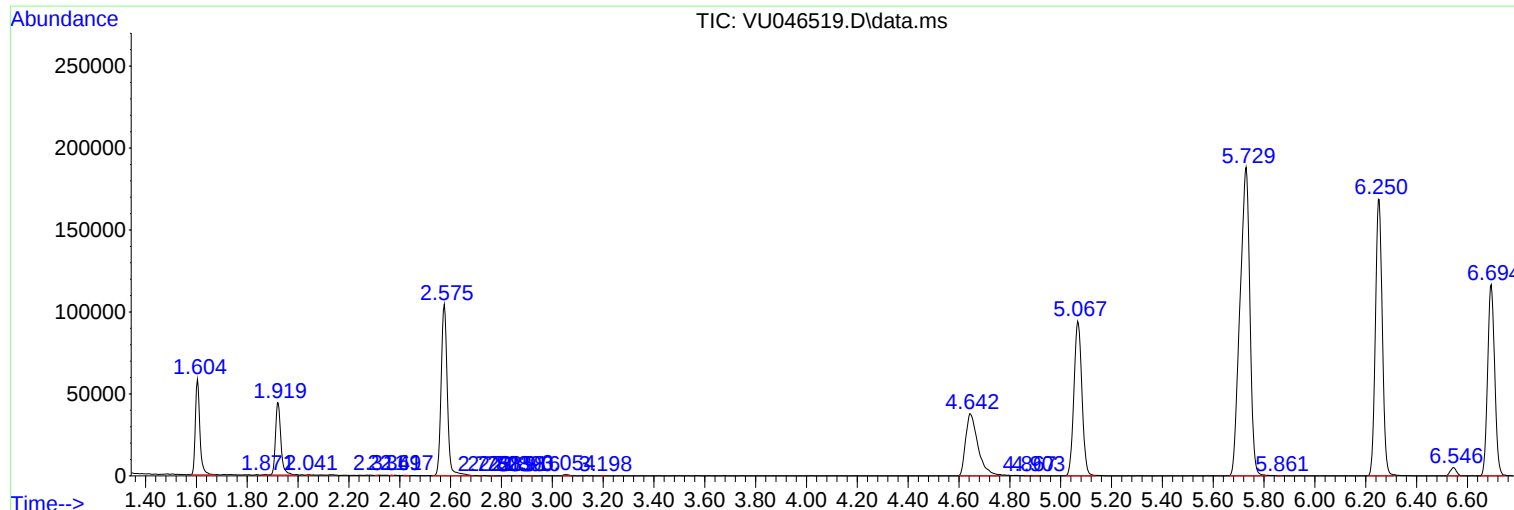

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046519.D
Acq On : 20 Dec 2021 18:45
Operator : SY/MD
Sample : M5121-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046519.D
Acq On : 20 Dec 2021 18:45
Operator : SY/MD
Sample : M5121-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc