


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122021\
Data File : VU046503.D
Acq On : 20 Dec 2021 10:11
Operator : SY/MD
Sample : BFB036
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB036

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis
Last Update : Mon Dec 20 00:25:10 2021

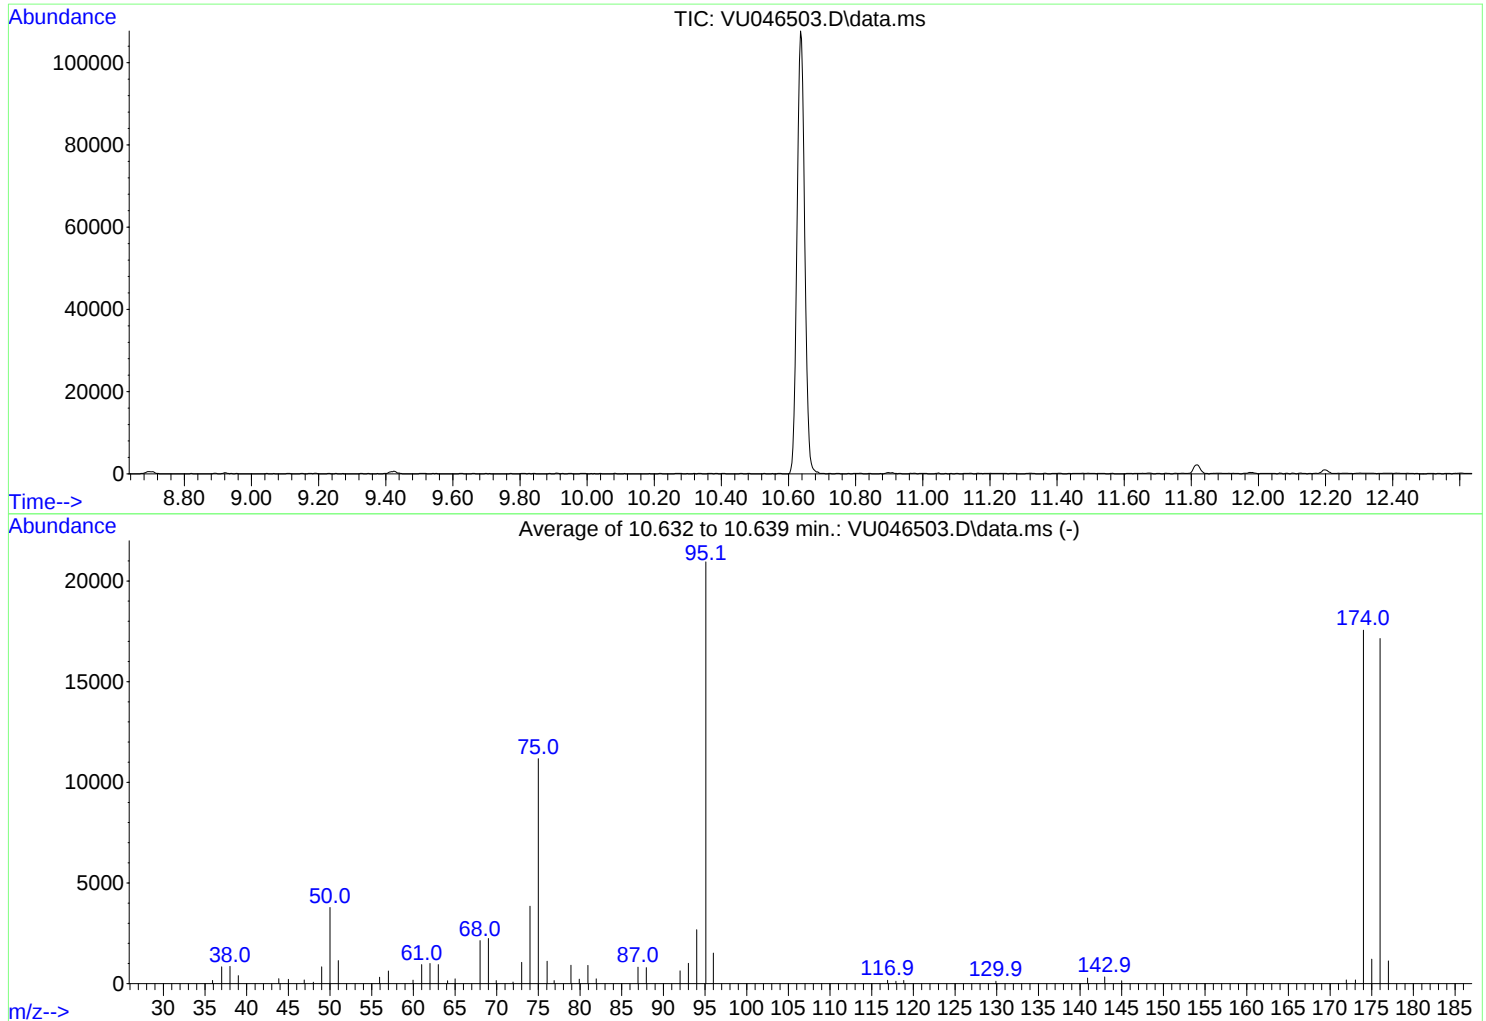

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	3780	PASS
75	95	30	80	53.3	11175	PASS
95	95	100	100	100.0	20952	PASS
96	95	5	9	7.2	1519	PASS
173	174	0.00	2	1.0	183	PASS
174	95	50	120	83.8	17555	PASS
175	174	5	9	6.9	1218	PASS
176	174	95	101	97.7	17143	PASS
177	176	5	9	6.6	1127	PASS

m/z	Abundance
35.90	161.0
37.00	893.0
38.00	790.0
39.00	402.0
43.80	236.0
45.00	203.0
46.90	182.0
48.00	109.0
49.00	806.0
50.00	3697.0
51.00	1091.0
56.00	331.0
57.00	610.0
59.90	136.0
61.00	936.0
62.00	961.0
63.00	985.0
64.10	162.0
65.00	233.0
68.00	2040.0
69.00	2149.0
69.90	134.0
72.00	126.0
73.00	1011.0
74.00	3691.0
75.00	10582.0
76.10	1146.0
76.90	166.0
78.90	897.0
79.90	216.0
80.90	908.0
82.00	232.0
87.00	708.0
88.00	796.0
92.00	607.0
93.00	927.0
94.00	2609.0
95.10	20088.0
96.00	1498.0
116.90	161.0
117.90	125.0
118.80	112.0
129.90	127.0
140.90	267.0
142.90	282.0
145.00	128.0
171.90	151.0
173.10	173.0
174.00	16672.0
175.00	1187.0
176.00	16093.0
177.00	1180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.00	159.0
37.00	755.0
38.00	905.0
39.00	387.0
43.00	251.0
45.00	222.0
46.00	182.0
49.00	836.0
50.00	3739.0
51.00	1174.0
55.00	294.0
57.00	624.0
60.00	210.0
61.00	939.0
62.00	1049.0
63.00	889.0
64.10	118.0
65.00	232.0
68.00	2196.0
69.00	2250.0
70.00	163.0
73.00	1072.0
74.00	3876.0
75.00	11465.0
76.00	1058.0
76.90	139.0
78.90	891.0
79.90	236.0
81.00	887.0
81.90	231.0
86.90	899.0
87.90	781.0
92.00	664.0
93.00	1051.0
94.00	2673.0
95.10	21256.0
96.00	1498.0
116.90	165.0
117.90	120.0
118.90	198.0
129.90	111.0
140.90	280.0
143.00	389.0
145.00	151.0
172.00	216.0
173.00	192.0
174.00	17824.0
175.00	1232.0
176.00	17584.0
177.00	1029.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.00	159.0
37.00	755.0
38.00	905.0
39.00	387.0
43.00	251.0
45.00	222.0
46.00	182.0
49.00	836.0
50.00	3739.0
51.00	1174.0
55.00	294.0
57.00	624.0
60.00	210.0
61.00	939.0
62.00	1049.0
63.00	889.0
64.10	118.0
65.00	232.0
68.00	2196.0
69.00	2250.0
70.00	163.0
73.00	1072.0
74.00	3876.0
75.00	11465.0
76.00	1058.0
76.90	139.0
78.90	891.0
79.90	236.0
81.00	887.0
81.90	231.0
86.90	899.0
87.90	781.0
92.00	664.0
93.00	1051.0
94.00	2673.0
95.10	21256.0
96.00	1498.0
116.90	165.0
117.90	120.0
118.90	198.0
129.90	111.0
140.90	280.0
143.00	389.0
145.00	151.0
172.00	216.0
173.00	192.0
174.00	17824.0
175.00	1232.0
176.00	17584.0
177.00	1029.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	157.0
37.00	863.0
38.00	878.0
39.00	402.0
43.90	254.0
45.00	221.0
46.90	198.0
48.00	100.0
49.00	850.0
50.00	3904.0
51.00	1179.0
56.00	319.0
57.00	652.0
59.90	177.0
61.00	955.0
62.00	1003.0
63.00	972.0
64.10	150.0
65.00	241.0
68.00	2190.0
69.00	2324.0
70.00	159.0
71.90	113.0
73.00	1097.0
74.00	3972.0
75.00	11479.0
76.00	1136.0
76.90	160.0
78.90	953.0
79.90	224.0
81.00	935.0
81.90	244.0
87.00	843.0
88.00	810.0
92.00	646.0
93.00	1053.0
94.00	2743.0
95.10	21512.0
96.00	1562.0
116.90	177.0
117.90	125.0
118.90	158.0
129.90	120.0
140.90	289.0
142.90	336.0
145.00	149.0
172.00	174.0
173.00	185.0
174.00	18168.0
175.00	1235.0
176.00	17752.0
177.00	1171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036