
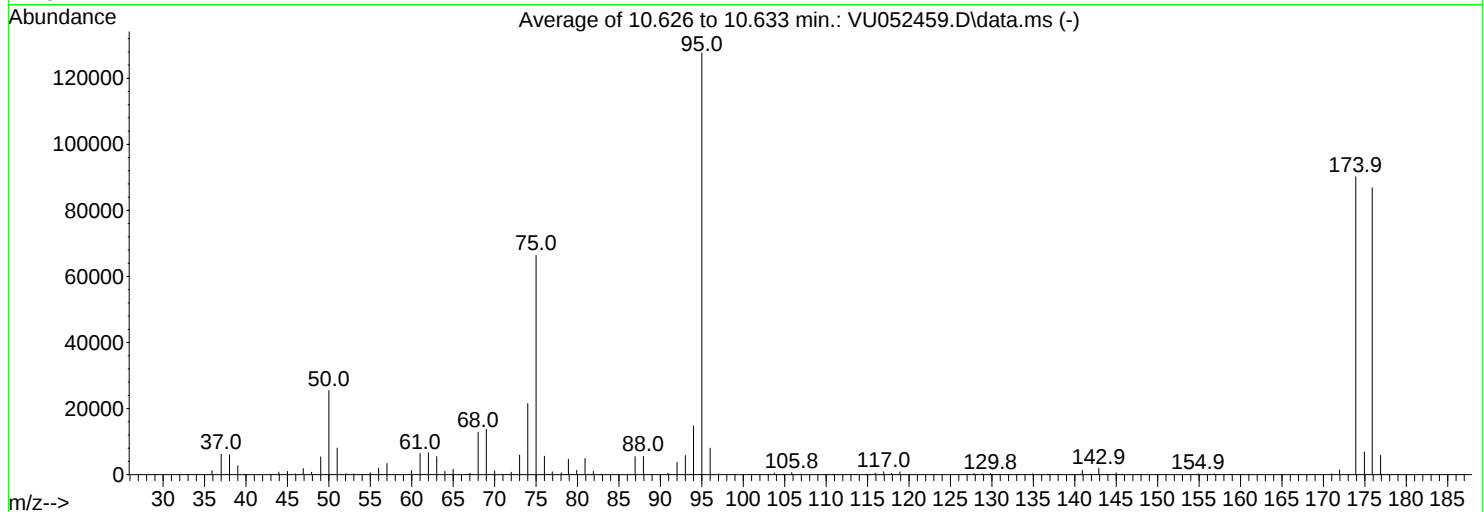


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122022\
Data File : VU052459.D
Acq On : 20 Dec 2022 14:53
Operator : JC/MD
Sample : BFB181
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB181

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 21 03:39:33 2022

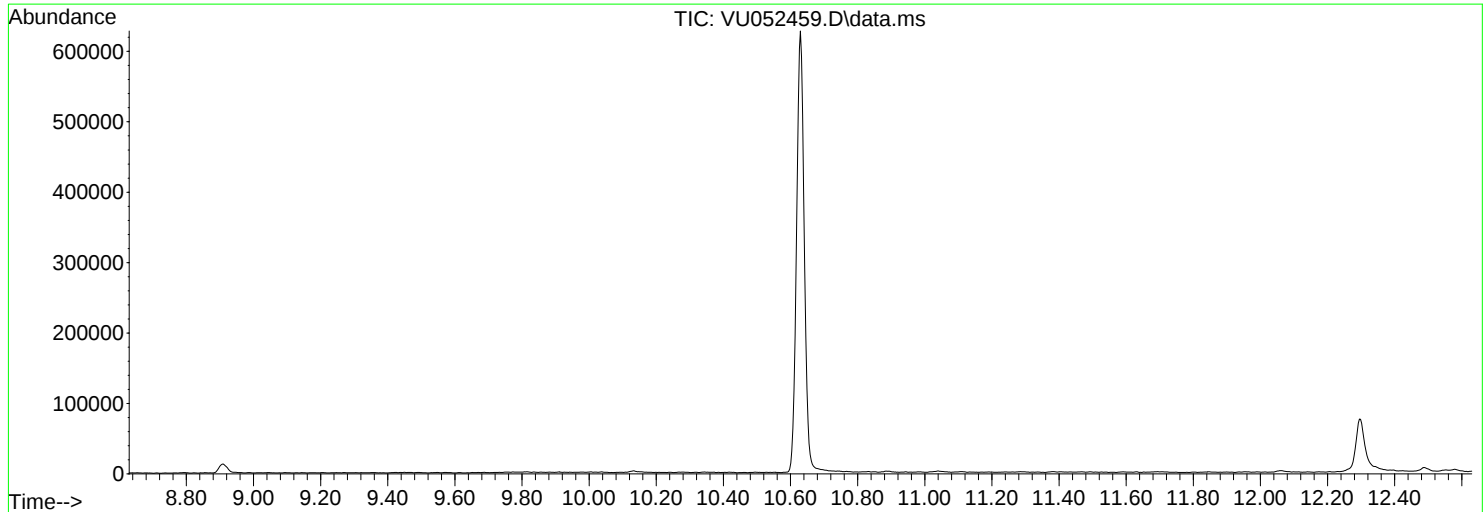

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2872

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	25427	PASS
75	95	30	80	52.0	66384	PASS
95	95	100	100	100.0	127699	PASS
96	95	5	9	6.3	8028	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	90211	PASS
175	174	5	9	7.7	6911	PASS
176	174	95	101	96.3	86853	PASS
177	176	5	9	6.8	5880	PASS

m/z	Abundance
39.90	219.0
41.10	191.0
42.90	378.0
43.90	509.0
70.90	546.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181

m/z	Abundance
35.90	1240.0
37.00	6284.0
38.00	6076.0
39.00	2774.0
39.90	412.0
40.90	217.0
43.00	481.0
44.00	1251.0
45.00	970.0
46.00	231.0
46.90	1841.0
47.90	666.0
49.00	5394.0
50.00	25856.0
51.00	8289.0
52.00	350.0
53.00	251.0
54.00	104.0
55.00	528.0
56.00	2005.0
57.00	3459.0
58.10	149.0
59.90	1179.0
61.00	6632.0
62.00	6524.0
63.00	5553.0
64.00	1017.0
65.00	1706.0
66.00	163.0
67.00	371.0
68.00	12996.0
69.00	14051.0
70.00	1117.0
71.00	741.0
72.00	727.0
73.00	5996.0
74.00	21896.0
75.00	66344.0
76.00	5600.0
76.90	891.0
78.20	636.0
78.90	4720.0
79.90	1411.0
80.90	4967.0
81.90	994.0
83.00	149.0
86.10	184.0
86.90	5630.0
88.00	5560.0
90.90	457.0
92.00	3600.0
93.00	6129.0
94.00	14813.0
95.00	126456.0
96.00	8447.0
97.10	287.0
103.80	542.0
104.80	174.0
105.90	660.0
107.00	156.0
114.90	130.0
115.90	505.0
116.90	903.0
117.90	394.0
118.90	873.0
127.80	395.0
128.90	223.0
129.90	350.0
130.80	172.0
134.90	187.0
136.80	175.0
140.90	1169.0
141.80	128.0
142.90	1783.0
143.90	188.0
145.00	642.0
145.70	200.0
148.00	145.0
149.80	135.0
154.90	254.0
156.80	206.0
158.80	142.0
160.90	159.0
171.00	277.0
172.00	1372.0
173.90	87360.0
175.00	6687.0
175.90	84416.0
176.90	5863.0
177.90	217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181

m/z	Abundance
35.90	1254.0
37.00	6424.0
38.00	6220.0
39.00	2818.0
39.90	433.0
40.90	240.0
43.00	523.0
44.00	1319.0
45.00	1028.0
45.90	241.0
46.90	1957.0
47.90	767.0
49.00	5531.0
50.00	26408.0
51.00	8301.0
52.10	330.0
53.00	252.0
54.00	107.0
55.00	583.0
56.00	2053.0
57.00	3520.0
58.10	171.0
59.90	1289.0
61.00	6623.0
62.00	6798.0
63.00	5674.0
64.00	1061.0
65.00	1728.0
66.00	162.0
67.00	443.0
68.00	13213.0
69.00	14251.0
70.00	1215.0
71.00	736.0
72.00	752.0
73.00	6080.0
74.00	22192.0
75.00	68824.0
76.00	5765.0
77.00	946.0
78.00	582.0
78.90	4789.0
79.90	1354.0
80.90	5050.0
81.90	980.0
83.00	147.0
86.00	195.0
86.90	5586.0
87.90	5722.0
90.90	480.0
92.00	3803.0
93.00	5985.0
94.00	15271.0
95.00	132352.0
96.00	8270.0
97.10	229.0
103.80	566.0
104.80	177.0
105.90	671.0
107.00	125.0
110.80	101.0
114.80	190.0
115.90	478.0
117.00	914.0
117.90	444.0
118.90	936.0
127.90	332.0
128.90	249.0
129.90	377.0
130.90	158.0
134.90	230.0
136.70	198.0
140.90	1394.0
141.90	142.0
142.90	1968.0
143.80	151.0
145.00	629.0
145.80	208.0
148.10	171.0
149.80	115.0
154.90	267.0
156.80	280.0
158.80	147.0
160.90	152.0
171.00	249.0
172.00	1429.0
173.90	93272.0
175.00	7105.0
175.90	89752.0
176.90	6098.0
177.90	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181

m/z	Abundance
35.90	1183.0
37.00	5986.0
38.00	5661.0
39.00	2563.0
39.90	466.0
40.90	251.0
43.00	536.0
44.00	1277.0
45.00	941.0
45.90	226.0
46.90	1765.0
47.90	832.0
49.00	5236.0
50.00	24016.0
51.00	7507.0
52.10	344.0
53.00	232.0
54.00	117.0
55.00	577.0
56.00	1948.0
57.00	3173.0
58.10	170.0
60.00	1337.0
61.00	6059.0
62.00	6429.0
63.00	5244.0
64.00	980.0
65.00	1544.0
66.00	131.0
67.00	469.0
68.00	12441.0
69.00	12963.0
70.00	1143.0
71.00	660.0
72.00	657.0
73.00	5724.0
74.00	20584.0
75.00	63984.0
76.00	5293.0
77.00	858.0
77.90	546.0
78.90	4427.0
79.90	1197.0
80.90	4701.0
81.90	930.0
82.90	152.0
86.00	256.0
87.00	5269.0
87.90	5343.0
90.90	447.0
92.00	3673.0
93.00	5379.0
94.00	14299.0
95.00	124288.0
96.00	7368.0
97.00	219.0
103.70	526.0
104.80	166.0
105.80	634.0
106.90	109.0
113.00	100.0
114.80	213.0
115.90	451.0
117.00	865.0
117.90	488.0
118.90	823.0
127.90	334.0
128.90	288.0
129.80	353.0
131.00	153.0
134.90	284.0
136.70	212.0
139.70	111.0
140.90	1433.0
141.90	169.0
142.90	1913.0
143.80	106.0
145.00	549.0
145.90	211.0
147.70	112.0
148.10	143.0
154.90	243.0
156.90	276.0
158.80	129.0
161.00	123.0
171.00	225.0
171.90	1387.0
173.90	90000.0
174.90	6942.0
175.90	86392.0
176.90	5679.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181