




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057117.D
Acq On : 21 Dec 2023 02:12
Operator : MD/SY
Sample : 05892-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7B01

Manual IntegrationsAPPROVED

Quant Time: Dec 21 05:02:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 21 01:34:13 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
Supervised By :Semsettin Yesilyurt 12/21/2023

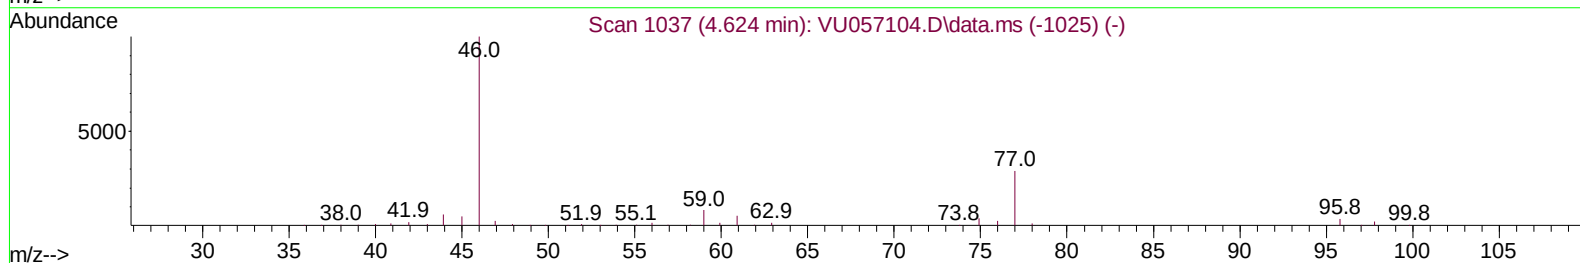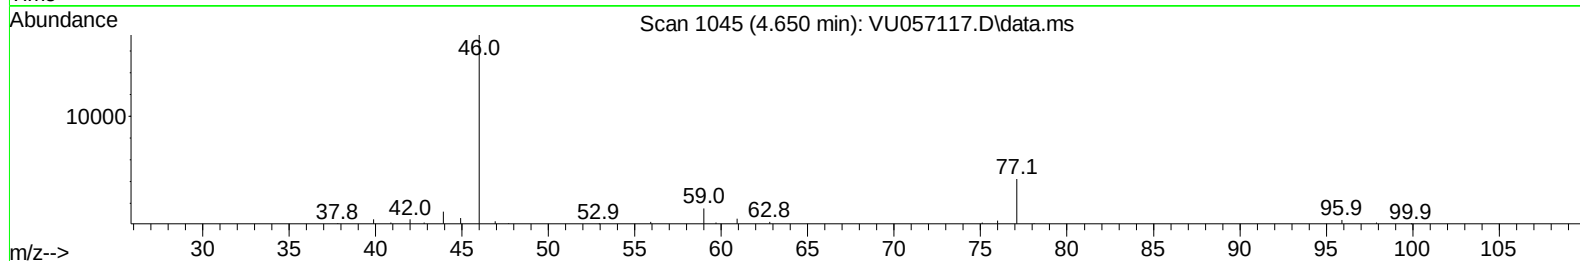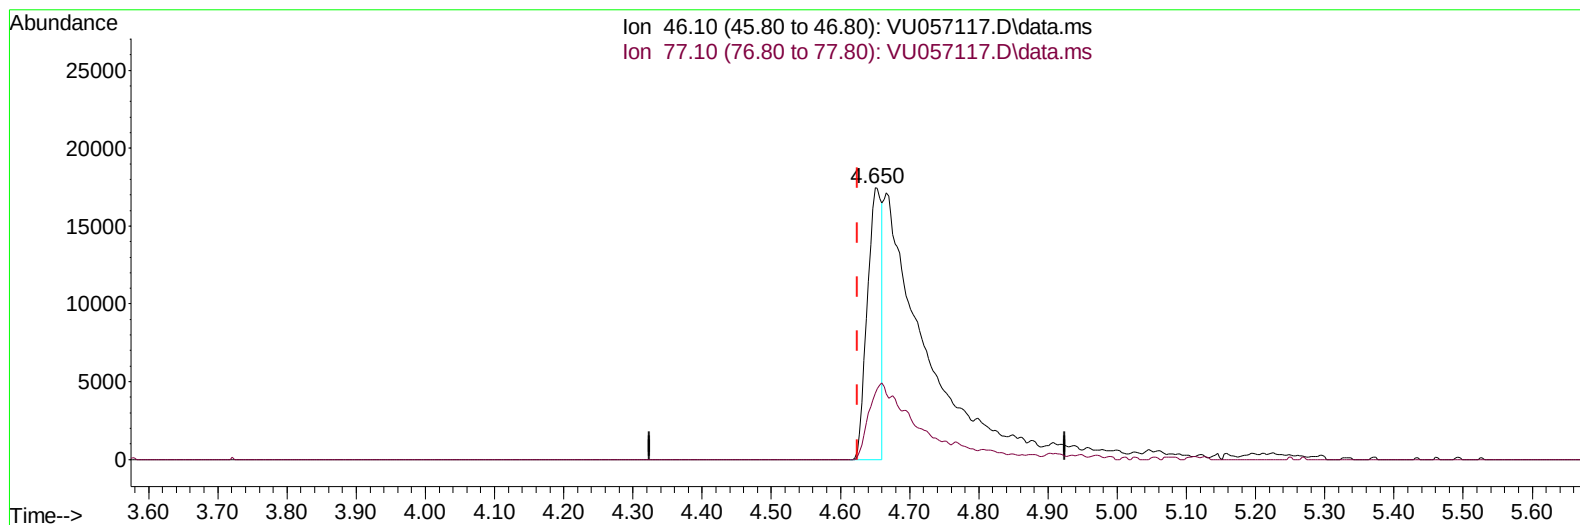

TIC: VU057117.D\data.ms

(20) 2-Butanone-d5 (S)

4.650min (+ 0.026) 8.35 ug/L

response 25222

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.70	83.42#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
 Data File : VU057117.D
 Acq On : 21 Dec 2023 02:12
 Operator : MD/SY
 Sample : 05892-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7B01

Manual IntegrationsAPPROVED

Quant Time: Dec 21 05:02:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 21 01:34:13 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

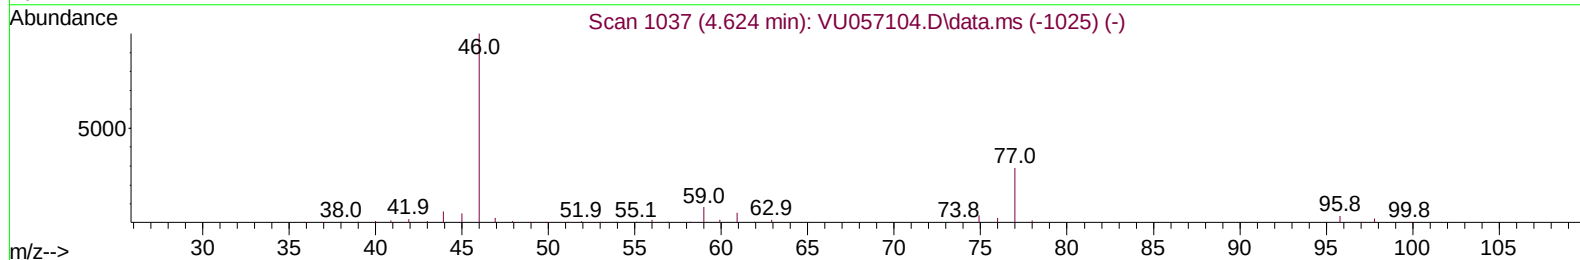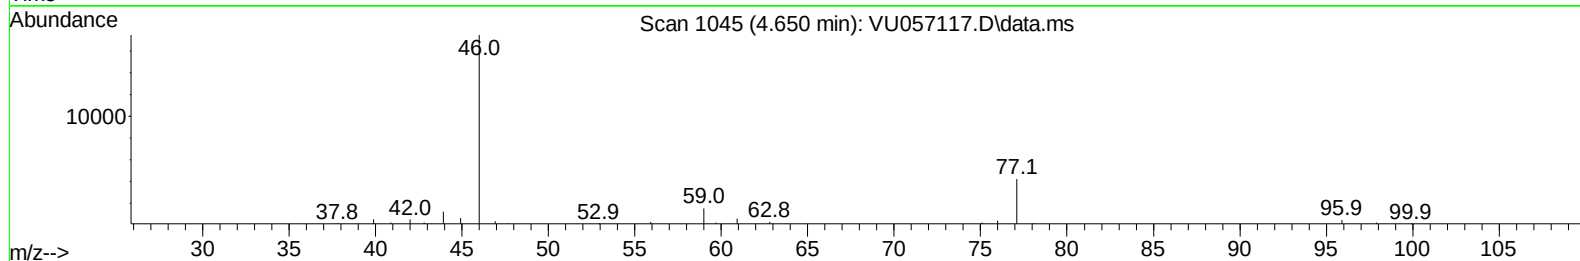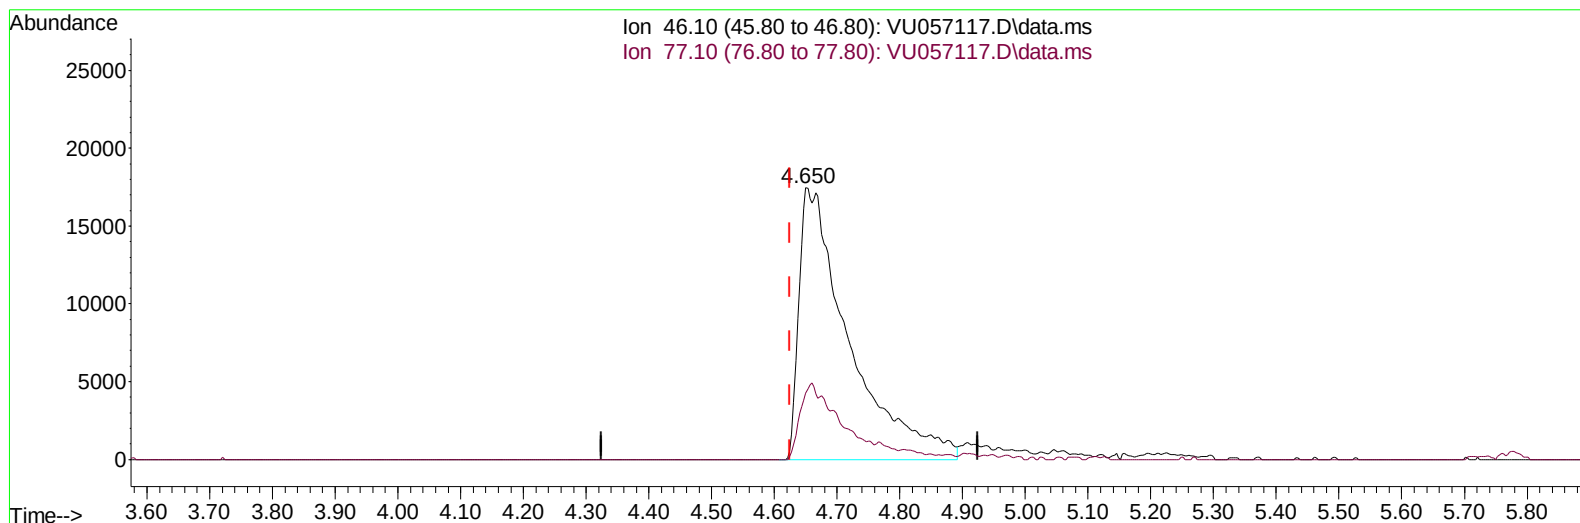

TIC: VU057117.D\data.ms

(20) 2-Butanone-d5 (S)

4.650min (+ 0.026) 31.91 ug/L m

response 96371

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.70	21.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
 Data File : VU057117.D
 Acq On : 21 Dec 2023 02:12
 Operator : MD/SY
 Sample : 05892-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7B01

Manual IntegrationsAPPROVED

Quant Time: Dec 21 05:02:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 21 01:34:13 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	178433	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	178572	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	85750	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	53660	3.508	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	70.200%	
7) Chloroethane-d5	1.911	69	48238	4.215	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	84.200%	
11) 1,1-Dichloroethene-d2	2.560	65	25999	3.973	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	79.400%	
20) 2-Butanone-d5	4.650	46	96371m	31.906	ug/L	0.03
Spiked Amount 50.000	Range 40	- 130	Recovery	=	63.820%	
24) Chloroform-d	5.055	84	125556	4.335	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.698	65	61594	4.494	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	89.800%	
32) Benzene-d6	5.721	84	222512	4.017	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	80.400%	
36) 1,2-Dichloropropane-d6	6.685	67	67514	3.894	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	77.800%	
41) Toluene-d8	7.894	98	187936	3.796	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	8.177	79	24270	3.610	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	72.200%	
46) 2-Hexanone-d5	8.634	63	89810	35.419	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	70.840%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	53759	4.286	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	85.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152	75959	4.506	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	90.200%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.576	96	11955	0.825	ug/L #	23
14) Carbon disulfide	2.788	76	7555	0.150	ug/L #	94
19) 1,1-Dichloroethane	3.865	63	3706	0.131	ug/L #	88
22) cis-1,2-Dichloroethene	4.666	96	1640	0.103	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057117.D
Acq On : 21 Dec 2023 02:12
Operator : MD/SY
Sample : 05892-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7B01

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/21/2023
Supervised By :Semsettin Yesilyurt 12/21/2023

Quant Time: Dec 21 05:02:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 21 01:34:13 2023
Response via : Initial Calibration

