




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057121.D
Acq On : 21 Dec 2023 04:13
Operator : MD/SY
Sample : 05892-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7B10

Manual IntegrationsAPPROVED

Quant Time: Dec 21 05:04:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 21 01:34:13 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
Supervised By :Semsettin Yesilyurt 12/21/2023

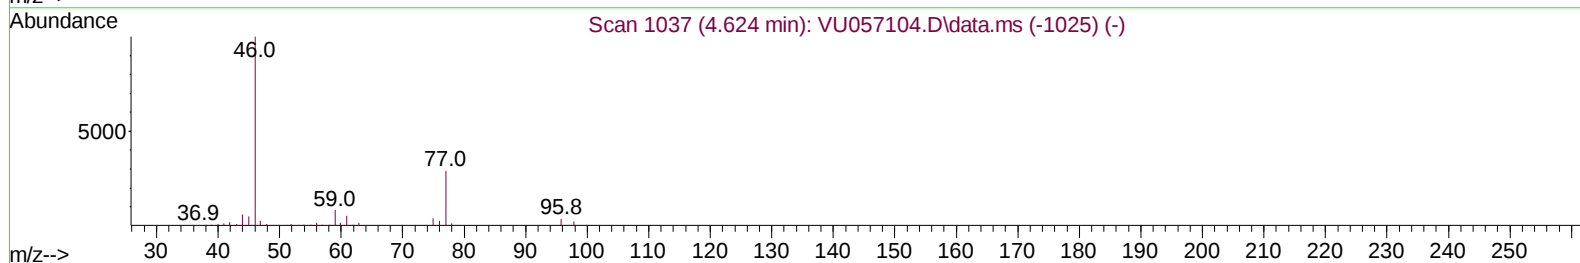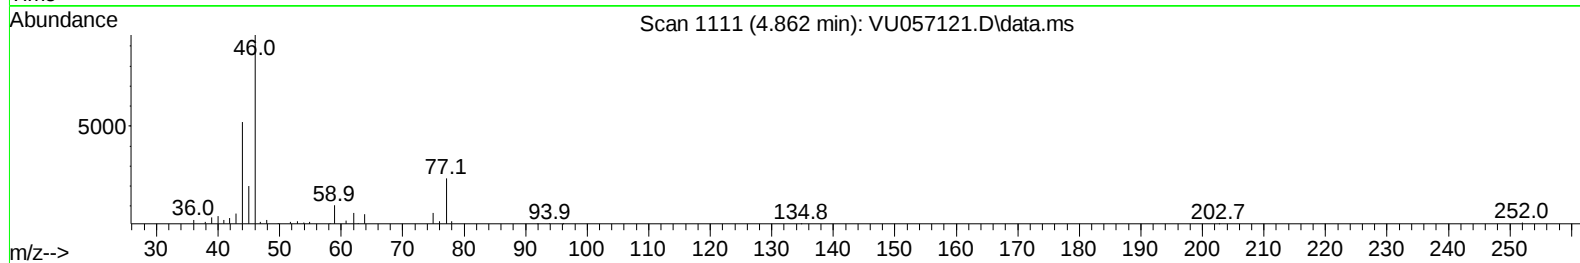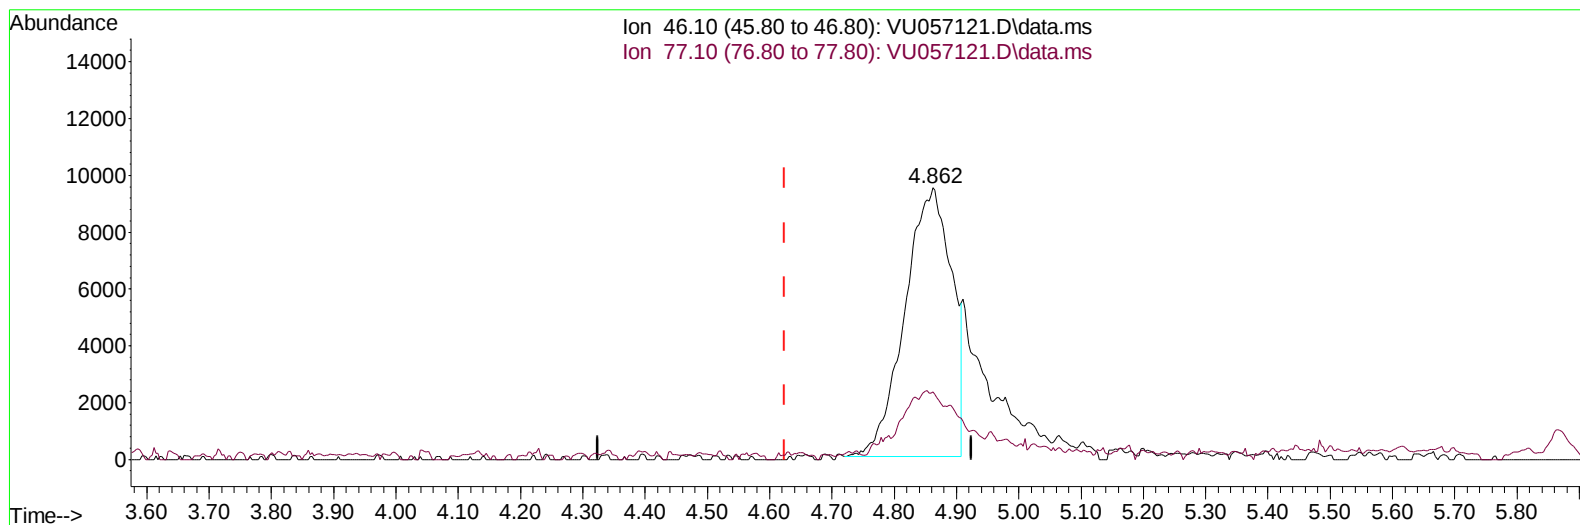

TIC: VU057121.D\data.ms

(20) 2-Butanone-d5 (S)

4.862min (+ 0.238) 16.91 ug/L

response 49291

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.70	4.86#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
 Data File : VU057121.D
 Acq On : 21 Dec 2023 04:13
 Operator : MD/SY
 Sample : 05892-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7B10

Manual IntegrationsAPPROVED

Quant Time: Dec 21 05:04:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 21 01:34:13 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

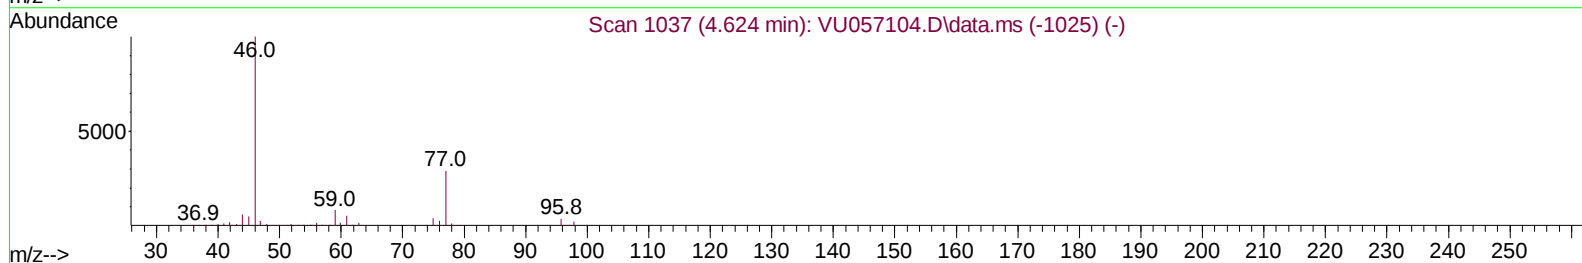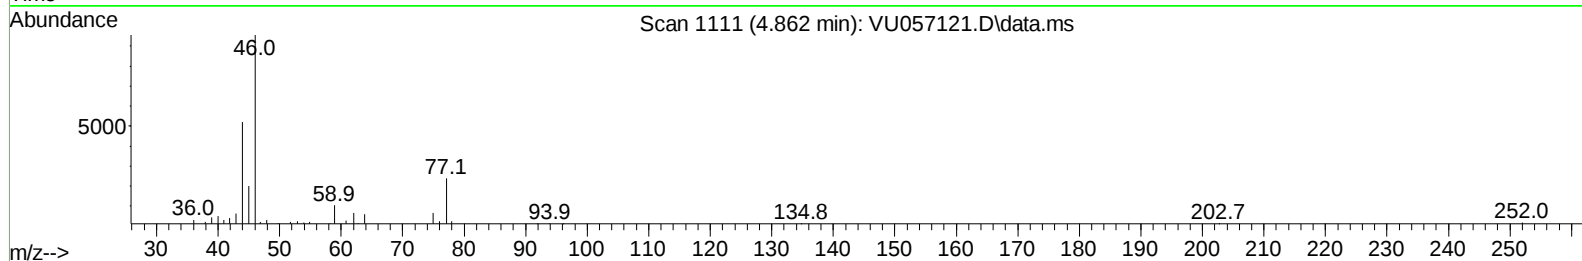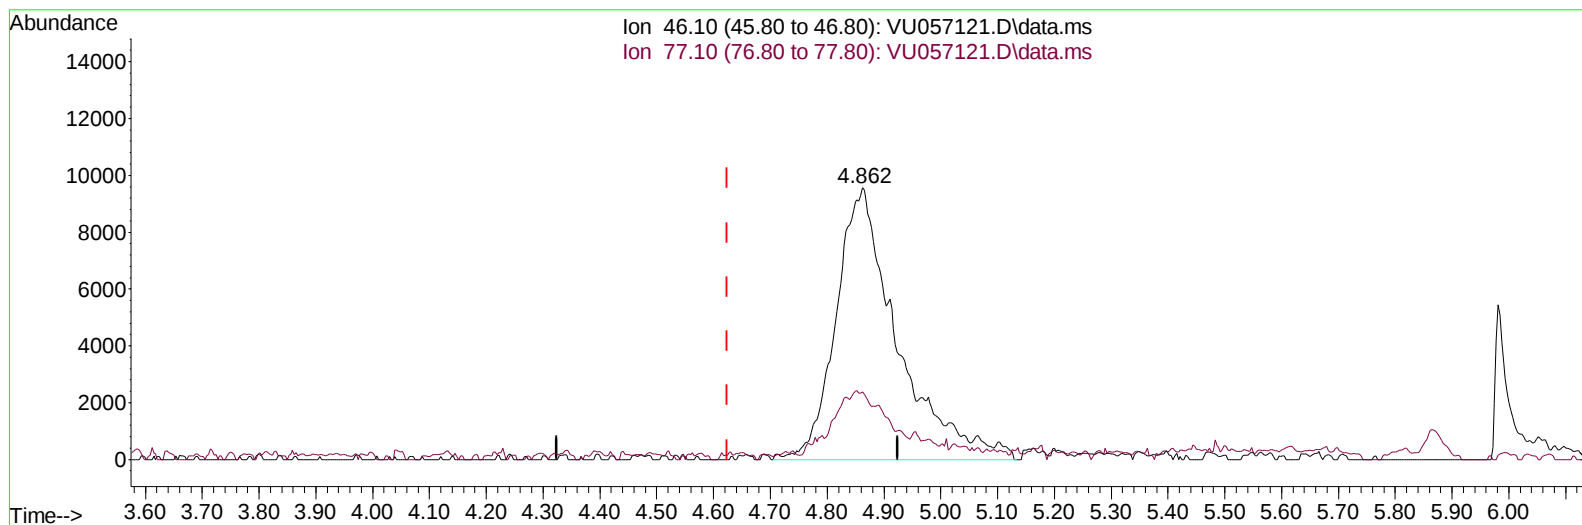

TIC: VU057121.D\data.ms

(20) 2-Butanone-d5 (S)

4.862min (+ 0.238) 24.55 ug/L m

response 71573

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.70	3.35#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
 Data File : VU057121.D
 Acq On : 21 Dec 2023 04:13
 Operator : MD/SY
 Sample : 05892-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7B10

Manual IntegrationsAPPROVED

Quant Time: Dec 21 05:04:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 21 01:34:13 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.373	114	172211	5.000	ug/L	0.13
28) Chlorobenzene-d5	9.444	117	169985	5.000	ug/L	0.03
58) 1,4-Dichlorobenzene-d4	11.817	152	72194	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.644	65	59952	4.061	ug/L	0.05
Spiked Amount 5.000	Range 40	- 130	Recovery	=	81.200%	
7) Chloroethane-d5	2.013	69	54006	4.889	ug/L	0.10
Spiked Amount 5.000	Range 65	- 130	Recovery	=	97.800%	
11) 1,1-Dichloroethene-d2	2.672	65	28125	4.453	ug/L	0.11
Spiked Amount 5.000	Range 60	- 125	Recovery	=	89.000%	
20) 2-Butanone-d5	4.862	46	71573m	24.552	ug/L	0.24
Spiked Amount 50.000	Range 40	- 130	Recovery	=	49.100%	
24) Chloroform-d	5.142	84	117904	4.218	ug/L	0.09
Spiked Amount 5.000	Range 70	- 125	Recovery	=	84.400%	
26) 1,2-Dichloroethane-d4	5.798	65	45843	3.466	ug/L	0.10
Spiked Amount 5.000	Range 70	- 130	Recovery	=	69.400%#	
32) Benzene-d6	5.814	84	222082	4.212	ug/L	0.09
Spiked Amount 5.000	Range 70	- 125	Recovery	=	84.200%	
36) 1,2-Dichloropropane-d6	6.795	67	60500	3.666	ug/L	0.11
Spiked Amount 5.000	Range 60	- 140	Recovery	=	73.400%	
41) Toluene-d8	7.955	98	165742	3.517	ug/L	0.06
Spiked Amount 5.000	Range 70	- 130	Recovery	=	70.400%	
43) trans-1,3-Dichloroprop...	8.232	79	16935	2.646	ug/L	0.06
Spiked Amount 5.000	Range 55	- 130	Recovery	=	53.000%#	
46) 2-Hexanone-d5	8.685	63	49522	20.517	ug/L	0.06
Spiked Amount 50.000	Range 45	- 130	Recovery	=	41.040%#	
56) 1,1,2,2-Tetrachloroeth...	10.765	84	30930	2.590	ug/L	0.02
Spiked Amount 5.000	Range 65	- 120	Recovery	=	51.800%#	
66) 1,2-Dichlorobenzene-d4	12.196	152	53362	3.760	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	75.200%#	
Target Compounds						
						Qvalue
12) 1,1-Dichloroethene	2.685	96	127811	9.142	ug/L	79
19) 1,1-Dichloroethane	4.004	63	43656	1.601	ug/L	99
22) cis-1,2-Dichloroethene	4.766	96	14539	0.943	ug/L	87
34) Trichloroethene	6.650	95	7996	0.488	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057121.D
Acq On : 21 Dec 2023 04:13
Operator : MD/SY
Sample : 05892-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7B10

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/21/2023
Supervised By :Semsettin Yesilyurt 12/21/2023

Quant Time: Dec 21 05:04:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 21 01:34:13 2023
Response via : Initial Calibration

