

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
 Data File : VU057082.D
 Acq On : 20 Dec 2023 11:14
 Operator : MD/SY
 Sample : VIBLK175
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK175

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

Quant Time: Dec 20 23:43:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 20 23:41:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	197424	5.000	ug/L	0.01
28) Chlorobenzene-d5	9.415	117	188424	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	84141	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	65731	3.884	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.600%	
7) Chloroethane-d5	1.911	69	58050	4.584	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.600%	
11) 1,1-Dichloroethene-d2	2.557	65	32812	4.532	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	90.600%	
20) 2-Butanone-d5	4.750	46	95239m	28.498	ug/L	0.14
Spiked Amount	50.000	Range 40 - 130	Recovery	=	57.000%	
24) Chloroform-d	5.055	84	142574	4.449	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.000%	
26) 1,2-Dichloroethane-d4	5.718	65	65245	4.303	ug/L	0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.000%	
32) Benzene-d6	5.734	84	256043	4.381	ug/L	0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.600%	
36) 1,2-Dichloropropane-d6	6.698	67	75111	4.106	ug/L	0.01
Spiked Amount	5.000	Range 60 - 140	Recovery	=	82.200%	
41) Toluene-d8	7.897	98	220473	4.221	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.400%	
43) trans-1,3-Dichloroprop...	8.184	79	26221	3.696	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.000%	
46) 2-Hexanone-d5	8.647	63	70659	26.409	ug/L	0.02
Spiked Amount	50.000	Range 45 - 130	Recovery	=	52.820%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	49249	3.721	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	74.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152	74761	4.520	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	90.400%	
Target Compounds						Qvalue
51) Chlorobenzene	9.447	112	12337	0.283	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057082.D
Acq On : 20 Dec 2023 11:14
Operator : MD/SY
Sample : VIBLK175
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
VIBLK175

Quant Time: Dec 20 23:43:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 20 23:41:59 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 12/21/2023
Supervised By :Semsettin Yesilyurt 12/21/2023

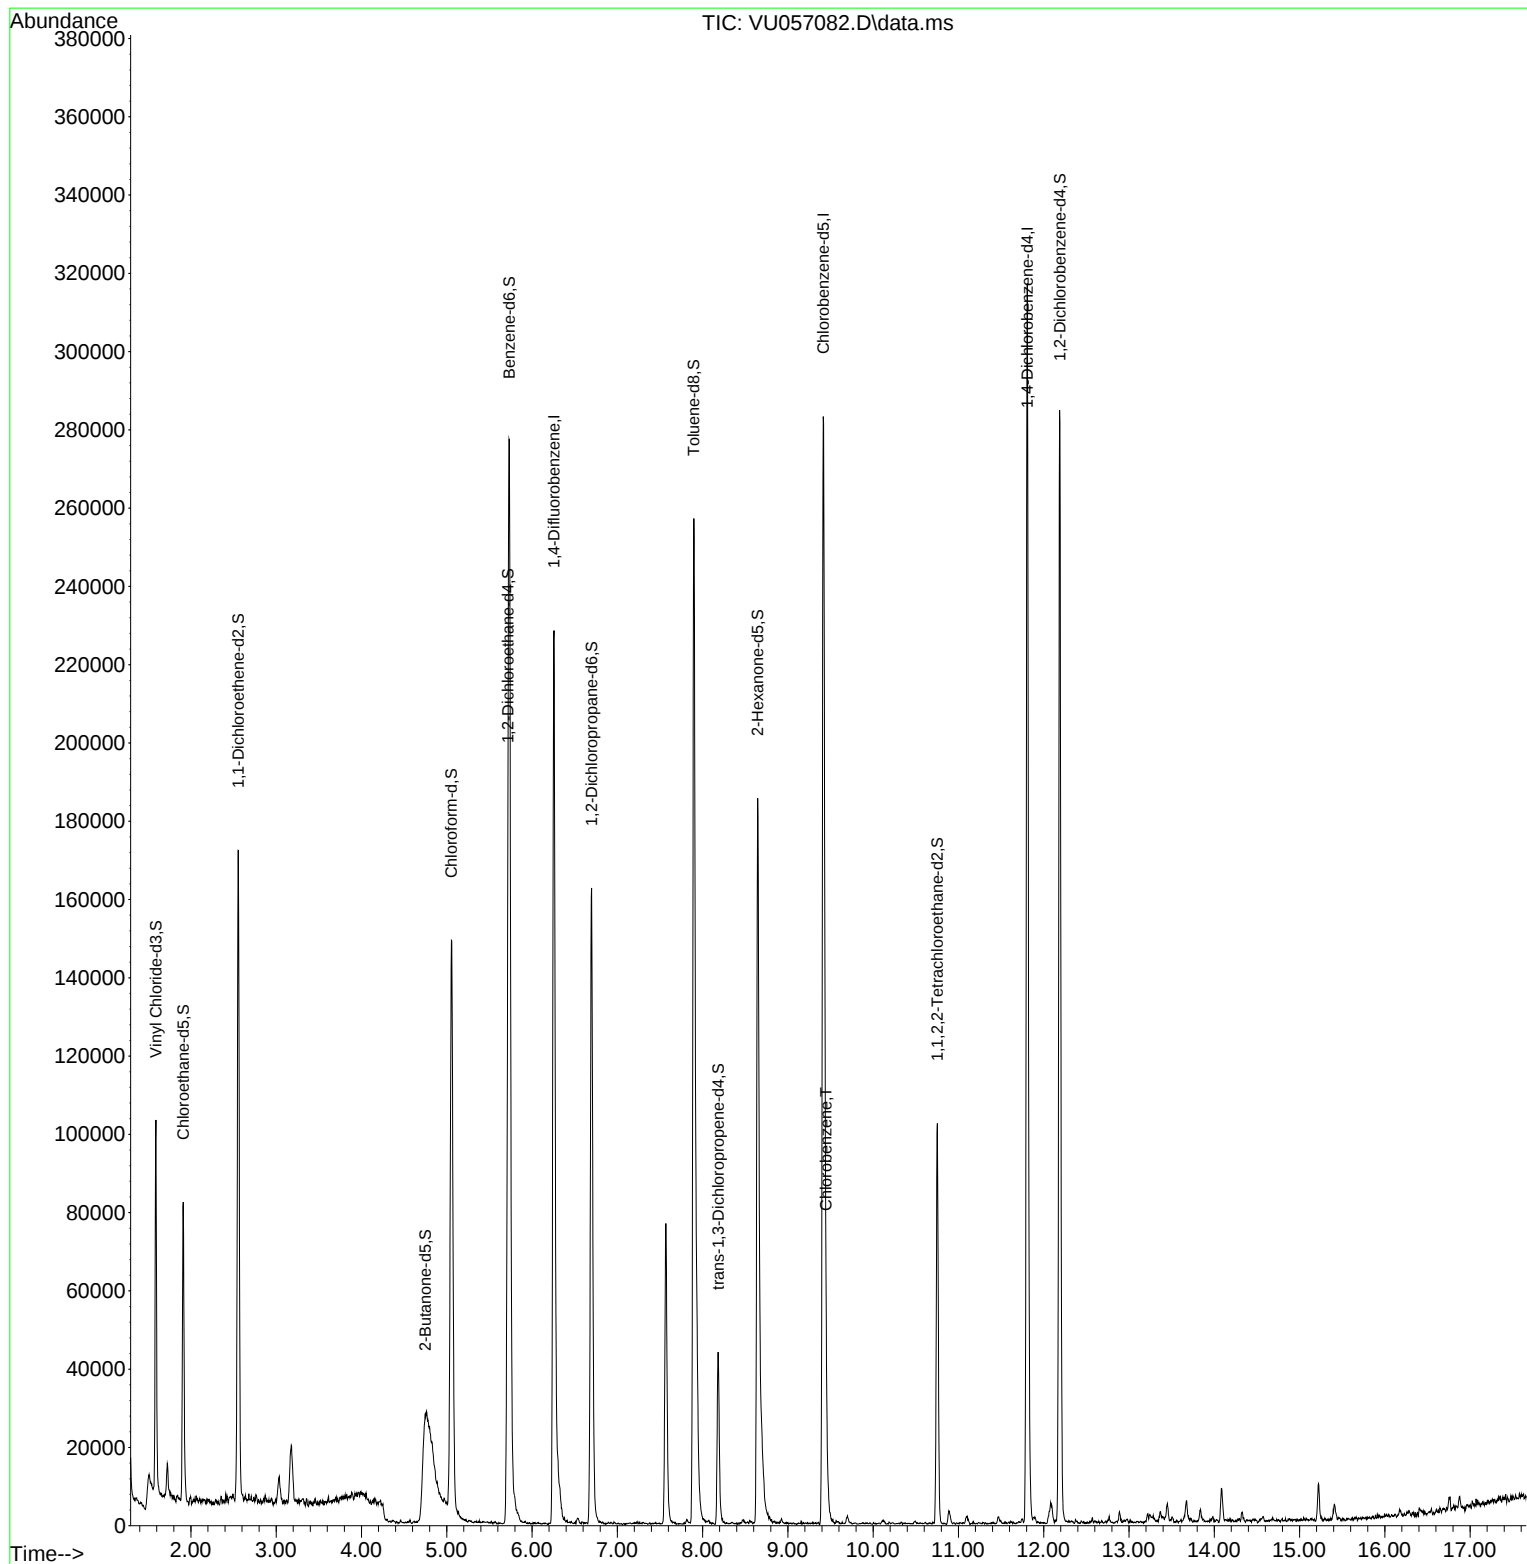

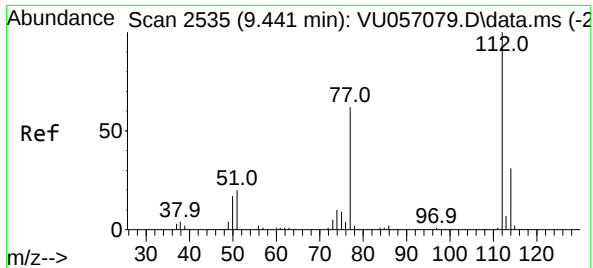

#51
 Chlorobenzene
 Concen: 0.283 ug/L
 RT: 9.447 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VU057082.D
 Acq: 20 Dec 2023 11:14

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK175

Tgt Ion:112	Resp:	1233
Ion Ratio	Lower	Upper
112	100	
114	29.6	21.9 40.7
77	68.6	51.6 77.4

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 12/21/2023
 Supervised By :Semsettin Yesilyurt 12/21/2023

