

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
 Data File : VU057102.D
 Acq On : 20 Dec 2023 19:17
 Operator : MD/SY
 Sample : 05949-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGR38

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	79038	89986	8.87%	1.414%
2	1.907	184	192	206	rVB	63117	87966	8.67%	1.383%
3	2.563	383	396	411	rBV	134551	221114	21.80%	3.475%
4	4.621	1024	1036	1065	rBV	76854	239474	23.61%	3.764%
5	5.055	1155	1171	1193	rBV2	135654	303927	29.97%	4.777%
6	5.718	1357	1377	1395	rBV2	238019	624097	61.54%	9.809%
7	6.245	1528	1541	1573	rBV	221075	439666	43.35%	6.910%
8	6.541	1622	1633	1647	rBV6	9937	19321	1.91%	0.304%
9	6.685	1664	1678	1696	rBV	148754	295475	29.13%	4.644%
10	7.560	1938	1950	1965	rBV	71328	130051	12.82%	2.044%
11	7.894	2038	2054	2072	rBV	277171	499271	49.23%	7.847%
12	8.177	2128	2142	2161	rBV2	42705	77519	7.64%	1.218%
13	8.547	2243	2257	2273	rBV	593709	1014188	100.00%	15.940%
14	8.631	2273	2283	2310	rVB2	292621	578814	57.07%	9.097%
15	9.412	2511	2526	2558	rBV	325929	573090	56.51%	9.007%
16	10.749	2930	2942	2962	rBV	110401	182775	18.02%	2.873%
17	11.807	3259	3271	3291	rBV	314289	506441	49.94%	7.960%
18	12.061	3340	3350	3364	rBV4	11632	23939	2.36%	0.376%
19	12.187	3378	3389	3408	rBV	272385	455341	44.90%	7.157%




Sum of corrected areas: 6362455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057102.D
Acq On : 20 Dec 2023 19:17
Operator : MD/SY
Sample : 05949-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

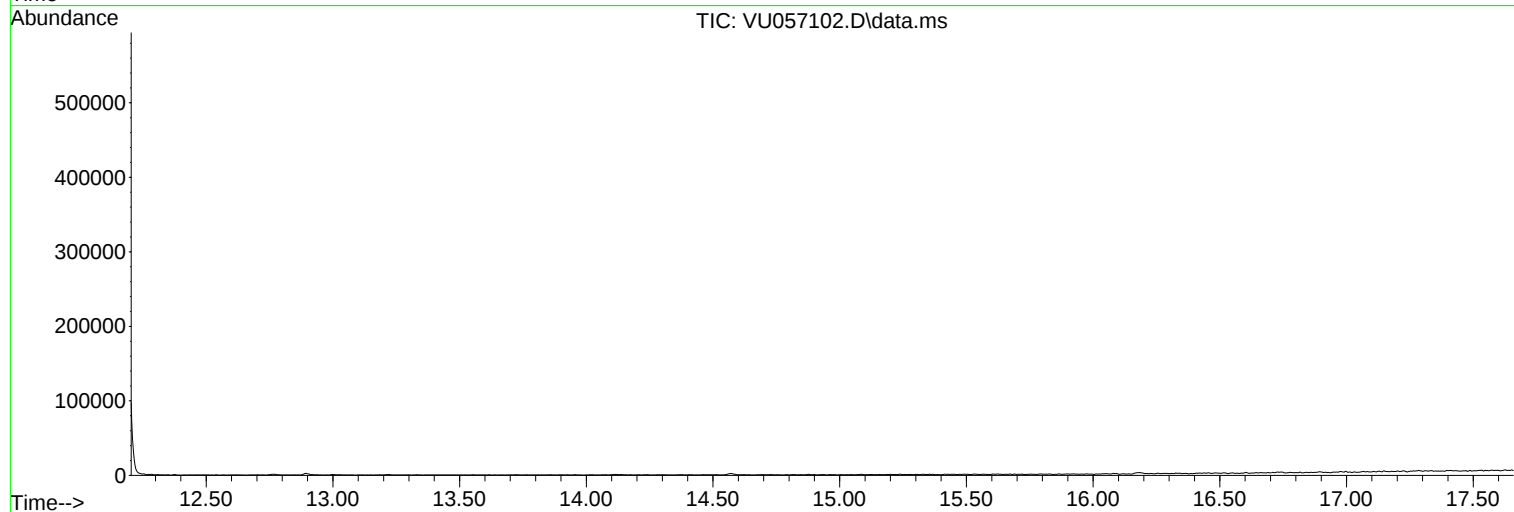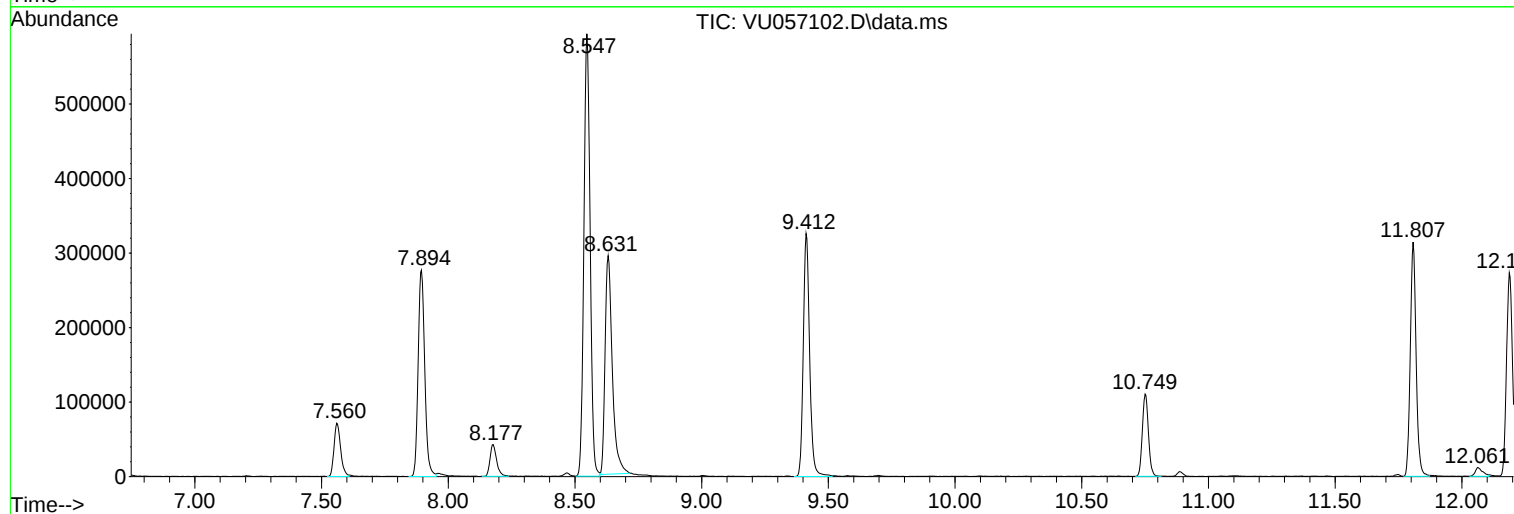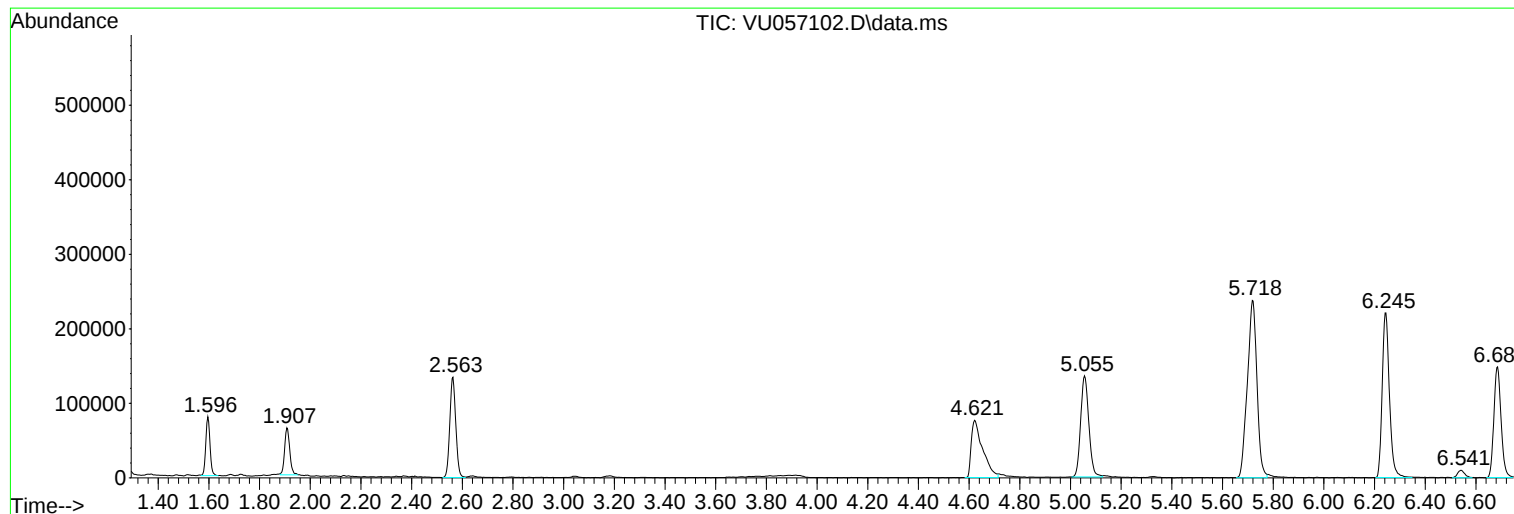

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057102.D
Acq On : 20 Dec 2023 19:17
Operator : MD/SY
Sample : 05949-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057102.D
Acq On : 20 Dec 2023 19:17
Operator : MD/SY
Sample : 05949-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc