
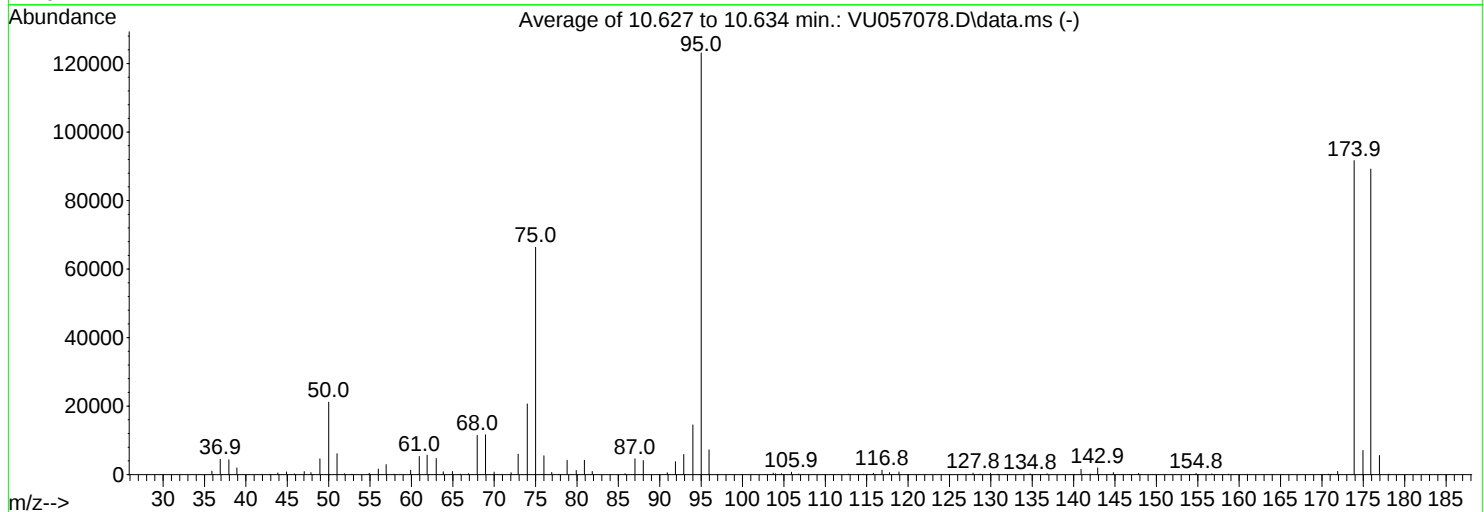


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122023\
Data File : VU057078.D
Acq On : 20 Dec 2023 08:43
Operator : MD/SY
Sample : BFB098
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB098

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 21 01:34:13 2023

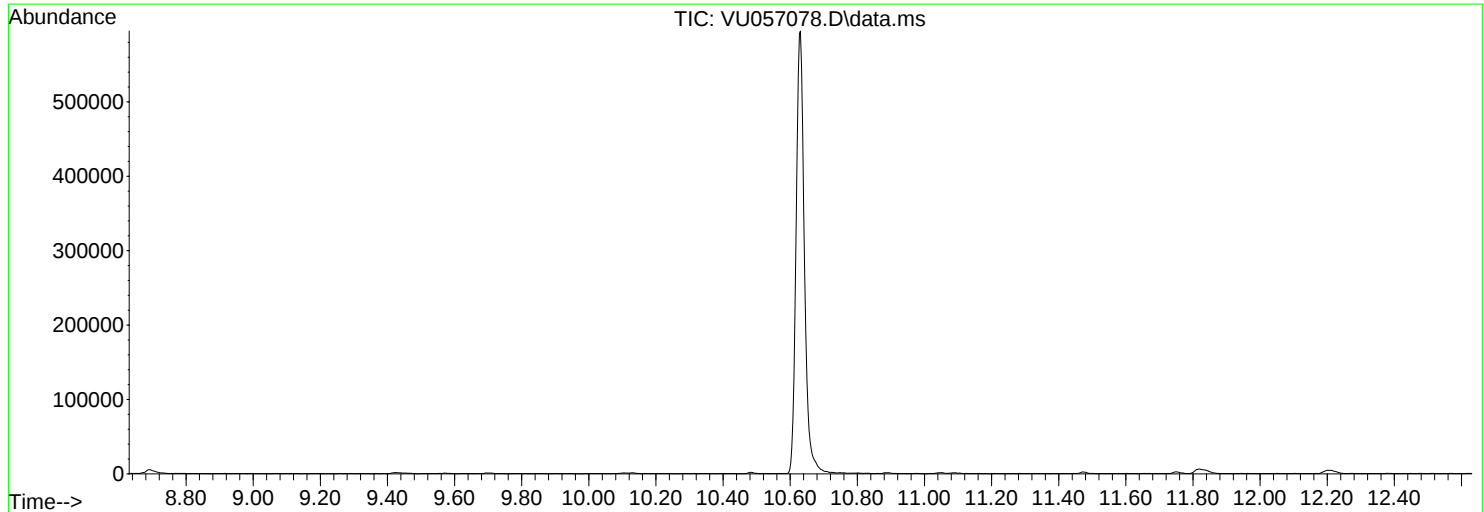

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	21144	PASS
75	95	30	80	53.9	66352	PASS
95	95	100	100	100.0	123117	PASS
96	95	5	9	5.9	7245	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.5	91677	PASS
175	174	5	9	7.7	7044	PASS
176	174	95	101	97.3	89189	PASS
177	176	5	9	6.3	5603	PASS

m/z	Abundance
39.90	196.0
43.80	129.0
44.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098

m/z	Abundance
35.90	1074.0
36.90	4691.0
38.00	4357.0
38.90	2035.0
39.90	193.0
43.90	788.0
44.90	818.0
45.80	283.0
47.00	914.0
47.90	766.0
49.00	4697.0
50.00	21560.0
51.00	6216.0
51.90	274.0
52.80	196.0
54.90	450.0
56.00	1709.0
57.00	2863.0
57.90	169.0
59.90	1187.0
60.90	5833.0
61.90	5741.0
63.00	5149.0
63.90	885.0
64.90	920.0
65.90	155.0
66.90	365.0
68.00	11624.0
68.90	12674.0
70.00	779.0
72.00	594.0
72.90	6256.0
74.00	21056.0
75.00	68664.0
76.00	5781.0
77.00	641.0
77.80	487.0
78.80	4295.0
79.90	1240.0
80.90	4574.0
81.80	905.0
85.80	268.0
87.00	4862.0
88.00	4183.0
90.90	591.0
91.90	3985.0
92.90	5691.0
94.00	14753.0
95.00	125720.0
96.00	7995.0
96.90	110.0
103.70	554.0
104.70	301.0
105.90	621.0
106.80	179.0
112.80	131.0
114.60	139.0
115.80	422.0
116.80	1238.0
117.70	515.0
118.90	812.0
127.90	507.0
128.60	218.0
130.00	415.0
130.80	149.0
134.70	248.0
136.80	317.0
140.90	1509.0
142.00	191.0
142.90	2116.0
144.80	556.0
145.80	144.0
146.80	103.0
147.80	365.0
154.80	351.0
156.60	231.0
158.70	159.0
161.00	171.0
171.10	241.0
171.90	971.0
173.90	92448.0
174.90	7014.0
175.90	90056.0
176.90	5805.0
178.10	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098

m/z	Abundance
35.90	1085.0
36.90	4491.0
38.00	4522.0
38.90	2086.0
40.00	169.0
43.90	787.0
44.90	831.0
45.80	290.0
47.10	868.0
47.90	605.0
48.90	4830.0
50.00	21632.0
51.00	6178.0
51.90	291.0
52.80	143.0
54.90	440.0
56.00	1633.0
56.90	2906.0
57.90	145.0
59.90	1368.0
60.90	5434.0
61.90	5917.0
63.00	4804.0
63.80	854.0
64.90	983.0
65.90	143.0
66.90	306.0
67.90	11806.0
68.90	11928.0
70.00	743.0
72.00	552.0
72.90	6270.0
74.00	21072.0
75.00	68368.0
76.00	5679.0
76.90	626.0
78.80	4304.0
79.90	1290.0
80.90	4309.0
81.90	925.0
85.80	313.0
87.00	4807.0
88.00	4236.0
90.90	587.0
91.90	3889.0
92.90	6131.0
94.00	14930.0
95.00	126616.0
95.90	7374.0
103.70	451.0
104.00	415.0
104.70	289.0
105.90	751.0
106.80	185.0
112.80	187.0
114.70	140.0
115.80	461.0
116.90	1374.0
117.70	633.0
118.90	841.0
127.90	508.0
128.70	193.0
130.00	436.0
130.90	169.0
134.80	263.0
136.80	304.0
140.90	1594.0
142.00	199.0
142.90	2001.0
144.80	622.0
146.00	158.0
146.80	107.0
147.80	365.0
154.80	399.0
156.70	236.0
158.70	144.0
161.00	120.0
170.80	242.0
171.90	908.0
173.90	94584.0
175.00	7289.0
175.90	92312.0
177.00	5799.0
178.10	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098

m/z	Abundance
35.90	954.0
36.90	4262.0
37.90	4107.0
38.90	1817.0
40.00	165.0
42.90	105.0
43.80	766.0
44.90	801.0
45.90	199.0
47.10	924.0
47.80	500.0
48.90	4407.0
50.00	20240.0
51.00	5928.0
51.90	265.0
52.80	119.0
54.90	419.0
56.00	1574.0
56.90	3003.0
57.90	136.0
59.90	1335.0
61.00	4770.0
61.90	5479.0
63.00	4268.0
63.90	860.0
65.00	917.0
65.90	139.0
66.90	231.0
67.90	11068.0
69.00	10301.0
70.00	731.0
72.10	515.0
72.90	5360.0
74.00	19760.0
75.00	62024.0
76.00	5028.0
76.90	639.0
78.80	3984.0
79.90	1144.0
80.90	3692.0
81.90	953.0
85.80	245.0
87.00	4265.0
88.00	3863.0
90.90	532.0
91.90	3476.0
92.90	5821.0
94.00	13890.0
95.00	117016.0
96.00	6366.0
103.70	354.0
104.00	366.0
104.70	225.0
105.90	712.0
106.80	148.0
112.80	181.0
114.60	135.0
115.80	427.0
116.90	1364.0
117.80	619.0
118.90	781.0
127.80	447.0
128.80	153.0
129.90	437.0
130.80	171.0
134.80	260.0
136.80	277.0
140.10	122.0
140.90	1529.0
142.00	216.0
142.90	1789.0
144.80	638.0
146.00	185.0
147.90	371.0
149.60	103.0
154.80	398.0
156.80	248.0
158.70	122.0
170.80	215.0
171.90	897.0
173.90	88000.0
175.00	6830.0
175.90	85200.0
177.00	5205.0
178.10	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098