

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122118\
 Data File : VU028903.D
 Acq On : 22 Dec 2018 03:08
 Operator : MD/SY
 Sample : J6542-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	81	rVB	93762	91864	14.23%	1.906%
2	1.665	146	153	171	rVB	69084	86425	13.39%	1.793%
3	2.267	329	340	354	rBV	138514	208376	32.29%	4.324%
4	2.453	390	398	410	rVB	1546	2515	0.39%	0.052%
5	2.627	446	452	459	rBV2	321	562	0.09%	0.012%
6	2.694	470	473	478	rBV2	430	320	0.05%	0.007%
7	2.836	507	517	530	rVB	1336	2661	0.41%	0.055%
8	3.000	564	568	572	rBV	120	127	0.02%	0.003%
9	3.279	650	655	657	rBV	107	90	0.01%	0.002%
10	3.395	688	691	695	rBV	75	59	0.01%	0.001%
11	3.443	700	706	709	rBV	100	105	0.02%	0.002%
12	3.463	709	712	715	rBV	107	63	0.01%	0.001%
13	3.533	725	734	738	rBV	128	194	0.03%	0.004%
14	3.585	746	750	757	rVB	164	181	0.03%	0.004%
15	3.623	757	762	763	rBV	124	97	0.02%	0.002%
16	3.923	852	855	858	rBV	97	90	0.01%	0.002%
17	3.942	858	861	867	rBV2	333	328	0.05%	0.007%
18	4.074	898	902	905	rVB2	204	178	0.03%	0.004%
19	4.177	920	934	962	rBV	62275	163324	25.31%	3.389%
20	4.447	1012	1018	1022	rBV2	218	296	0.05%	0.006%
21	4.527	1041	1043	1046	rBV2	161	95	0.01%	0.002%
22	4.646	1062	1080	1104	rBV	104314	241501	37.42%	5.011%
23	4.730	1104	1106	1110	rVV	148	53	0.01%	0.001%
24	4.794	1124	1126	1128	rVB	164	70	0.01%	0.001%
25	4.829	1134	1137	1141	rVV	82	64	0.01%	0.001%
26	4.881	1152	1153	1154	rBV	224	71	0.01%	0.001%
27	5.016	1192	1195	1198	rBV	65	54	0.01%	0.001%
28	5.093	1216	1219	1223	rVB	84	63	0.01%	0.001%
29	5.128	1228	1230	1234	rBV	64	58	0.01%	0.001%
30	5.148	1234	1236	1240	rVV	143	67	0.01%	0.001%
31	5.337	1272	1295	1320	rBV2	224526	645391	100.00%	13.391%
32	5.662	1388	1396	1400	rBV	114	127	0.02%	0.003%
33	5.736	1417	1419	1422	rBV	68	56	0.01%	0.001%
34	5.791	1431	1436	1439	rVB	101	89	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122118\
 Data File : VU028903.D
 Acq On : 22 Dec 2018 03:08
 Operator : MD/SY
 Sample : J6542-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

35	5.820	1439	1445	1447	rBV	107	123	0.02%	0.003%
36	5.884	1452	1465	1485	rBV	198135	382497	59.27%	7.937%
37	6.112	1534	1536	1540	rVB	173	72	0.01%	0.001%
38	6.189	1558	1560	1562	rVV	136	58	0.01%	0.001%
39	6.328	1590	1603	1629	rBV	151266	296576	45.95%	6.154%
40	6.418	1629	1631	1634	rBV	182	114	0.02%	0.002%
41	6.456	1640	1643	1645	rBV	292	162	0.03%	0.003%
42	6.504	1655	1658	1661	rVB	167	78	0.01%	0.002%
43	6.604	1686	1689	1692	rBV	74	53	0.01%	0.001%
44	6.839	1759	1762	1765	rBV	122	96	0.01%	0.002%
45	6.887	1775	1777	1779	rBV	120	65	0.01%	0.001%
46	6.958	1794	1799	1803	rBV	70	71	0.01%	0.001%
47	6.987	1803	1808	1811	rVB	59	57	0.01%	0.001%
48	7.012	1812	1816	1819	rBV	112	69	0.01%	0.001%
49	7.051	1825	1828	1836	rBV	94	100	0.02%	0.002%
50	7.096	1839	1842	1844	rVB	171	80	0.01%	0.002%
51	7.112	1844	1847	1849	rBV	137	90	0.01%	0.002%
52	7.225	1870	1882	1908	rBV	79940	140255	21.73%	2.910%
53	7.430	1943	1946	1951	rVB	94	72	0.01%	0.001%
54	7.456	1951	1954	1959	rBV	93	115	0.02%	0.002%
55	7.562	1974	1987	2010	rBV	290354	507533	78.64%	10.531%
56	7.848	2062	2076	2096	rBV	55683	92513	14.33%	1.920%
57	7.961	2108	2111	2115	rBV	243	171	0.03%	0.004%
58	7.980	2115	2117	2121	rVB	158	76	0.01%	0.002%
59	8.048	2134	2138	2140	rBV	176	140	0.02%	0.003%
60	8.176	2167	2178	2189	rBV2	3018	4952	0.77%	0.103%
61	8.231	2193	2195	2197	rVB	168	84	0.01%	0.002%
62	8.250	2197	2201	2206	rVB	148	146	0.02%	0.003%
63	8.311	2208	2220	2253	rBV	219364	370953	57.48%	7.697%
64	8.578	2300	2303	2305	rBV2	347	209	0.03%	0.004%
65	8.668	2330	2331	2333	rVB2	143	53	0.01%	0.001%
66	8.803	2371	2373	2376	rVB	143	61	0.01%	0.001%
67	8.855	2384	2389	2393	rBV	89	117	0.02%	0.002%
68	8.906	2403	2405	2408	rVB	197	89	0.01%	0.002%
69	8.964	2417	2423	2429	rBV	139	165	0.03%	0.003%
70	8.993	2429	2432	2434	rBV	86	61	0.01%	0.001%
71	9.090	2449	2462	2492	rBV	277598	467317	72.41%	9.696%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122118\
 Data File : VU028903.D
 Acq On : 22 Dec 2018 03:08
 Operator : MD/SY
 Sample : J6542-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

72	9.247	2508	2511	2514	rBV	288	204	0.03%	0.004%
73	9.305	2527	2529	2530	rBV	127	56	0.01%	0.001%
74	9.347	2537	2542	2544	rBV	122	120	0.02%	0.002%
75	9.376	2549	2551	2553	rBV	169	75	0.01%	0.002%
76	9.459	2575	2577	2580	rBV	103	55	0.01%	0.001%
77	9.479	2580	2583	2584	rBV	185	89	0.01%	0.002%
78	9.501	2587	2590	2592	rBV	155	112	0.02%	0.002%
79	9.591	2615	2618	2623	rBV	209	131	0.02%	0.003%
80	9.617	2624	2626	2629	rBV	108	67	0.01%	0.001%
81	9.671	2641	2643	2646	rBV2	128	71	0.01%	0.001%
82	9.726	2658	2660	2665	rVB	201	168	0.03%	0.003%
83	9.765	2670	2672	2675	rBV	155	67	0.01%	0.001%
84	9.839	2693	2695	2698	rBV	108	63	0.01%	0.001%
85	10.080	2768	2770	2772	rVB	246	105	0.02%	0.002%
86	10.205	2807	2809	2813	rVB	147	81	0.01%	0.002%
87	10.430	2866	2879	2898	rBV	202718	321977	49.89%	6.681%
88	10.540	2911	2913	2914	rBV	123	53	0.01%	0.001%
89	10.607	2925	2934	2944	rVB4	2927	4208	0.65%	0.087%
90	10.829	3001	3003	3006	rBV	121	72	0.01%	0.001%
91	11.028	3063	3065	3069	rVB	222	108	0.02%	0.002%
92	11.131	3094	3097	3099	rVV	128	83	0.01%	0.002%
93	11.250	3132	3134	3138	rBV	183	111	0.02%	0.002%
94	11.482	3193	3206	3230	rBV	241629	379439	58.79%	7.873%
95	11.687	3266	3270	3272	rBV2	230	136	0.02%	0.003%
96	11.858	3311	3323	3342	rBV	251302	400177	62.01%	8.303%
97	12.134	3404	3409	3413	rBV	206	217	0.03%	0.005%
98	12.276	3450	3453	3458	rBV2	165	152	0.02%	0.003%
99	12.327	3466	3469	3471	rVB2	278	137	0.02%	0.003%
100	12.659	3570	3572	3575	rVB	174	58	0.01%	0.001%


Sum of corrected areas: 4819449

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122118\
Data File : VU028903.D
Acq On : 22 Dec 2018 03:08
Operator : MD/SY
Sample : J6542-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

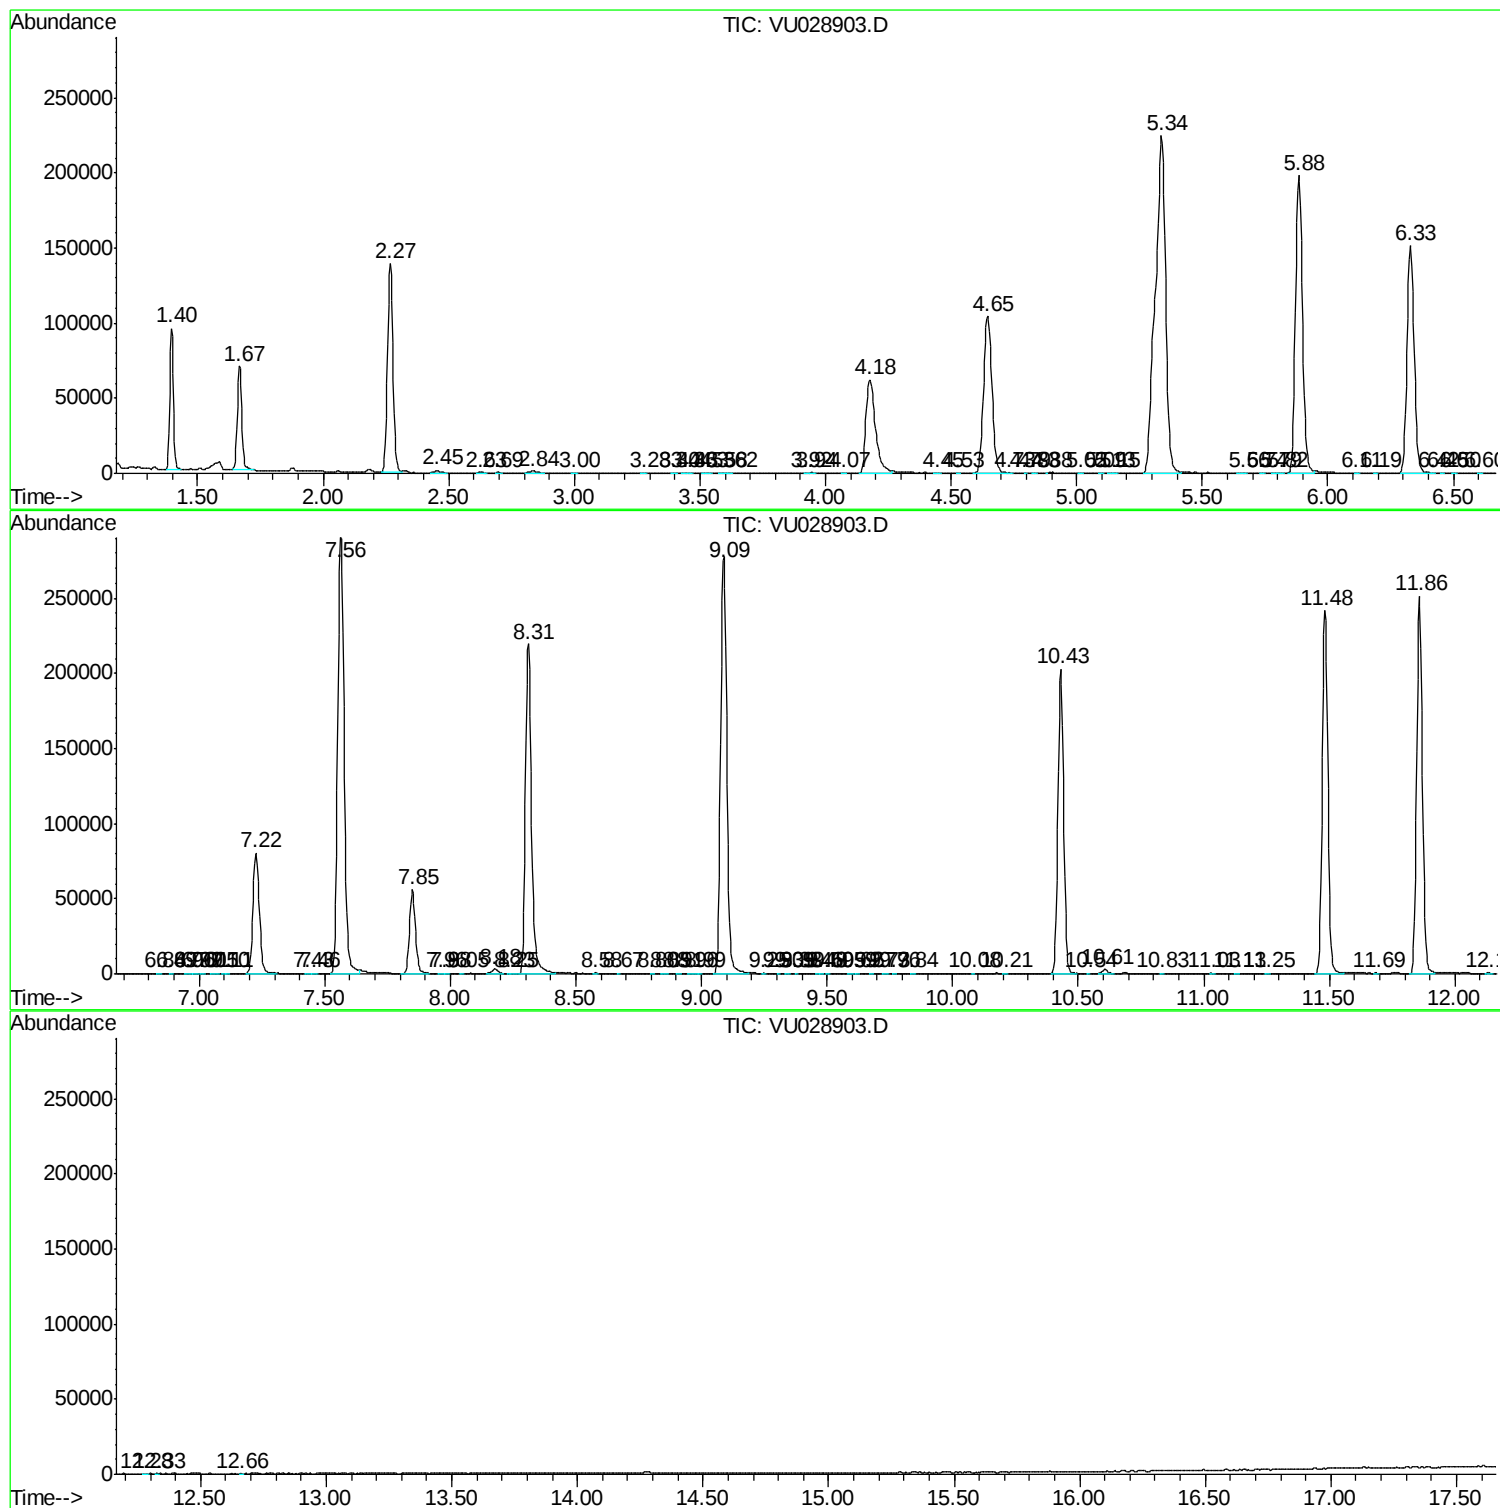

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122118\
Data File : VU028903.D
Acq On : 22 Dec 2018 03:08
Operator : MD/SY
Sample : J6542-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122118\
Data File : VU028903.D
Acq On : 22 Dec 2018 03:08
Operator : MD/SY
Sample : J6542-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc