

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122118\
 Data File : VU028905.D
 Acq On : 22 Dec 2018 03:56
 Operator : MD/SY
 Sample : J6542-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	83	rVB	88527	89032	14.04%	1.874%
2	1.665	145	153	163	rBV	68328	83193	13.12%	1.751%
3	2.267	329	340	354	rBV	139231	209144	32.99%	4.401%
4	2.691	470	472	474	rBV	171	84	0.01%	0.002%
5	2.839	506	518	530	rVB2	1895	4030	0.64%	0.085%
6	3.235	638	641	643	rBV2	171	94	0.01%	0.002%
7	3.328	667	670	674	rBV	65	64	0.01%	0.001%
8	3.379	684	686	688	rBV	59	34	0.01%	0.001%
9	3.537	733	735	740	rVB	188	100	0.02%	0.002%
10	3.562	740	743	747	rBV	214	149	0.02%	0.003%
11	3.627	761	763	764	rBV	117	54	0.01%	0.001%
12	3.656	769	772	774	rBV	94	62	0.01%	0.001%
13	3.906	846	850	855	rBV	104	107	0.02%	0.002%
14	3.980	872	873	876	rVB	170	41	0.01%	0.001%
15	4.093	905	908	909	rBV	84	52	0.01%	0.001%
16	4.177	921	934	963	rBV	62824	164780	25.99%	3.468%
17	4.376	994	996	999	rBV	262	93	0.01%	0.002%
18	4.460	1018	1022	1025	rBV	217	149	0.02%	0.003%
19	4.479	1025	1028	1031	rBV	216	166	0.03%	0.003%
20	4.540	1043	1047	1050	rBV	105	79	0.01%	0.002%
21	4.569	1055	1056	1059	rVB	172	87	0.01%	0.002%
22	4.646	1059	1080	1102	rBV	102827	237677	37.49%	5.002%
23	4.816	1131	1133	1135	rBV	144	66	0.01%	0.001%
24	4.871	1146	1150	1151	rBV	249	126	0.02%	0.003%
25	4.977	1182	1183	1185	rVB	137	49	0.01%	0.001%
26	4.993	1185	1188	1191	rBV	58	48	0.01%	0.001%
27	5.077	1212	1214	1217	rVB	109	53	0.01%	0.001%
28	5.099	1217	1221	1223	rBV	110	93	0.01%	0.002%
29	5.128	1227	1230	1233	rBV	81	56	0.01%	0.001%
30	5.234	1260	1263	1266	rVB	137	84	0.01%	0.002%
31	5.257	1266	1270	1272	rBV	114	105	0.02%	0.002%
32	5.337	1272	1295	1316	rBV2	222080	633923	100.00%	13.341%
33	5.527	1351	1354	1355	rBV	247	105	0.02%	0.002%
34	5.595	1374	1375	1377	rVB	158	55	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122118\
 Data File : VU028905.D
 Acq On : 22 Dec 2018 03:56
 Operator : MD/SY
 Sample : J6542-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

35	5.614	1377	1381	1383	rBV	126	106	0.02%	0.002%
36	5.643	1388	1390	1393	rBV	160	100	0.02%	0.002%
37	5.694	1404	1406	1409	rBV	135	71	0.01%	0.001%
38	5.749	1418	1423	1425	rBV	59	62	0.01%	0.001%
39	5.794	1435	1437	1439	rVB	165	68	0.01%	0.001%
40	5.810	1440	1442	1444	rBV	143	62	0.01%	0.001%
41	5.884	1452	1465	1497	rBV	192864	376302	59.36%	7.919%
42	6.125	1537	1540	1542	rBV	57	37	0.01%	0.001%
43	6.160	1547	1551	1555	rBV	103	87	0.01%	0.002%
44	6.260	1579	1582	1584	rBV	76	42	0.01%	0.001%
45	6.328	1590	1603	1628	rBV	147958	292410	46.13%	6.154%
46	6.453	1639	1642	1644	rBV2	143	96	0.02%	0.002%
47	6.559	1672	1675	1679	rVB	145	95	0.01%	0.002%
48	6.585	1679	1683	1687	rBV	143	141	0.02%	0.003%
49	6.742	1729	1732	1734	rBV	59	39	0.01%	0.001%
50	6.852	1762	1766	1767	rBV	89	68	0.01%	0.001%
51	6.913	1782	1785	1789	rBV	87	76	0.01%	0.002%
52	6.939	1791	1793	1794	rBV	165	52	0.01%	0.001%
53	7.225	1871	1882	1906	rBV	78068	137868	21.75%	2.901%
54	7.363	1922	1925	1927	rBV	61	45	0.01%	0.001%
55	7.411	1939	1940	1942	rBV	105	41	0.01%	0.001%
56	7.440	1945	1949	1952	rBV	203	117	0.02%	0.002%
57	7.475	1956	1960	1963	rBV	187	114	0.02%	0.002%
58	7.514	1969	1972	1974	rBV	86	48	0.01%	0.001%
59	7.562	1974	1987	2020	rBV	283970	501955	79.18%	10.564%
60	7.781	2053	2055	2059	rVB	173	75	0.01%	0.002%
61	7.848	2066	2076	2096	rBV	53978	90558	14.29%	1.906%
62	7.967	2111	2113	2117	rVB	148	69	0.01%	0.001%
63	7.990	2117	2120	2121	rBV	86	46	0.01%	0.001%
64	8.003	2122	2124	2125	rVV	192	66	0.01%	0.001%
65	8.025	2128	2131	2134	rVV	111	71	0.01%	0.001%
66	8.061	2140	2142	2145	rVB	214	73	0.01%	0.002%
67	8.176	2167	2178	2189	rBV3	2783	5029	0.79%	0.106%
68	8.247	2197	2200	2202	rVB	81	42	0.01%	0.001%
69	8.266	2203	2206	2208	rBV	100	68	0.01%	0.001%
70	8.311	2208	2220	2244	rBV	216277	366143	57.76%	7.705%
71	8.540	2288	2291	2294	rBV	189	137	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122118\
 Data File : VU028905.D
 Acq On : 22 Dec 2018 03:56
 Operator : MD/SY
 Sample : J6542-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis

72	8.578	2302	2303	2307	rVB	139	49	0.01%	0.001%
73	8.627	2316	2318	2320	rVB	153	40	0.01%	0.001%
74	8.681	2332	2335	2338	rBV2	188	134	0.02%	0.003%
75	8.713	2343	2345	2347	rVB2	252	104	0.02%	0.002%
76	8.771	2360	2363	2364	rBV2	116	47	0.01%	0.001%
77	9.090	2448	2462	2493	rBV	273043	454486	71.69%	9.565%
78	9.257	2511	2514	2516	rBV	177	119	0.02%	0.003%
79	9.469	2577	2580	2584	rVB	129	94	0.01%	0.002%
80	9.784	2674	2678	2679	rBV	186	88	0.01%	0.002%
81	10.019	2748	2751	2754	rBV	96	71	0.01%	0.001%
82	10.430	2867	2879	2898	rBV	202301	321798	50.76%	6.772%
83	10.536	2911	2912	2916	rVB	154	56	0.01%	0.001%
84	10.604	2927	2933	2942	rVB3	2285	3500	0.55%	0.074%
85	10.868	3012	3015	3021	rBV	190	166	0.03%	0.003%
86	10.945	3035	3039	3042	rBV	162	162	0.03%	0.003%
87	10.983	3050	3051	3052	rBV	121	35	0.01%	0.001%
88	11.061	3073	3075	3079	rVB2	204	142	0.02%	0.003%
89	11.366	3168	3170	3173	rBV	145	43	0.01%	0.001%
90	11.482	3195	3206	3223	rBV	237338	372401	58.75%	7.837%
91	11.694	3269	3272	3278	rVB3	439	365	0.06%	0.008%
92	11.787	3298	3301	3303	rVB2	260	166	0.03%	0.003%
93	11.858	3310	3323	3342	rBV	251425	400104	63.12%	8.420%
94	12.096	3395	3397	3399	rBV	210	120	0.02%	0.003%
95	12.151	3411	3414	3418	rVB2	204	171	0.03%	0.004%
96	12.173	3418	3421	3426	rVB2	286	186	0.03%	0.004%
97	12.527	3530	3531	3534	rBV	160	71	0.01%	0.001%
98	12.636	3563	3565	3570	rVB	289	218	0.03%	0.005%
99	12.662	3570	3573	3576	rBV	296	196	0.03%	0.004%
100	12.726	3591	3593	3594	rBV	221	78	0.01%	0.002%


Sum of corrected areas: 4751723

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122118\
Data File : VU028905.D
Acq On : 22 Dec 2018 03:56
Operator : MD/SY
Sample : J6542-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

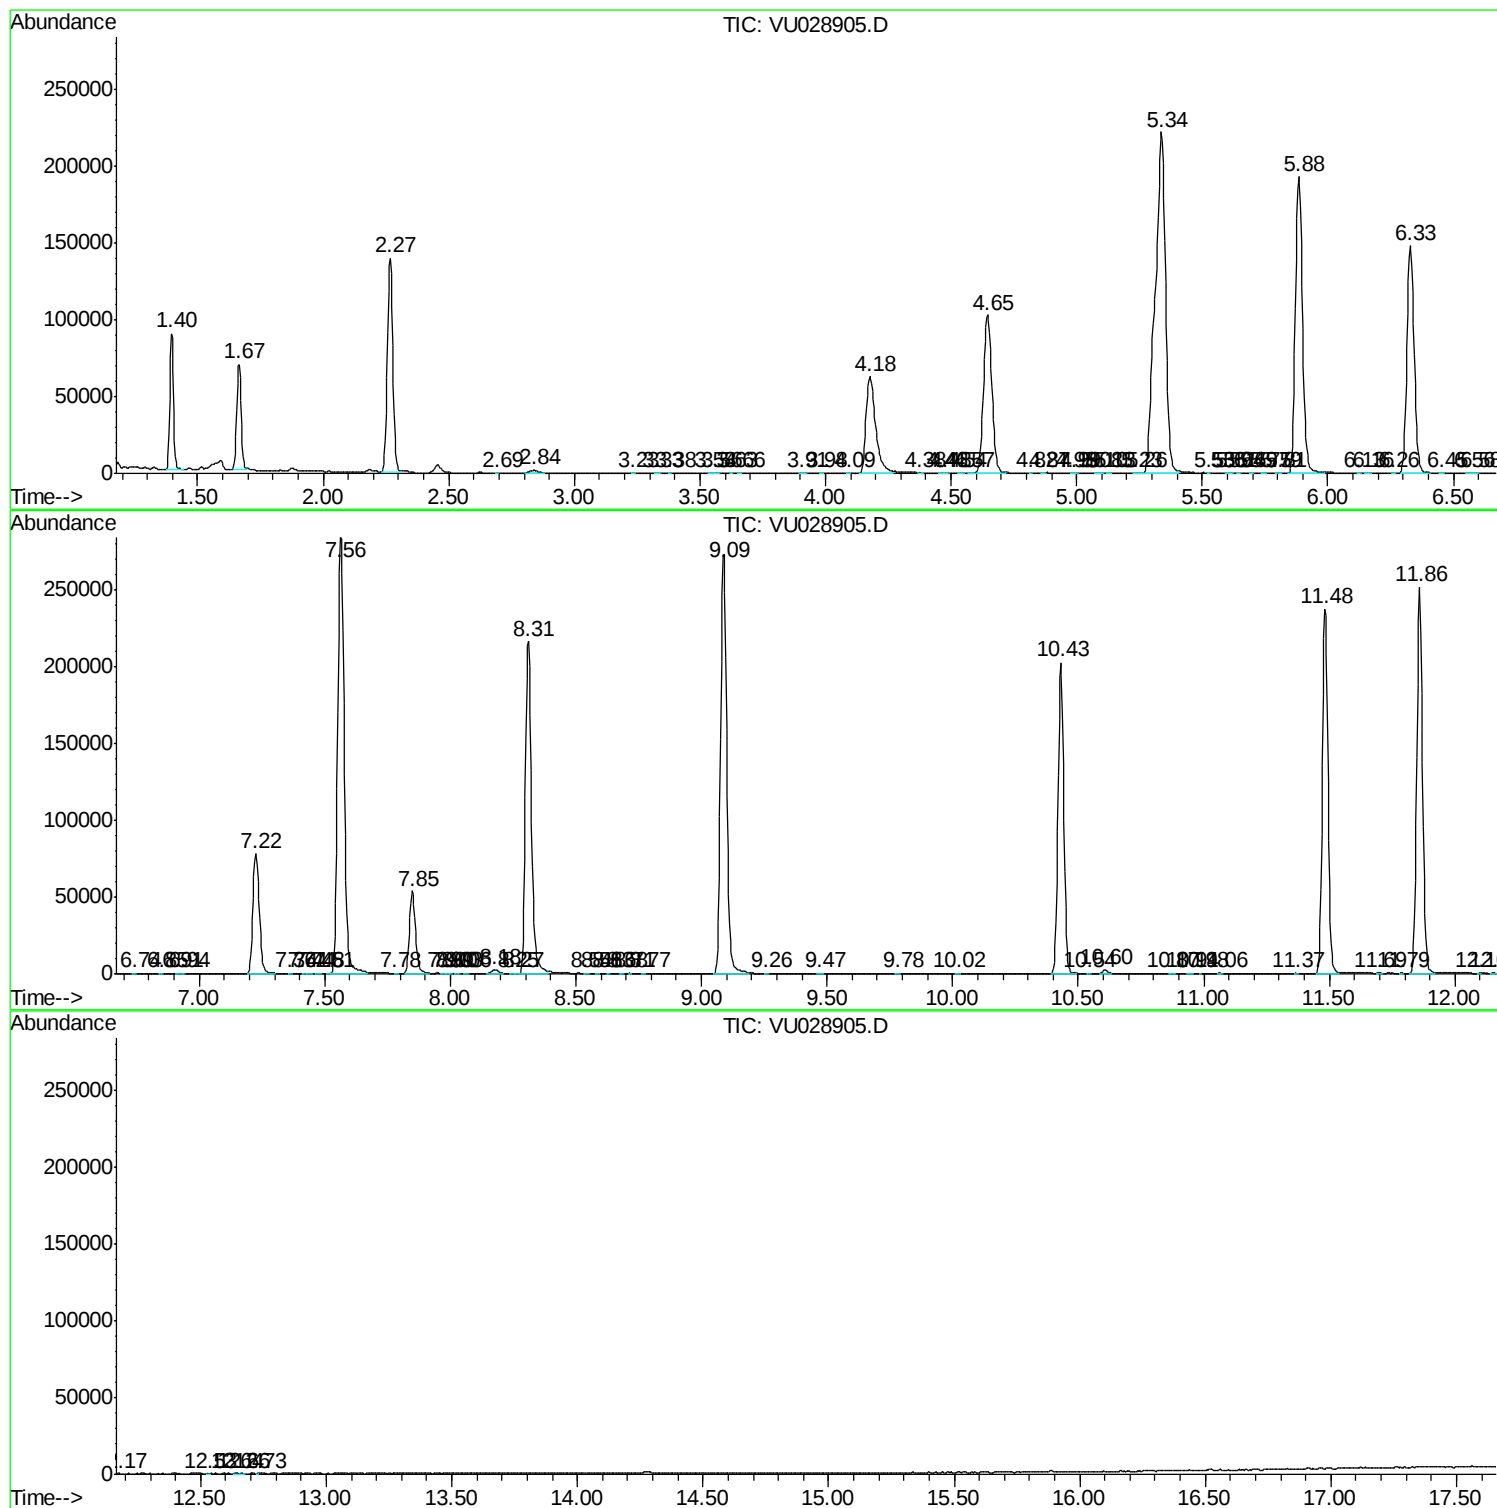

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU122118\
Data File : VU028905.D
Acq On : 22 Dec 2018 03:56
Operator : MD/SY
Sample : J6542-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122118\
Data File : VU028905.D
Acq On : 22 Dec 2018 03:56
Operator : MD/SY
Sample : J6542-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F65

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc