


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122118\
Data File : VU028859.D
Acq On : 21 Dec 2018 08:55
Operator : MD/SY
Sample : BFB99
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Title : VOC Analysis
Last Update : Fri Dec 28 00:46:50 2018

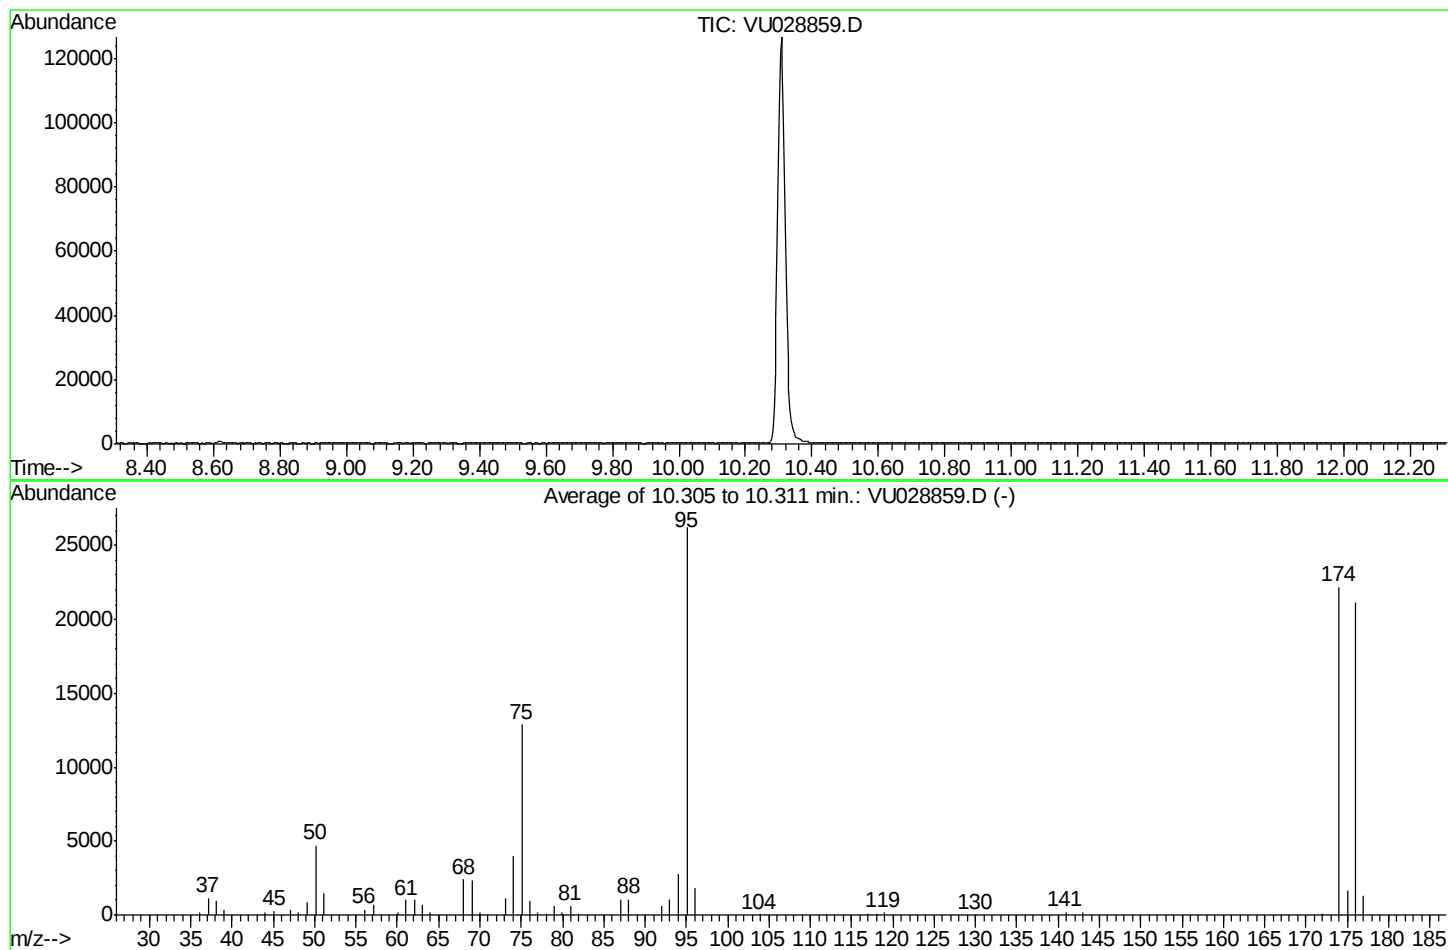

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	4687	PASS
75	95	30	80	49.2	12894	PASS
95	95	100	100	100.0	26229	PASS
96	95	5	9	6.8	1791	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	22173	PASS
175	174	5	9	7.3	1611	PASS
176	174	95	101	95.1	21096	PASS
177	176	5	9	6.0	1267	PASS

m/z	Abundance
36.00	139.0
37.10	1045.0
38.00	873.0
39.10	328.0
44.00	412.0
45.10	263.0
47.00	365.0
47.90	153.0
49.10	832.0
50.10	4351.0
51.00	1452.0
56.10	298.0
57.10	622.0
60.10	222.0
61.00	964.0
62.10	911.0
63.10	683.0
64.00	149.0
68.10	2263.0
69.10	2316.0
70.00	183.0
73.10	1146.0
74.10	3757.0
75.10	12273.0
76.10	910.0
76.90	186.0
78.00	111.0
79.00	577.0
79.90	194.0
81.00	575.0
82.00	132.0
87.10	1018.0
88.00	1038.0
92.00	577.0
93.00	972.0
94.00	2683.0
95.10	25128.0
96.10	1617.0
117.00	124.0
118.00	105.0
118.90	123.0
141.00	203.0
143.00	207.0
172.00	116.0
174.00	21840.0
175.00	1555.0
176.00	20808.0
177.00	1205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99

m/z	Abundance
36.00	161.0
37.10	1147.0
38.10	1009.0
39.10	292.0
44.00	374.0
45.10	255.0
47.00	312.0
48.00	160.0
49.10	946.0
50.10	4803.0
51.10	1421.0
56.00	394.0
57.10	721.0
60.00	182.0
61.10	1074.0
62.00	1083.0
63.10	783.0
64.00	166.0
68.00	2453.0
69.10	2273.0
70.00	249.0
73.00	1073.0
74.10	4148.0
75.10	13078.0
76.00	911.0
76.90	136.0
79.00	623.0
80.00	177.0
81.00	644.0
82.00	117.0
87.00	1027.0
88.00	1121.0
92.00	659.0
93.00	1089.0
94.10	2751.0
95.10	26456.0
96.10	1902.0
103.90	114.0
118.00	104.0
118.90	156.0
141.00	218.0
142.90	206.0
171.90	106.0
174.00	21808.0
175.00	1613.0
176.00	20608.0
177.00	1289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99

m/z	Abundance
36.00	140.0
37.10	1197.0
38.10	1007.0
39.00	303.0
44.00	414.0
45.10	275.0
47.00	342.0
47.90	179.0
49.10	923.0
50.10	4908.0
51.00	1573.0
56.10	350.0
57.10	718.0
60.10	213.0
61.10	1081.0
62.10	1055.0
63.10	743.0
64.00	179.0
68.10	2504.0
69.10	2416.0
70.00	222.0
73.00	1173.0
74.10	4149.0
75.10	13333.0
76.10	944.0
76.90	165.0
78.10	112.0
79.00	640.0
80.00	197.0
81.00	616.0
82.00	136.0
87.00	974.0
88.00	1075.0
92.00	669.0
93.00	1067.0
94.00	2805.0
95.10	27104.0
96.10	1856.0
103.90	113.0
117.00	121.0
118.00	114.0
118.90	155.0
130.00	105.0
140.90	213.0
143.00	210.0
172.00	112.0
174.00	22872.0
175.00	1667.0
176.00	21872.0
177.00	1308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99

m/z	Abundance
44.00	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99