

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122120\
 Data File : VU041708.D
 Acq On : 21 Dec 2020 18:17
 Operator : SY/MD
 Sample : L5162-11MSD
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB255MSD

Quant Time: Dec 22 02:53:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 22 02:49:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	126286	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	124857	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	53284	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	40025	4.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.00%
7) Chloroethane-d5	1.92	69	40572	5.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.20%
11) 1,1-Dichloroethene-d2	2.58	63	78432	4.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.20%
20) 2-Butanone-d5	4.65	46	178554	62.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.92%
24) Chloroform-d	5.08	84	87611	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
26) 1,2-Dichloroethane-d4	5.72	65	51233	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.80%
32) Benzene-d6	5.74	84	167875	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.70	67	56070	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.90	98	145128	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	8.19	79	24625	4.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.80%
46) 2-Hexanone-d5	8.64	63	152202	55.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.48%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	54066	5.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	54618	5.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Chloromethane	1.53	50	845	0.081	ug/L	97
10) 1,1,2-Trichloro-1,2,2-trif	2.58	101	590	0.068	ug/L #	22
12) 1,1-Dichloroethene	2.59	96	43158	5.038	ug/L	96
13) Acetone	2.66	43	16195	8.978	ug/L	80
21) 2-Butanone	4.74	43	3057	1.040	ug/L	91
25) Chloroform	5.11	83	13552	0.813	ug/L	93
27) 1,2-Dichloroethane	5.79	62	2466	0.218	ug/L #	73
31) Carbon tetrachloride	5.54	117	1779716	143.546	ug/L	99
33) Benzene	5.79	78	201831	5.054	ug/L	100
34) Trichloroethene	6.55	95	50174	5.000	ug/L	98
35) Methylcyclohexane	6.70	83	12743	0.786	ug/L #	19
37) 1,2-Dichloropropane	6.70	63	5812	0.569	ug/L #	88
38) Bromodichloromethane	7.12	83	824	0.065	ug/L #	85
39) cis-1,3-Dichloropropene	7.57	75	1263	0.083	ug/L #	65
42) Toluene	7.97	91	214815	5.211	ug/L	99
44) trans-1,3-Dichloropropene	8.19	75	1102	0.081	ug/L #	67
47) Tetrachloroethene	8.56	164	1322	0.188	ug/L #	85

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122120\
Data File : VU041708.D
Acq On : 21 Dec 2020 18:17
Operator : SY/MD
Sample : L5162-11MSD
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB255MSD

Quant Time: Dec 22 02:53:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 22 02:49:59 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
48) 2-Hexanone	8.64	43	19074	3.606	ug/L #	61
49) Dibromochloromethane	8.56	129	1471	0.170	ug/L #	10
51) Chlorobenzene	9.45	112	135748	5.297	ug/L	97
59) 1,2,3-Trichloropropane	11.81	75	6491	0.846	ug/L #	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122120\
Data File : VU041708.D
Acq On : 21 Dec 2020 18:17
Operator : SY/MD
Sample : L5162-11MSD
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB255MSD

Quant Time: Dec 22 02:53:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 22 02:49:59 2020
Response via : Initial Calibration




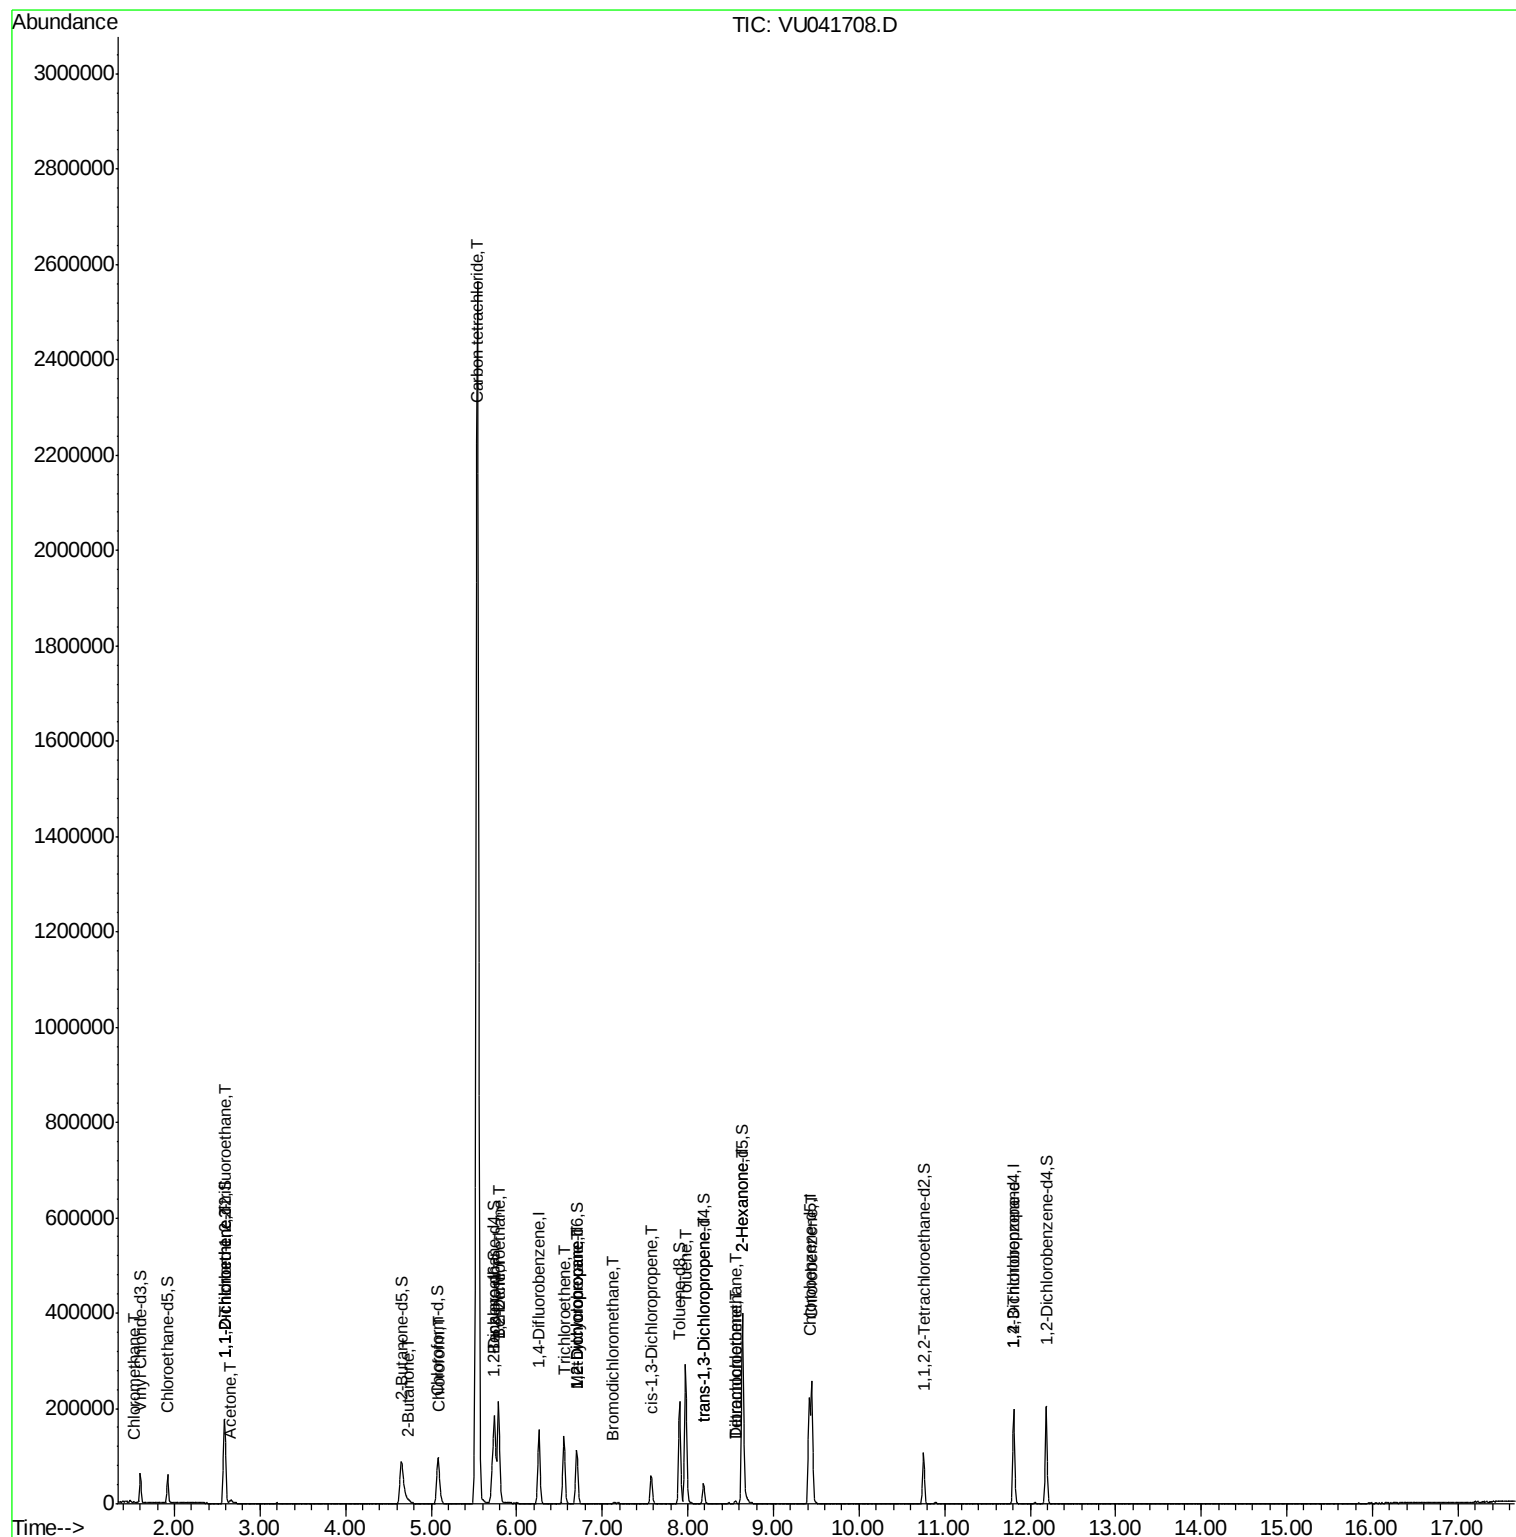


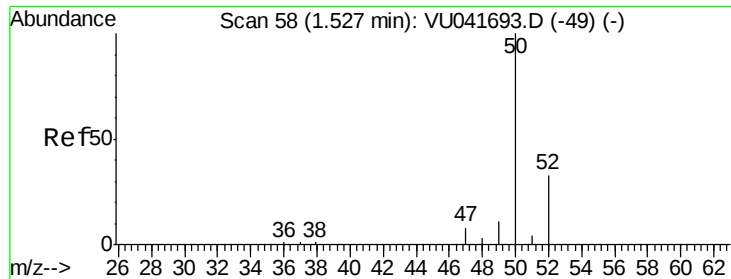

#3
 Chloromethane
 Concen: 0.081 ug/L
 RT: 1.53 min Scan# 58
 Delta R.T. -0.00 min
 Lab File: VU041708.D
 Acq: 21 Dec 2020 18:17




Instrument :
 MSVOA_U
 ClientSampleId :
 GB255MSD


Tot Ion: 50 Resp: 845
 Ion Ratio Lower Upper
 50 100
 52 32.8 24.1 44.8

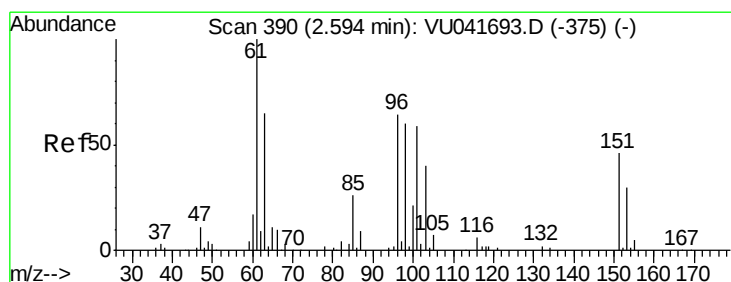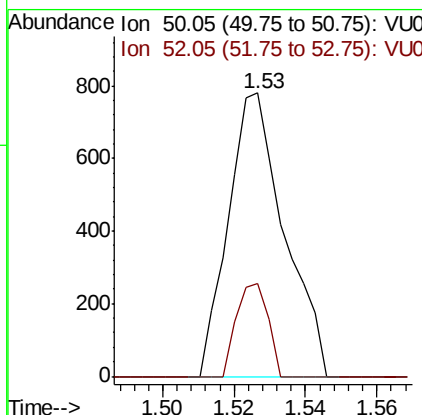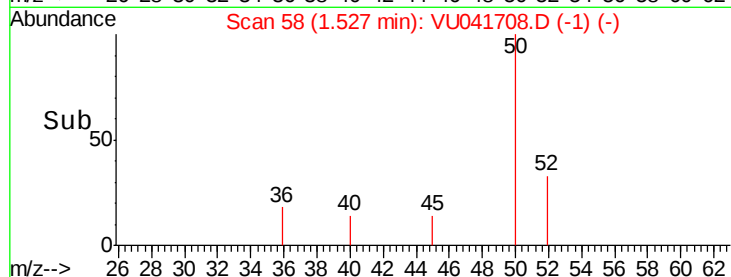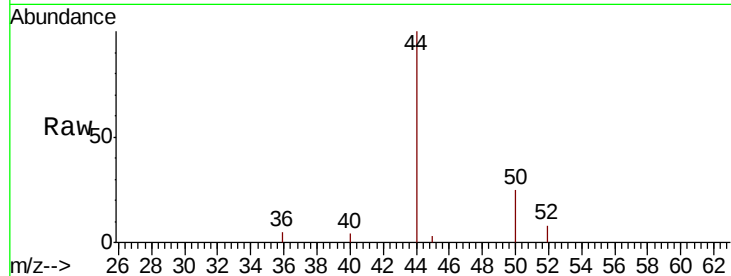

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.068 ug/L
 RT: 2.58 min Scan# 386
 Delta R.T. -0.01 min
 Lab File: VU041708.D
 Acq: 21 Dec 2020 18:17

Tgt Ion:101 Resp: 590
 Ion Ratio Lower Upper
 101 100
 85 0.0 33.6 50.4#
 151 0.0 56.2 84.4#


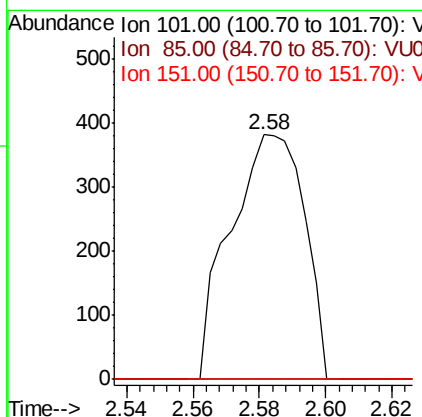
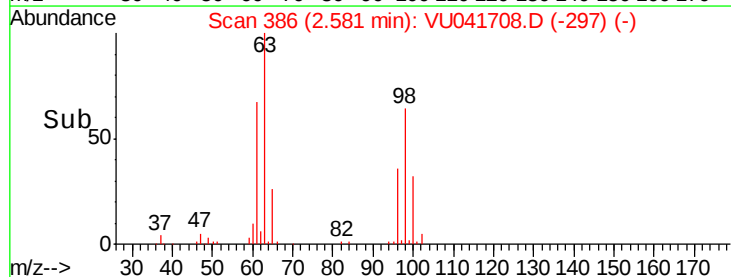
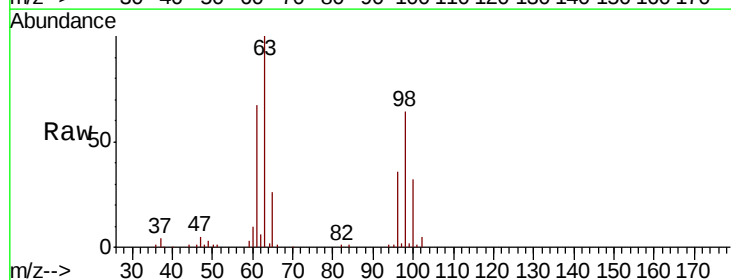


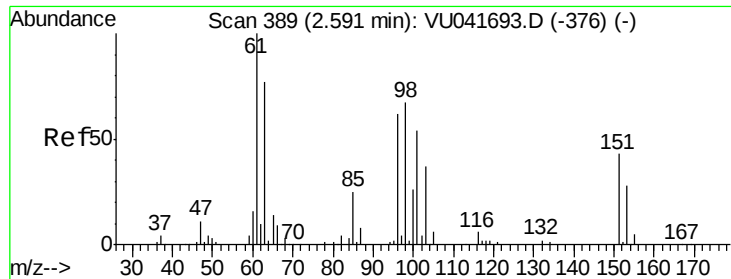

#12
 1,1-Dichloroethene
 Concen: 5.038 ug/L
 RT: 2.59 min Scan# 389
 Delta R.T. -0.00 min
 Lab File: VU041708.D
 Acq: 21 Dec 2020 18:17




Instrument :
 MSVOA_U
 ClientSampleId :
 GB255MSD


Tot Ion	Resp	Lower	Upper
96	100		
61	167.2	123.8	230.0
63	115.0	81.0	150.4

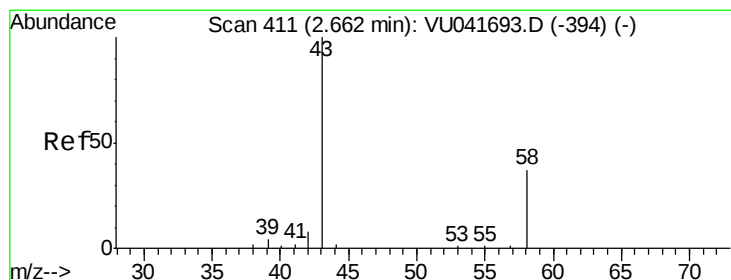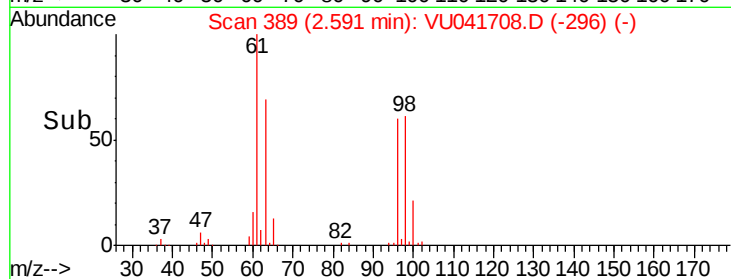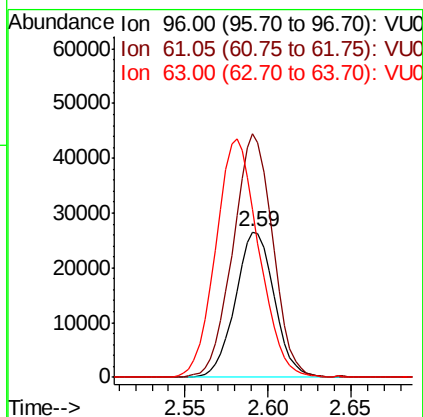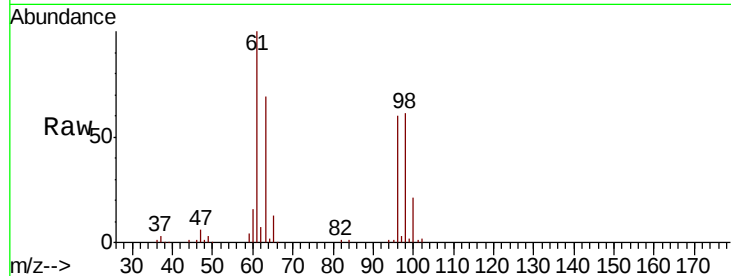

#13
 Acetone
 Concen: 8.978 ug/L
 RT: 2.66 min Scan# 409
 Delta R.T. -0.01 min
 Lab File: VU041708.D
 Acq: 21 Dec 2020 18:17

Tgt Ion	Resp	Lower	Upper
43	100		
58	25.0	0.0	73.2

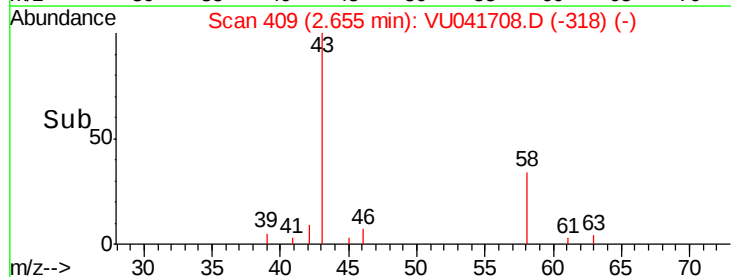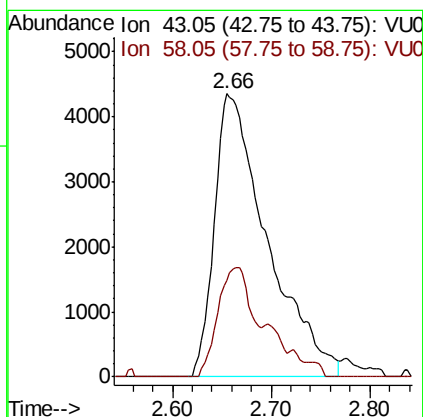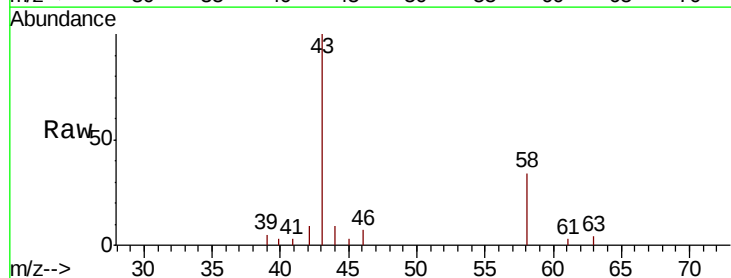

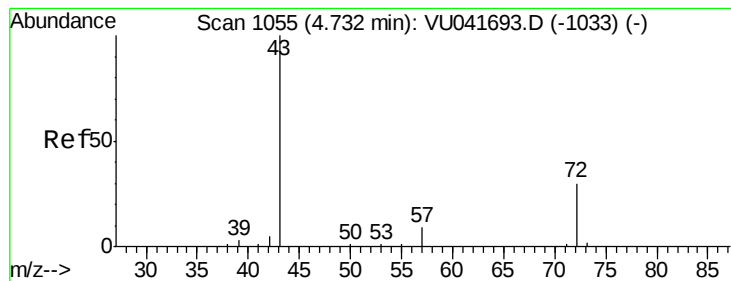

#21

2-Butanone

Concen: 1.040 ug/L

RT: 4.74 min Scan# 1058

Delta R.T. 0.01 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :


GB255MSD

Tot Ion: 43 Resp: 3057




Ion Ratio Lower Upper

43 100

72 34.0 14.6 44.0

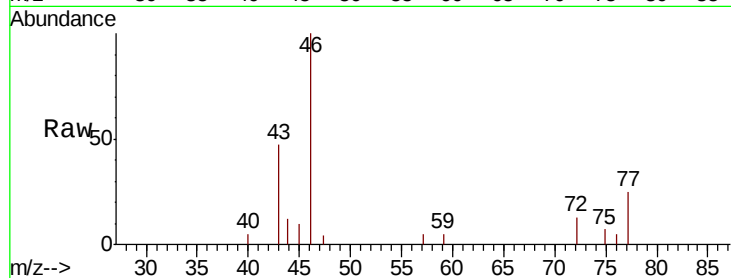

Abundance Ion 43.05 (42.75 to 43.75): VU041708.D (-962) (-)

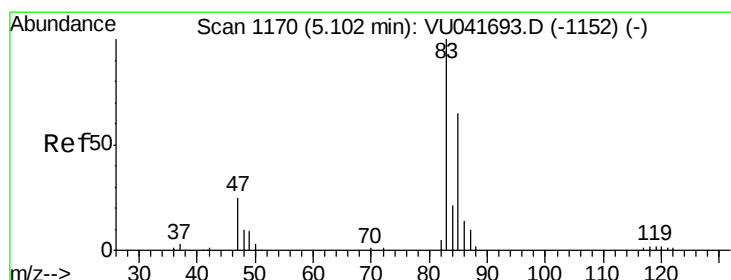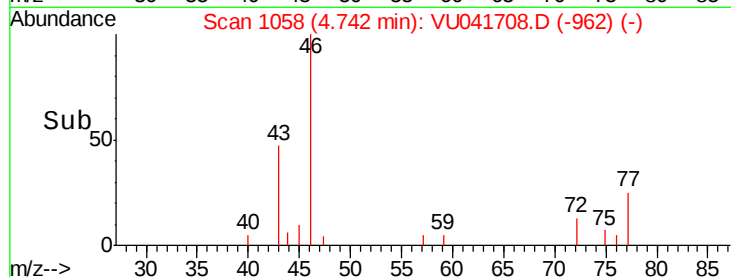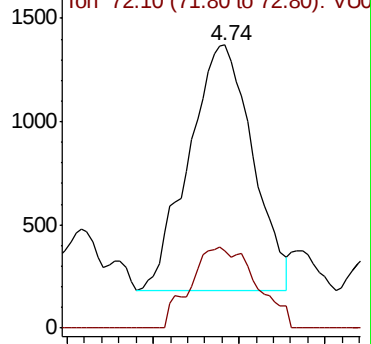

#25

Chloroform

Concen: 0.813 ug/L

RT: 5.11 min Scan# 1171

Delta R.T. 0.00 min

Lab File: VU041708.D


Acq: 21 Dec 2020 18:17

Tgt Ion: 83 Resp: 13552



Ion Ratio Lower Upper


83 100

85 68.7 44.2 82.0

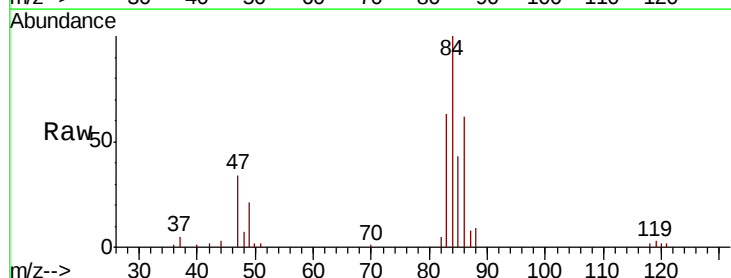

Abundance Ion 83.05 (82.75 to 83.75): VU041708.D (-1077) (-)

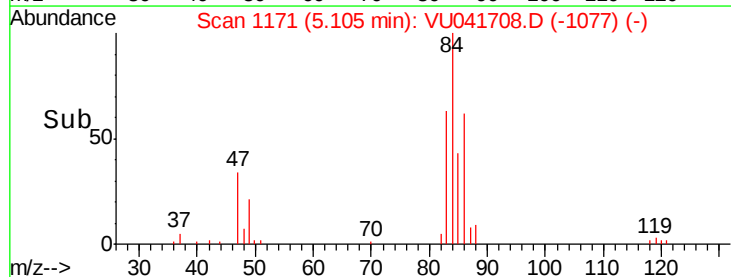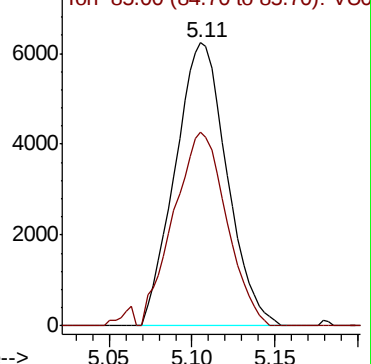

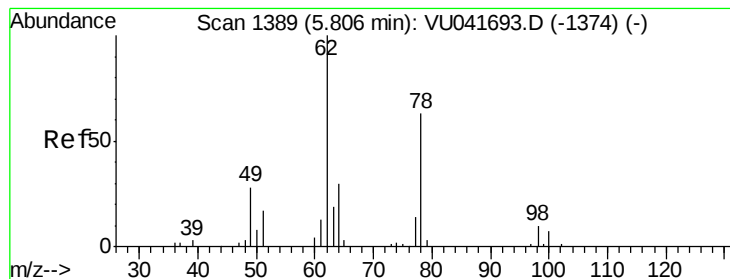

#27

1,2-Dichloroethane

Concen: 0.218 ug/L

RT: 5.79 min Scan# 1385

Delta R.T. -0.01 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :


GB255MSD

Tot Ion: 62 Resp: 2466

Ion Ratio Lower Upper

62 100

98 0.0 8.2 12.2#

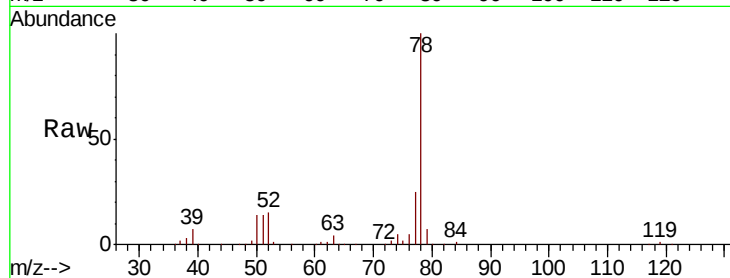

Abundance Ion 62.00 (61.70 to 62.70): VU041693.D (-1374) (-)

Ion 98.05 (97.75 to 98.75): VU041693.D (-1374) (-)

5.79

1200

1000

800

600



400

200

0

5.75 5.80 5.85

Time-->

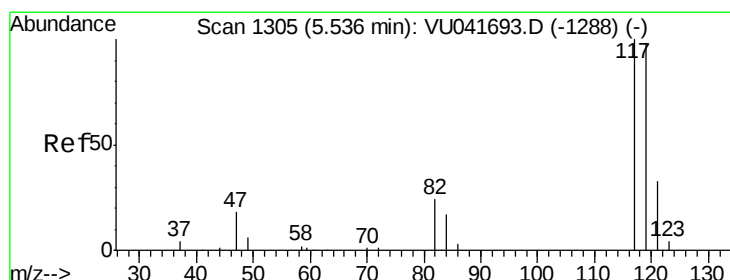

#31

Carbon tetrachloride

Concen: 143.546 ug/L

RT: 5.54 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU041708.D


Acq: 21 Dec 2020 18:17

Tgt Ion: 117 Resp: 1779716

Ion Ratio Lower Upper

117 100

119 96.6 76.2 114.2

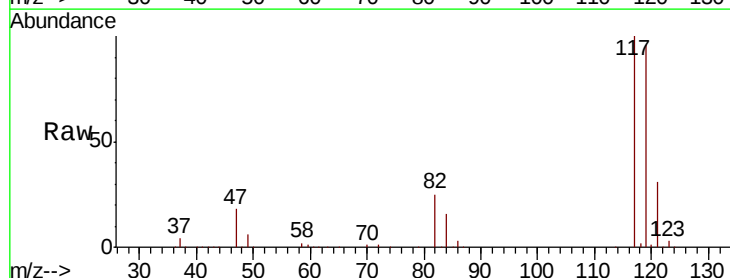

Abundance Ion 116.90 (116.60 to 117.60): VU041693.D (-1288) (-)

Ion 118.90 (118.60 to 119.60): VU041693.D (-1288) (-)

5.54

800000

600000


400000


200000

0

5.40 5.50 5.60 5.70

Time-->



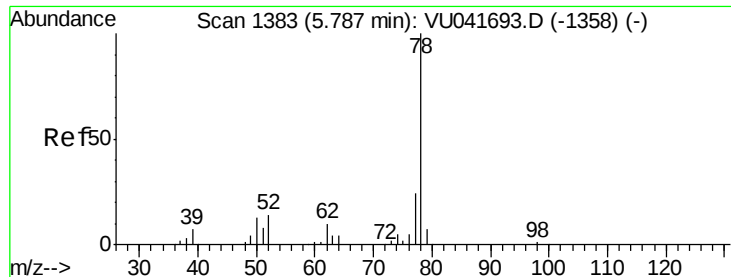

#33

Benzene

Concen: 5.054 ug/L

RT: 5.79 min Scan# 1383

Delta R.T. -0.00 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17


Instrument :

MSVOA_U




ClientSampleId :

GB255MSD

Tgt Ion: 78 Resp: 201831

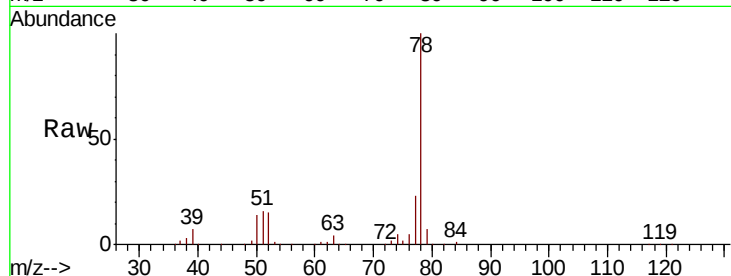

Abundance Ion 78.10 (77.80 to 78.80): VU0

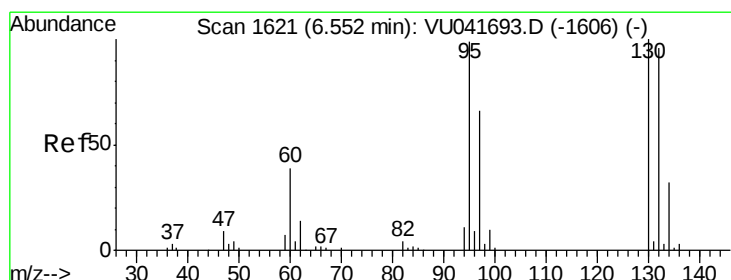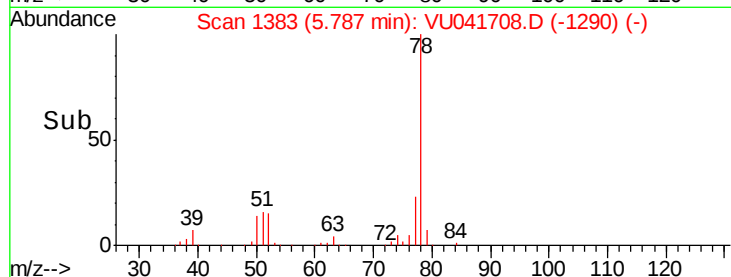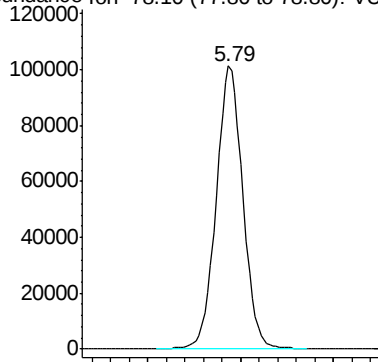

#34

Trichloroethene

Concen: 5.000 ug/L

RT: 6.55 min Scan# 1621

Delta R.T. -0.00 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Tgt Ion: 95 Resp: 50174




Ion	Ratio	Lower	Upper
95	100		
97	63.8	43.9	81.5
132	86.9	63.1	117.3
130	97.3	67.4	125.2


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

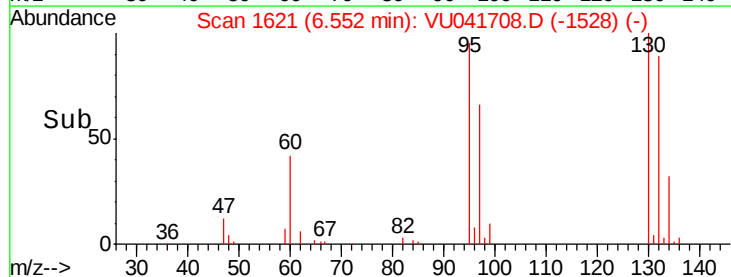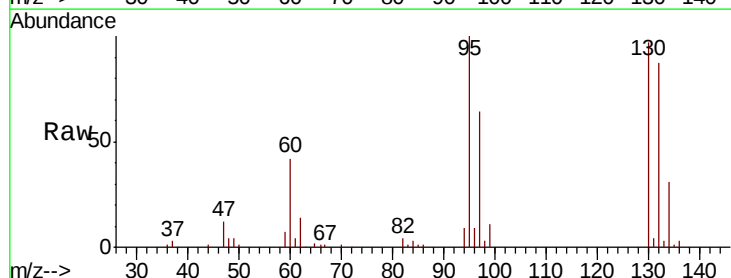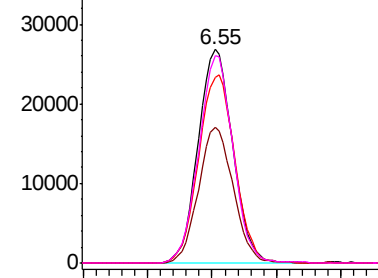

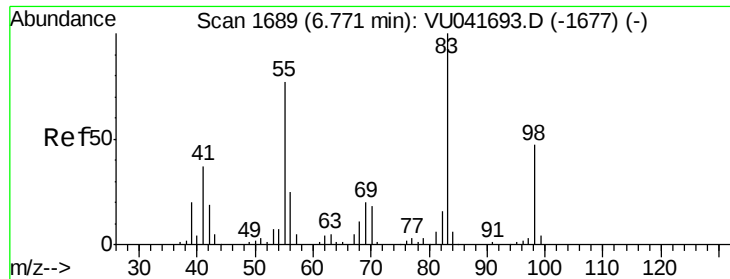

#35

Methylcyclohexane

Concen: 0.786 ug/L

RT: 6.70 min Scan# 1668

Delta R.T. -0.07 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :

GB255MSD


Tot Ion: 83 Resp: 12743

Ion Ratio Lower Upper

83 100

55 0.0 61.2 91.8#




98 0.9 36.6 54.8#

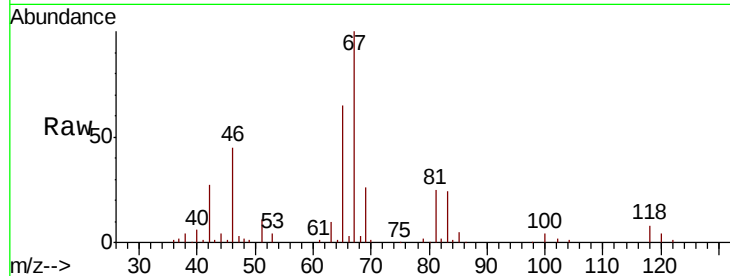

Abundance Ion 83.15 (82.85 to 83.85): VU0

Ion 55.10 (54.80 to 55.80): VU0

Ion 98.15 (97.85 to 98.85): VU0

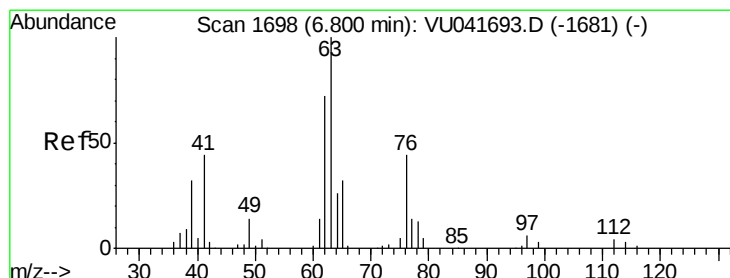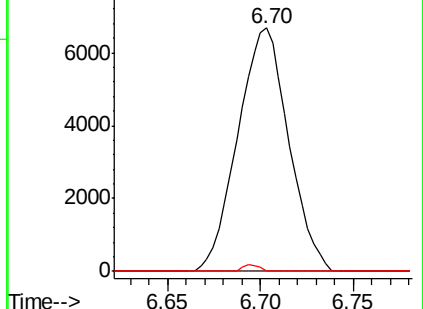

#37

1,2-Dichloropropane

Concen: 0.569 ug/L

RT: 6.70 min Scan# 1667

Delta R.T. -0.10 min

Lab File: VU041708.D


Acq: 21 Dec 2020 18:17

Tgt Ion: 63 Resp: 5812

Ion Ratio Lower Upper



63 100


112 0.0 3.1 4.7#

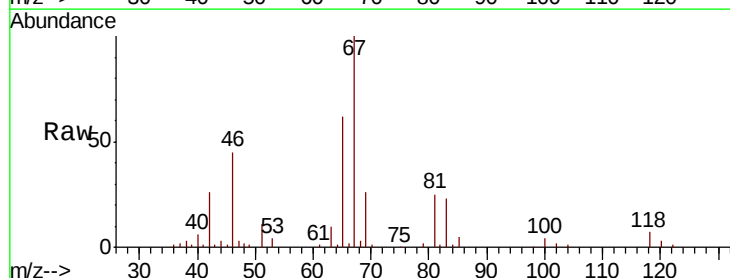

Abundance Ion 63.10 (62.80 to 63.80): VU0

Ion 112.10 (111.80 to 112.80): V

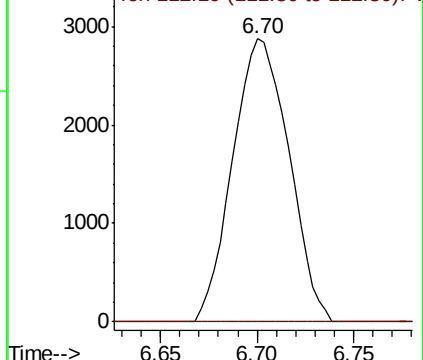

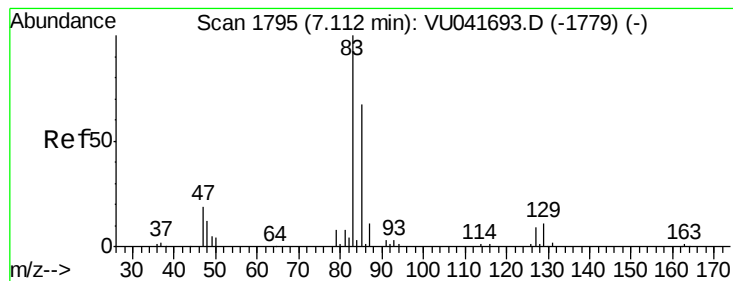

#38

Bromodichloromethane

Concen: 0.065 ug/L

RT: 7.12 min Scan# 1797

Delta R.T. 0.01 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :

GB255MSD


Tot Ion: 83 Resp: 824

Ion Ratio Lower Upper

83 100

85 53.9 45.5 84.5




127 0.0 7.0 10.6#

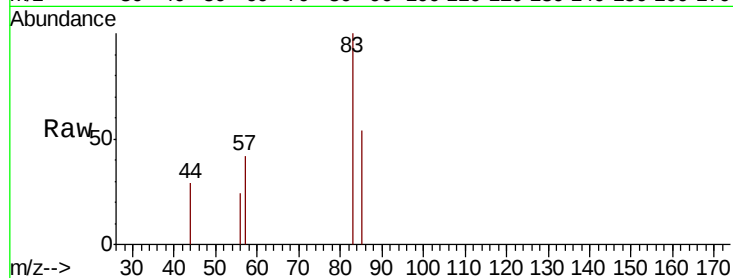

Abundance Ion 82.95 (82.65 to 83.65): VU041708.D (-1702) (-)

Ion 85.00 (84.70 to 85.70): VU041708.D (-1702) (-)

Ion 126.90 (126.60 to 127.60): VU041708.D (-1702) (-)

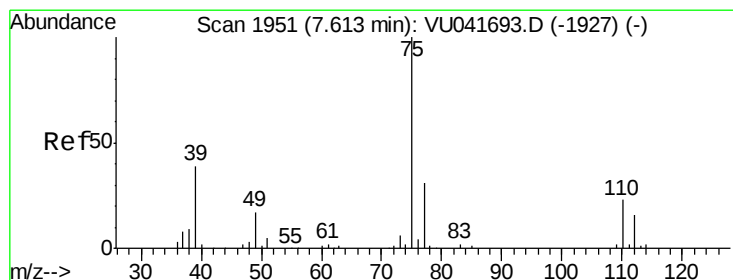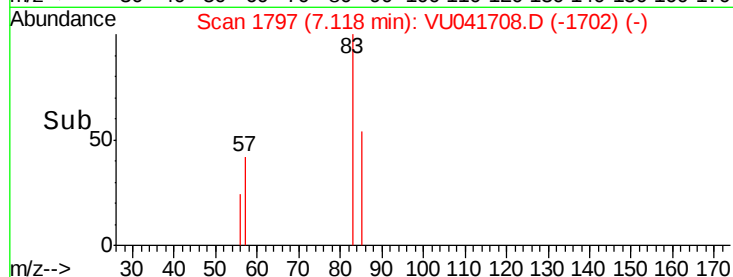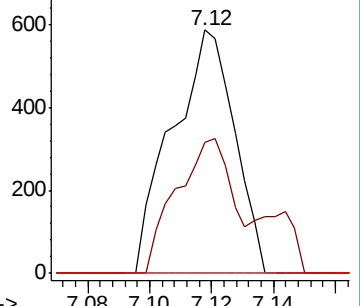

#39

cis-1,3-Dichloropropene

Concen: 0.083 ug/L

RT: 7.57 min Scan# 1938

Delta R.T. -0.04 min

Lab File: VU041708.D


Acq: 21 Dec 2020 18:17

Tgt Ion: 75 Resp: 1263

Ion Ratio Lower Upper

75 100

77 51.2 22.3 41.3#

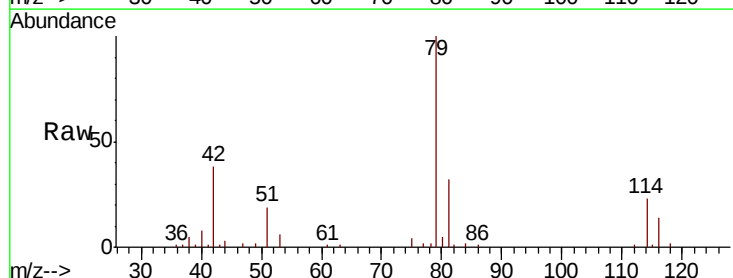

Abundance Ion 75.05 (74.75 to 75.75): VU041708.D (-1858) (-)

Ion 77.05 (76.75 to 77.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)


Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

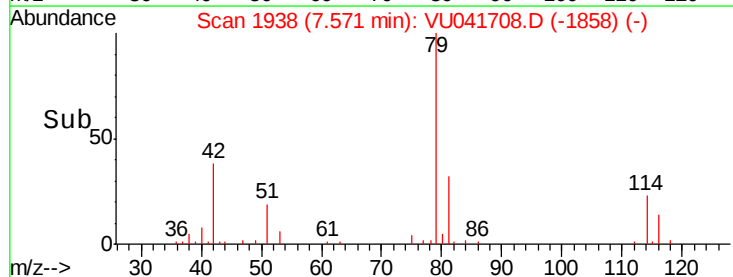

Abundance Ion 75.05 (74.75 to 75.75): VU041708.D (-1858) (-)

Ion 77.05 (76.75 to 77.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)


Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

Ion 114.05 (113.75 to 114.75): VU041708.D (-1858) (-)

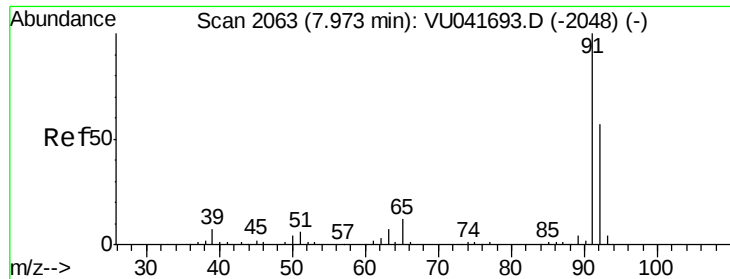

#42

Toluene

Concen: 5.211 ug/L

RT: 7.97 min Scan# 2063

Delta R.T. -0.00 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :


GB255MSD

Tot Ion: 91 Resp: 214815

Ion Ratio Lower Upper

91 100

92 58.0 40.0 74.2

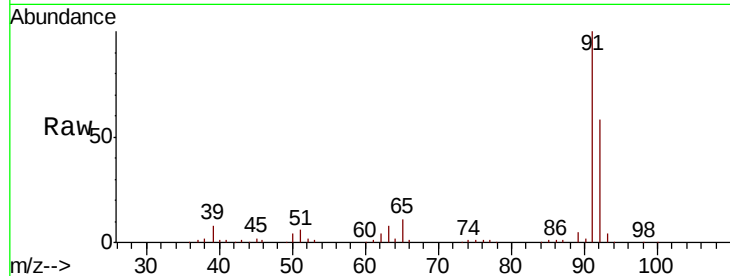

Abundance Ion 91.15 (90.85 to 91.85): VU041708.D (-1970) (-)

Ion 92.15 (91.85 to 92.85): VU041708.D (-1970) (-)

7.97

150000



100000

50000

0

7.90 8.00 8.10

Time-->

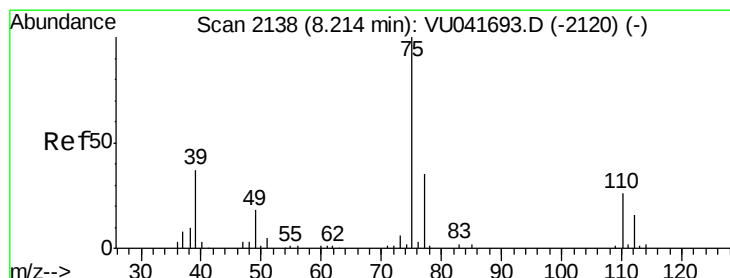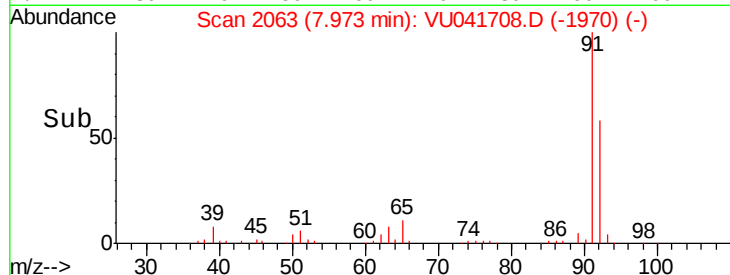

#44

trans-1,3-Dichloropropene

Concen: 0.081 ug/L

RT: 8.19 min Scan# 2130

Delta R.T. -0.03 min

Lab File: VU041708.D


Acq: 21 Dec 2020 18:17

Tgt Ion: 75 Resp: 1102

Ion Ratio Lower Upper

75 100

77 53.1 23.8 44.2#

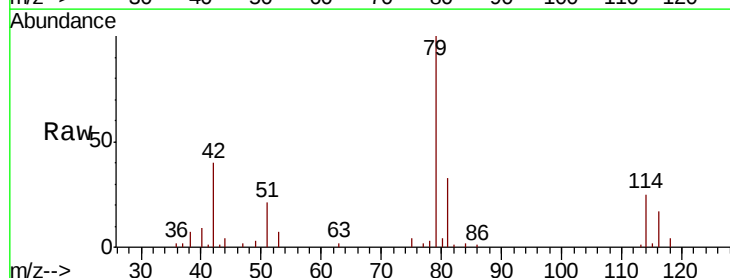

Abundance Ion 75.05 (74.75 to 75.75): VU041708.D (-2045) (-)

Ion 77.05 (76.75 to 77.75): VU041708.D (-2045) (-)

8.19

600


400


200

0

8.14 8.16 8.18 8.20 8.22

Time-->







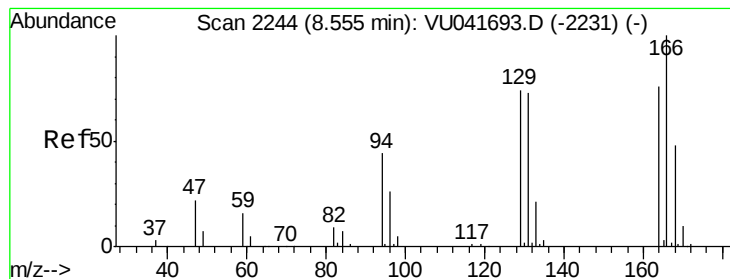

#47
Tetrachloroethene
Concen: 0.188 ug/L
RT: 8.56 min Scan# 2245
Delta R.T. 0.00 min
Lab File: VU041708.D
Acq: 21 Dec 2020 18:17




Instrument :
MSVOA_U
ClientSampleId :
GB255MSD


Tot Ion:	164	Resp:	1322
Ion	Ratio	Lower	Upper
164	100		
129	117.0	72.2	134.0
131	124.9	66.9	124.3#
166	132.6	89.6	166.4

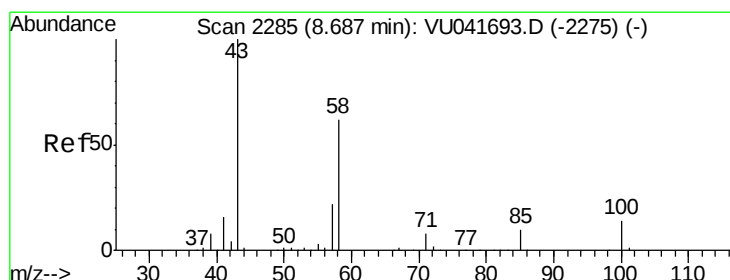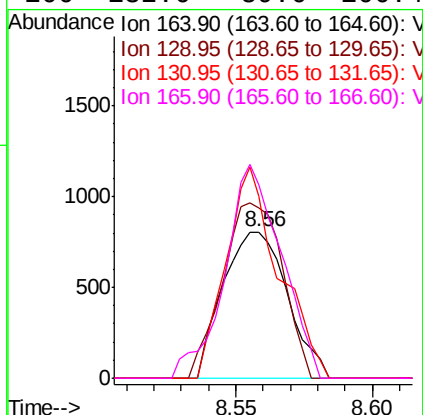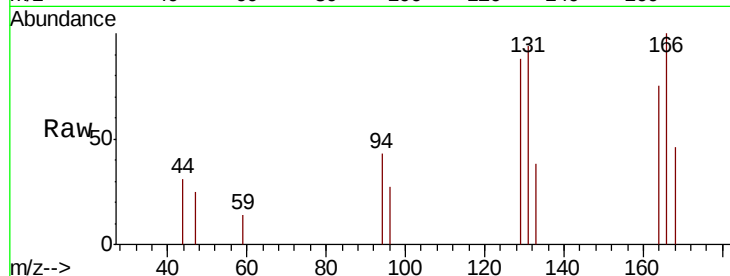

#48
2-Hexanone
Concen: 3.606 ug/L
RT: 8.64 min Scan# 2270
Delta R.T. -0.05 min
Lab File: VU041708.D
Acq: 21 Dec 2020 18:17

Tgt Ion:	43	Resp:	19074
Ion	Ratio	Lower	Upper
43	100		
58	21.7	47.9	71.9#
57	24.8	16.5	24.7#
100	0.6	9.4	14.2#

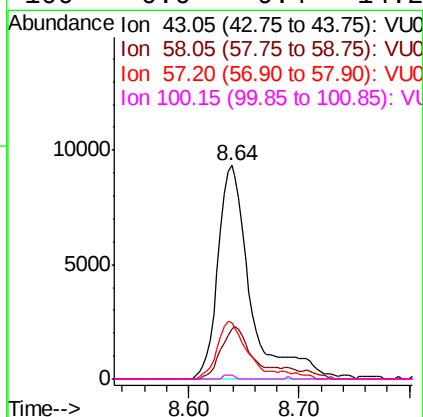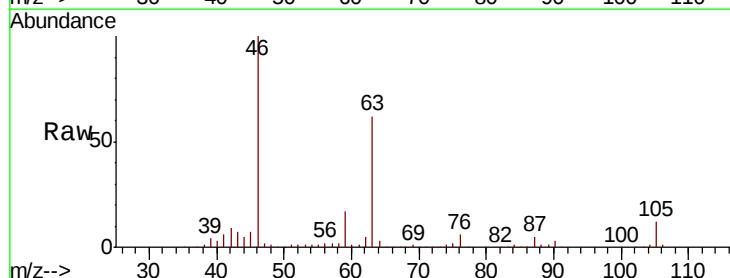



#49

Dibromochloromethane

Concen: 0.170 ug/L

RT: 8.56 min Scan# 2244

Delta R.T. -0.26 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :


GB255MSD

Tot Ion:129 Resp: 1471

Ion Ratio Lower Upper

129 100

127 0.0 54.7 101.7#

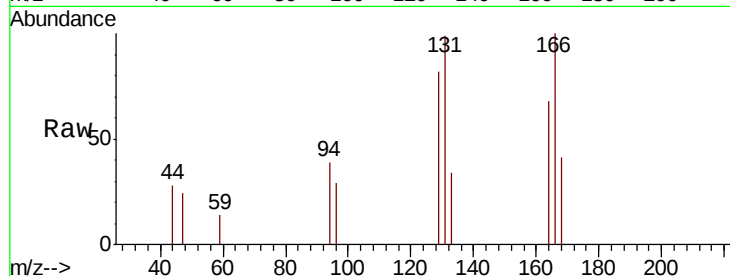

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

8.56

1000

800

600



400

200

0

8.52 8.54 8.56 8.58

Time-->

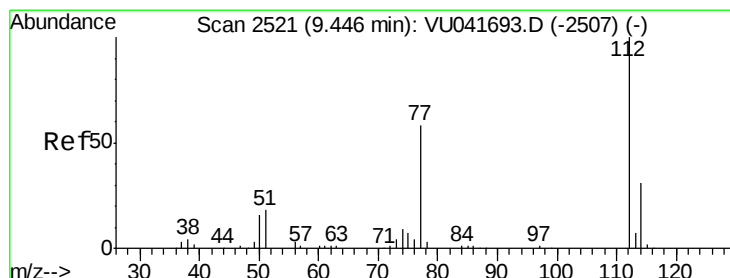

#51

Chlorobenzene

Concen: 5.297 ug/L

RT: 9.45 min Scan# 2522

Delta R.T. 0.00 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17


Tgt Ion:112 Resp: 135748

Ion Ratio Lower Upper

112 100

114 31.3 22.7 42.3

77 58.6 49.1 73.7

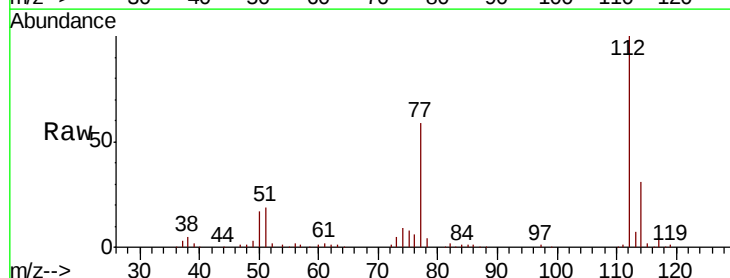

Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VU0

9.45

100000

80000

60000


40000


20000

0

9.35 9.40 9.45 9.50 9.55

Time-->



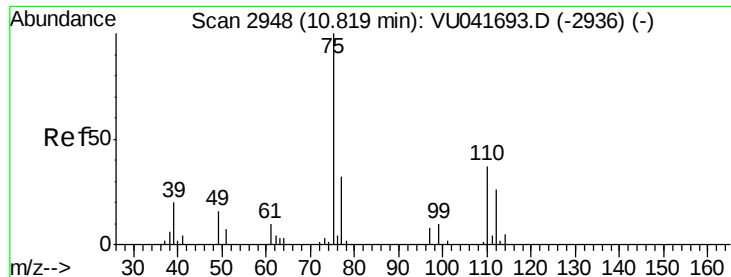

#59

1,2,3-Trichloropropane

Concen: 0.846 ug/L

RT: 11.81 min Scan# 3255

Delta R.T. 0.99 min

Lab File: VU041708.D

Acq: 21 Dec 2020 18:17

Instrument :

MSVOA_U

ClientSampleId :

GB255MSD

Tot Ion: 75 Resp: 6491

Ion Ratio Lower Upper

75 100

77 0.0 26.2 39.2#

