

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122120\
 Data File : VU041692.D
 Acq On : 21 Dec 2020 08:54
 Operator : SY/MD
 Sample : BFB27
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
 MSVOA_U
 ClientSampleId :
 GB256

Manual Integrations
 APPROVED

MMDadoda
 12/23/2020 11:30:45 AM

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Dec 22 05:59:09 2020

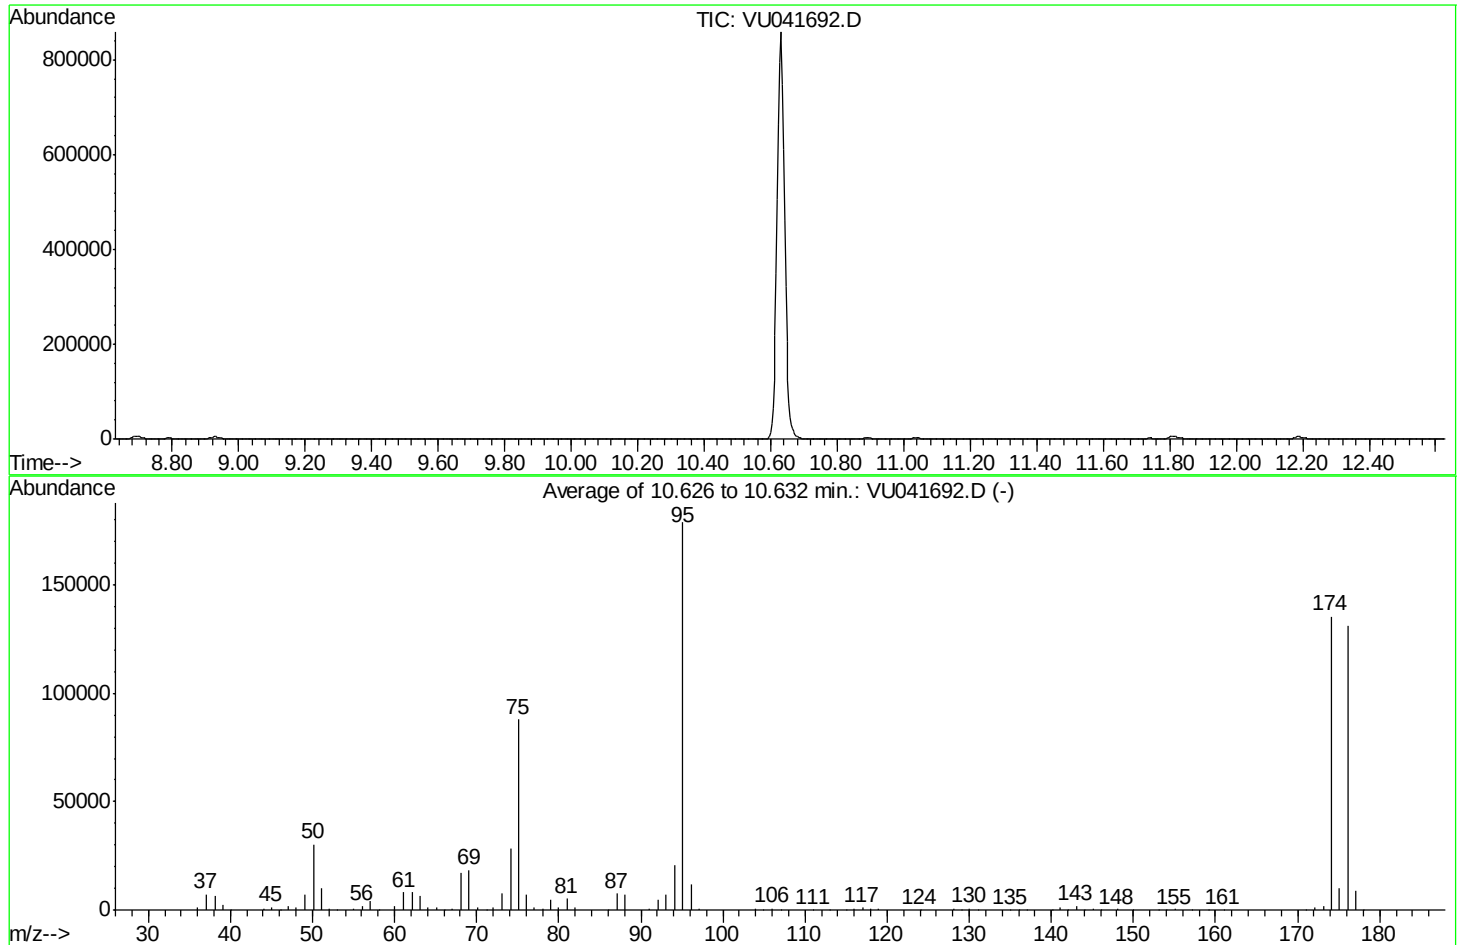

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	30242	PASS
75	95	30	80	49.2	87970	PASS
95	95	100	100	100.0	178901	PASS
96	95	5	9	6.6	11837	PASS
173	174	0.00	2	1.4	1925	PASS
174	95	50	120	75.7	135501	PASS
175	174	5	9	7.4	10006	PASS
176	174	95	101	96.9	131328	PASS
177	176	5	9	6.7	8763	PASS

m/z	Abundance
36.00	1270.0
37.00	7377.0
38.10	6134.0
39.10	2731.0
40.10	190.0
44.10	1132.0
45.00	1193.0
46.00	162.0
47.10	2153.0
48.00	1031.0
49.10	6535.0
50.10	29624.0
51.10	9938.0
52.00	473.0
52.90	176.0
55.00	398.0
56.00	1822.0
57.10	3980.0
60.00	1627.0
61.10	7971.0
62.10	7776.0
63.10	6504.0
64.00	1008.0
65.10	1075.0
66.00	192.0
67.00	407.0
68.10	16101.0
69.10	18016.0
70.10	882.0
72.10	1049.0
73.10	7248.0
74.10	27376.0
75.10	84416.0
76.10	6631.0
77.00	1116.0
78.00	885.0
79.00	4613.0
80.00	1455.0
81.00	5000.0
81.90	953.0
86.00	206.0
87.10	7506.0
88.10	6681.0
91.00	596.0
92.10	4468.0
93.10	7447.0
94.10	19784.0
95.10	171712.0
96.10	11386.0
97.10	338.0
104.00	696.0
105.00	217.0
106.00	697.0
107.00	142.0
111.00	182.0
113.00	108.0
114.90	250.0
116.00	628.0
117.00	1124.0
118.00	637.0
119.00	822.0
128.10	473.0
129.10	320.0
130.00	707.0
131.00	191.0
135.00	250.0
137.00	177.0
140.20	102.0
141.00	1244.0
142.00	193.0
143.10	1774.0
144.00	163.0
145.10	486.0
146.10	256.0
148.00	284.0
150.00	221.0
153.00	119.0
154.00	129.0
155.10	435.0
157.10	216.0
159.10	153.0
161.00	165.0
171.00	241.0
172.10	1294.0
173.10	1800.0
174.10	127400.0
175.10	9446.0
176.10	123200.0
177.10	8656.0
178.00	209.0

Instrument :
MSVOA_U
ClientSampleId :
GB256

Manual Integrations
APPROVED

MMDadoda
12/23/2020 11:30:45 AM

m/z	Abundance
36.00	1245.0
37.00	7402.0
38.10	6972.0
39.10	2672.0
40.00	144.0
44.10	1117.0
45.00	1295.0
46.10	175.0
47.10	2092.0
48.00	1088.0
49.10	7361.0
50.10	31352.0
51.10	10176.0
52.00	480.0
52.90	152.0
54.90	450.0
56.10	2048.0
57.10	4300.0
58.10	114.0
60.00	1656.0
61.10	8415.0
62.10	8339.0
63.10	6500.0
64.00	1034.0
65.10	1041.0
66.00	145.0
67.10	556.0
68.10	17760.0
69.10	19328.0
70.10	956.0
71.20	102.0
72.00	1051.0
73.10	7913.0
74.10	29648.0
75.10	90832.0
76.10	7218.0
77.00	1266.0
78.00	929.0
79.00	4862.0
80.00	1446.0
81.00	5261.0
81.90	1033.0
86.00	222.0
87.10	7815.0
88.00	7153.0
91.00	735.0
92.10	4816.0
93.10	7629.0
94.10	21424.0
95.10	185152.0
96.10	12353.0
97.10	407.0
104.00	784.0
104.90	242.0
106.00	805.0
107.00	189.0
111.00	193.0
113.00	100.0
114.90	231.0
116.00	658.0
117.00	1222.0
118.00	691.0
119.00	913.0
128.10	482.0
129.10	305.0
130.00	731.0
131.10	201.0
135.00	246.0
136.00	103.0
137.00	193.0
140.20	104.0
141.10	1487.0
142.00	247.0
143.10	1893.0
144.00	187.0
145.10	477.0
146.00	337.0
148.10	308.0
150.00	181.0
153.10	115.0
154.00	141.0
155.10	454.0
157.10	212.0
159.10	153.0
161.00	173.0
171.00	194.0
172.10	1414.0
173.20	1995.0
174.10	139584.0
175.10	10273.0
176.10	135616.0
177.10	9102.0

Instrument :
MSVOA_U
ClientSampleId :
GB256

Manual Integrations
APPROVED

MMDadoda
12/23/2020 11:30:45 AM

178.00

233.0

Instrument :
MSVOA_U
ClientSampleId :
GB256

Manual Integrations
APPROVED
MMDadoda
12/23/2020 11:30:45 AM

m/z	Abundance
36.00	1197.0
37.00	6733.0
38.10	6881.0
39.00	2528.0
40.00	115.0
44.10	989.0
45.00	1155.0
46.10	137.0
47.10	1788.0
48.00	1045.0
49.10	7371.0
50.10	29752.0
51.10	9425.0
52.00	471.0
52.90	101.0
55.00	424.0
56.10	2180.0
57.10	4234.0
58.00	162.0
60.00	1541.0
61.10	7918.0
62.10	8155.0
63.10	6134.0
64.10	934.0
65.10	1013.0
67.10	612.0
68.10	17512.0
69.10	18520.0
70.10	976.0
72.10	941.0
73.10	7771.0
74.10	28848.0
75.10	88664.0
76.10	7216.0
77.10	1279.0
78.00	849.0
79.00	4602.0
80.00	1412.0
81.00	4950.0
82.00	995.0
86.00	257.0
87.10	7291.0
88.00	7164.0
91.00	748.0
92.10	4842.0
93.10	6993.0
94.10	20952.0
95.10	179840.0
96.10	11774.0
97.10	407.0
104.00	803.0
104.90	248.0
106.00	807.0
107.00	211.0
111.00	148.0
115.00	195.0
115.90	625.0
117.00	1128.0
118.00	693.0
118.90	943.0
124.00	100.0
128.00	438.0
129.10	251.0
130.00	714.0
131.10	231.0
135.10	218.0
137.10	222.0
141.10	1509.0
142.00	297.0
143.00	1741.0
144.00	183.0
145.10	390.0
146.00	356.0
148.10	372.0
150.00	121.0
153.10	117.0
154.00	112.0
155.00	452.0
157.10	204.0
159.10	154.0
161.00	221.0
171.10	156.0
172.10	1478.0
173.20	1980.0
174.10	139520.0
175.10	10300.0
176.10	135168.0
177.10	8532.0
178.00	217.0

Instrument :
MSVOA_U
ClientSampleId :
GB256

Manual Integrations
APPROVED

MMDadoda
12/23/2020 11:30:45 AM

m/z	Abundance
43.90	215.0

Instrument :
MSVOA_U
ClientSampleId :
GB256

Manual Integrations
APPROVED

MMDadoda
12/23/2020 11:30:45 AM