

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122120\
 Data File : VU041698.D
 Acq On : 21 Dec 2020 14:02
 Operator : SY/MD
 Sample : L5148-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB1T8

Quant Time: Dec 22 03:19:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 22 02:49:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	134121	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	139116	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	64567	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	44827	4.28	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.60%
7) Chloroethane-d5	1.92	69	43757	5.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.80%
11) 1,1-Dichloroethene-d2	2.58	63	61667	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	4.65	46	177582	58.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.92%
24) Chloroform-d	5.08	84	96800	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
26) 1,2-Dichloroethane-d4	5.72	65	57484	5.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.80%
32) Benzene-d6	5.74	84	192296	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.70	67	58619	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.91	98	155842	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
43) trans-1,3-Dichloropropene-	8.19	79	25302	4.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.20%
46) 2-Hexanone-d5	8.64	63	157411	51.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.54%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	54282	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	64255	5.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.00%


Target Compounds					Ovalue
13) Acetone	2.65	43	4791	2.501 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122120\
Data File : VU041698.D
Acq On : 21 Dec 2020 14:02
Operator : SY/MD
Sample : L5148-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB1T8

Quant Time: Dec 22 03:19:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 22 02:49:59 2020
Response via : Initial Calibration

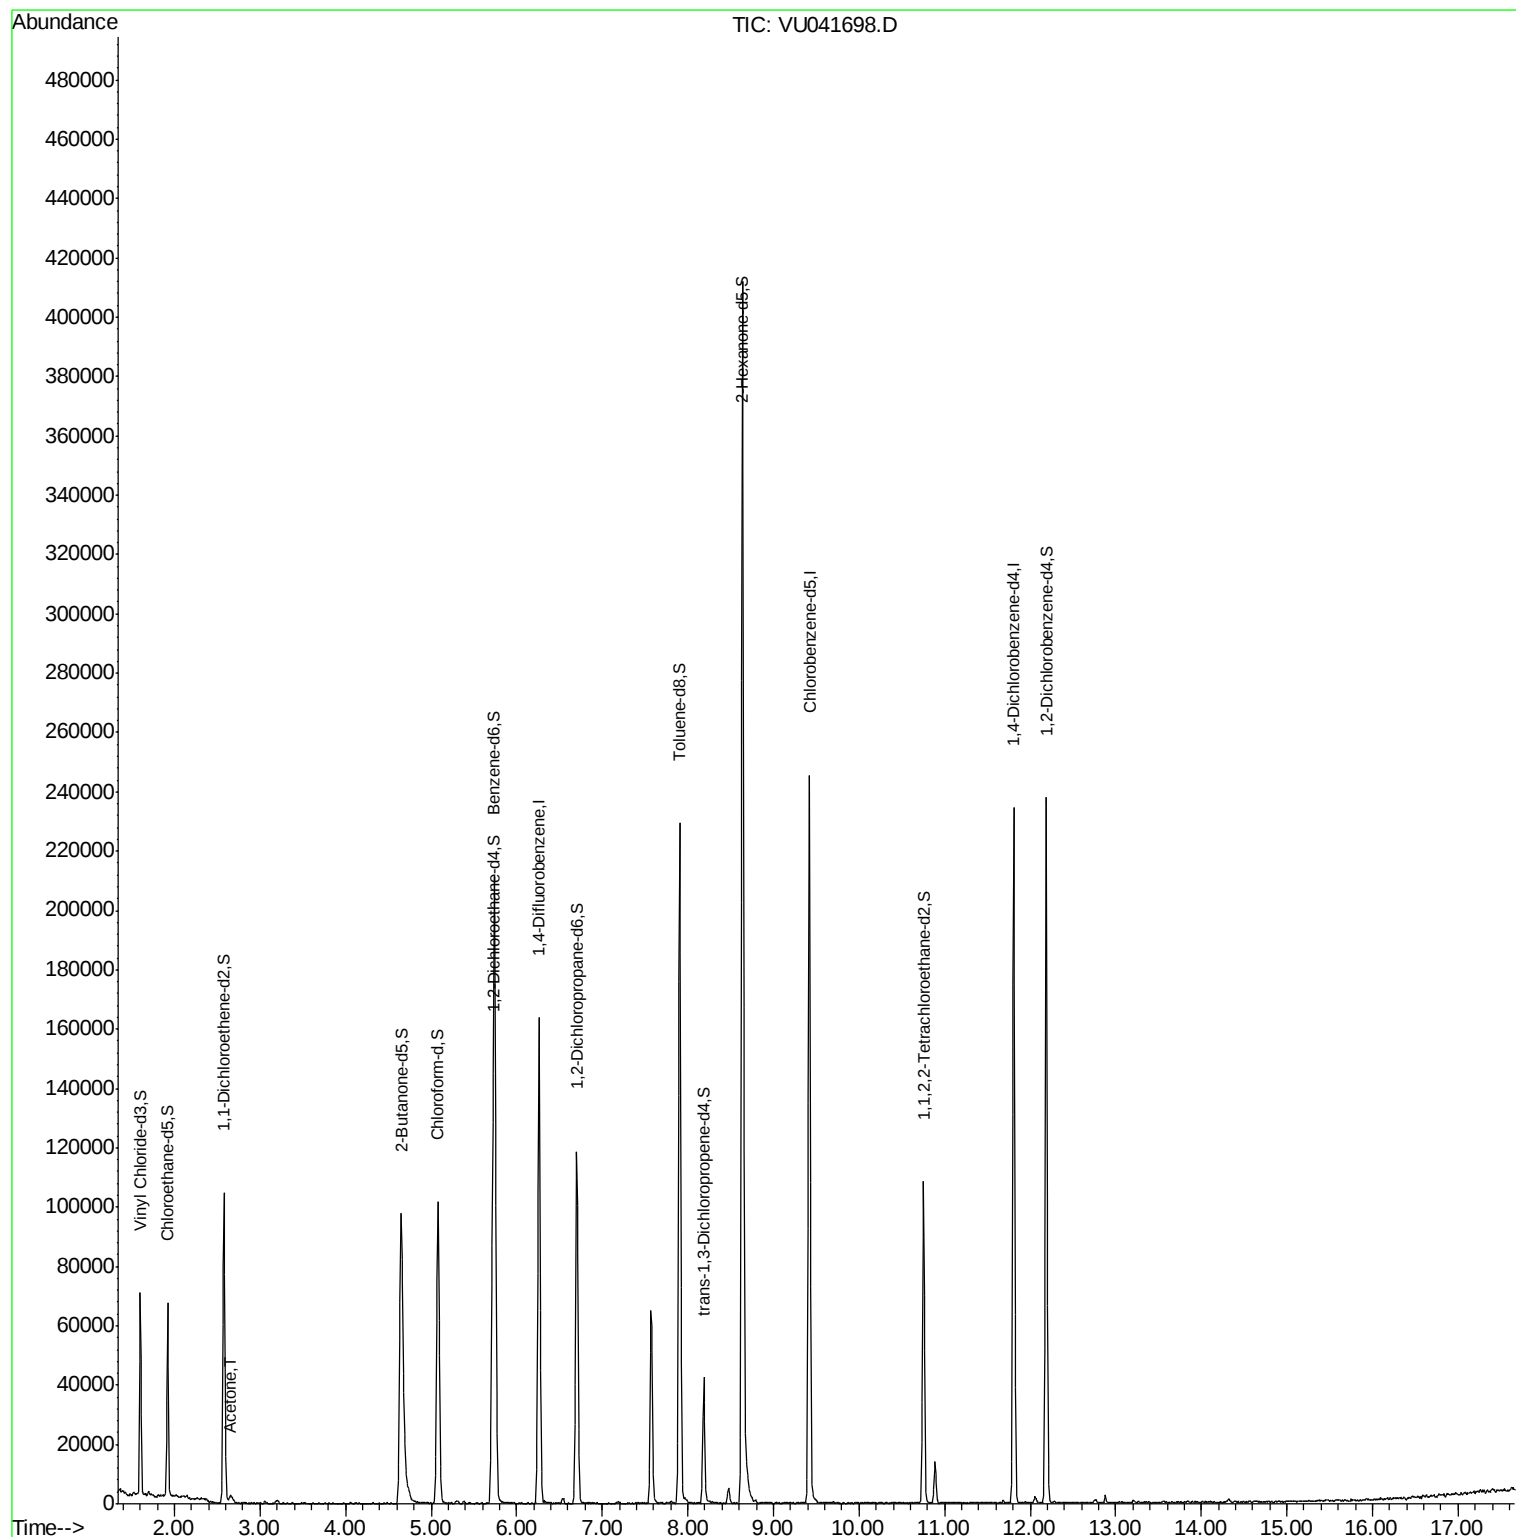

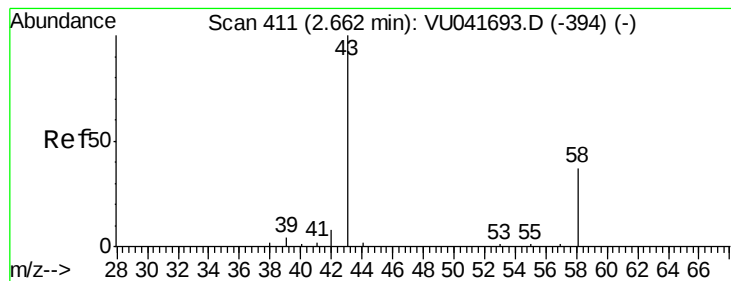

#13
 Acetone
 Concen: 2.501 ug/L
 RT: 2.65 min Scan# 409
 Delta R.T. -0.01 min
 Lab File: VU041698.D
 Acq: 21 Dec 2020 14:02

Instrument :
 MSVOA_U
 ClientSampleId :
 GB1T8

Tot Ion: 43 Resp: 4791
 Ion Ratio Lower Upper
 43 100
 58 22.5 0.0 73.2

