

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122120\
 Data File : VU041718.D
 Acq On : 22 Dec 2020 00:07
 Operator : SY/MD
 Sample : L5162-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB253

Quant Time: Dec 22 06:29:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 22 05:59:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	129854	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	131733	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	55053	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	38143	3.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.20%
7) Chloroethane-d5	1.92	69	35718	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.00%
11) 1,1-Dichloroethene-d2	2.58	63	53408	2.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.20%#
20) 2-Butanone-d5	4.65	46	170903	58.61	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.22%
24) Chloroform-d	5.08	84	85290	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.72	65	50633	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
32) Benzene-d6	5.74	84	161557	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
36) 1,2-Dichloropropane-d6	6.70	67	56448	4.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.40%
41) Toluene-d8	7.90	98	145783	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.19	79	23213	4.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.40%
46) 2-Hexanone-d5	8.64	63	159261	54.78	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.56%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	53093	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	50617	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.66	43	5220	2.814 ug/L	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122120\
Data File : VU041718.D
Acq On : 22 Dec 2020 00:07
Operator : SY/MD
Sample : L5162-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB253

Quant Time: Dec 22 06:29:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 22 05:59:09 2020
Response via : Initial Calibration

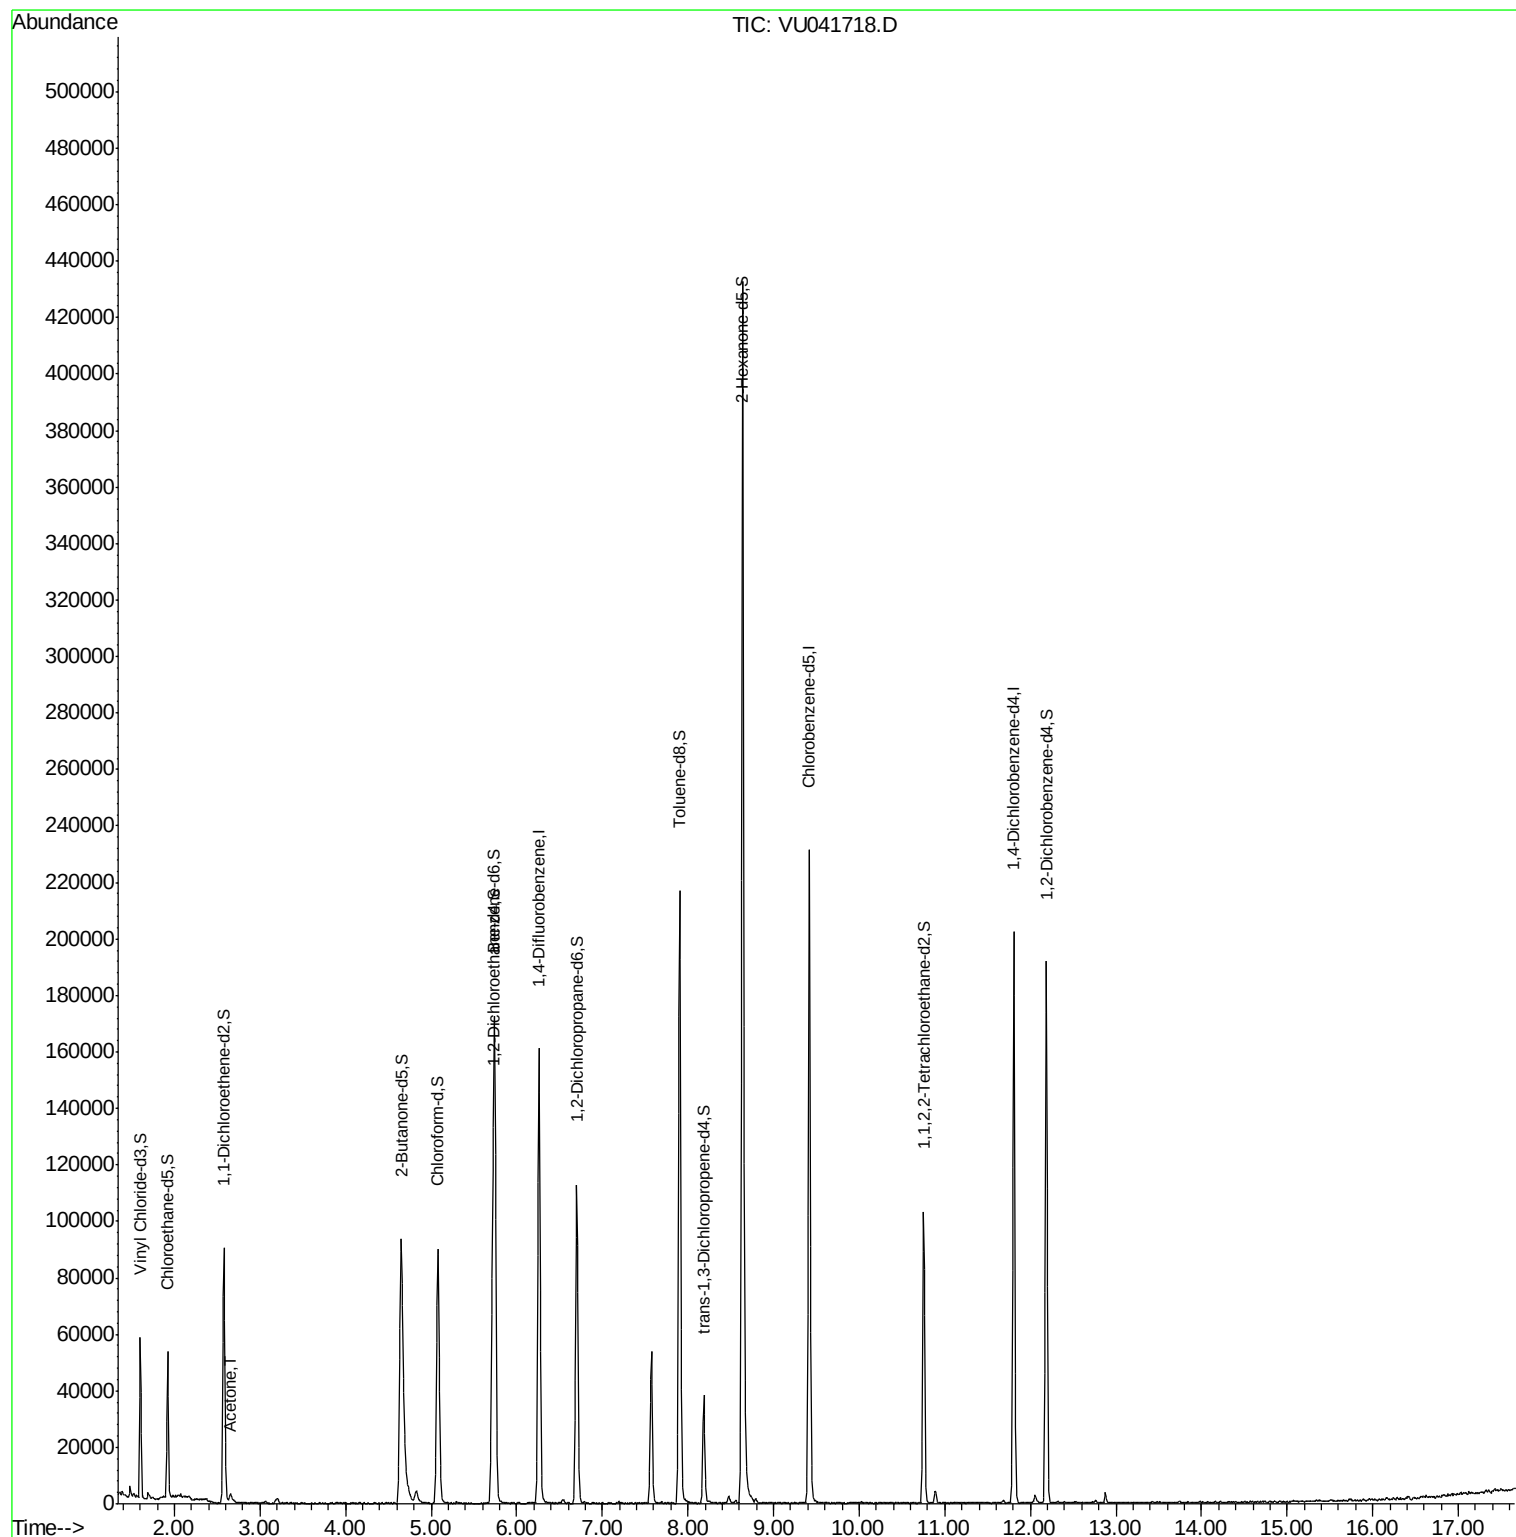

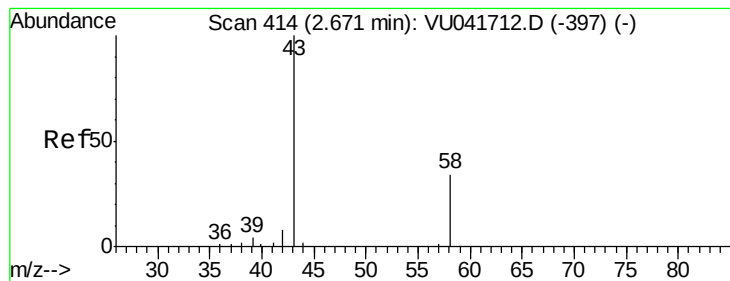

#13
 Acetone
 Concen: 2.814 ug/L
 RT: 2.66 min Scan# 409
 Delta R.T. -0.02 min
 Lab File: VU041718.D
 Acq: 22 Dec 2020 00:07

Instrument :
 MSVOA_U
 ClientSampleId :
 GB253

Tot Ion: 43 Resp: 5220
 Ion Ratio Lower Upper
 43 100
 58 12.5 0.0 73.2

