




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
Data File : VU046535.D
Acq On : 21 Dec 2021 20:09
Operator : SY/MD
Sample : M5149-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBT2

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:47:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 21 14:35:13 2021
Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
Supervised By :Mahesh Dadoda 12/28/2021

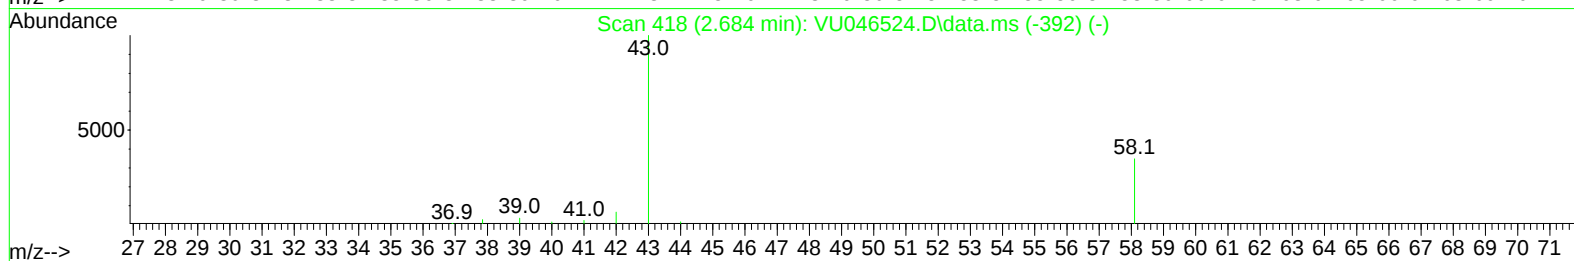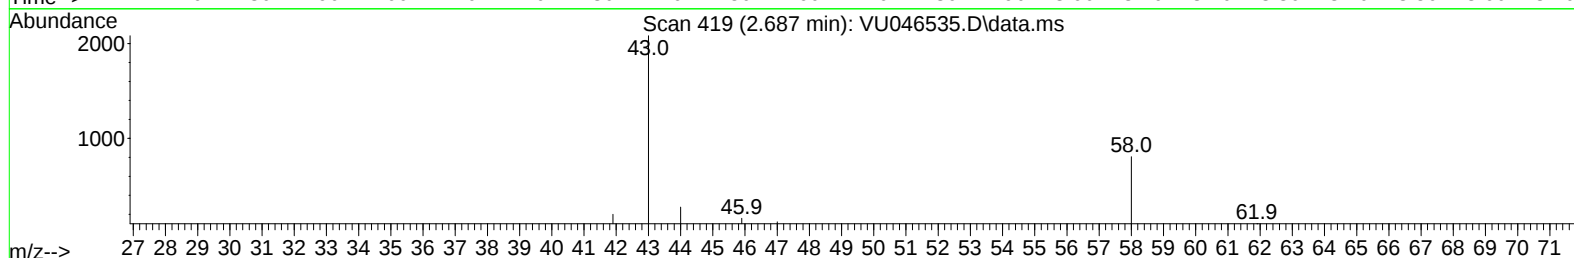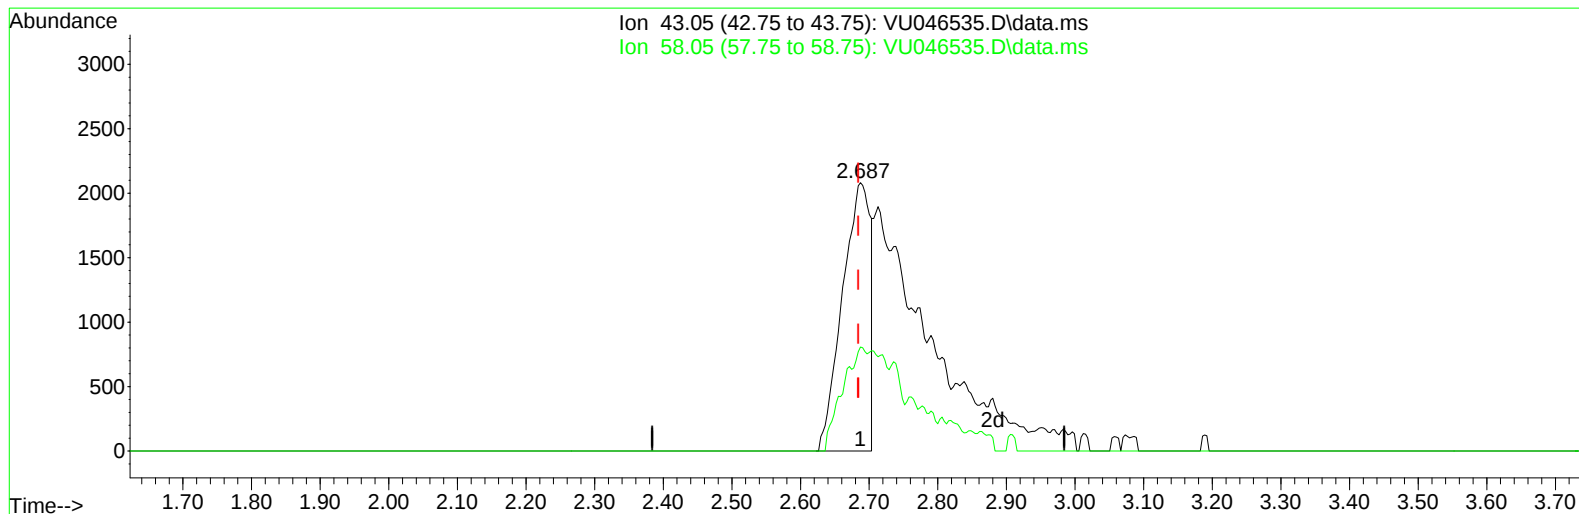

TIC: VU046535.D\data.ms

(13) Acetone (T)

2.687min (+ 0.003) 3.47 ug/L

response	5819	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	33.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
Data File : VU046535.D
Acq On : 21 Dec 2021 20:09
Operator : SY/MD
Sample : M5149-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBT2

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
Supervised By :Mahesh Dadoda 12/28/2021

Quant Time: Dec 22 05:47:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 21 14:35:13 2021
Response via : Initial Calibration

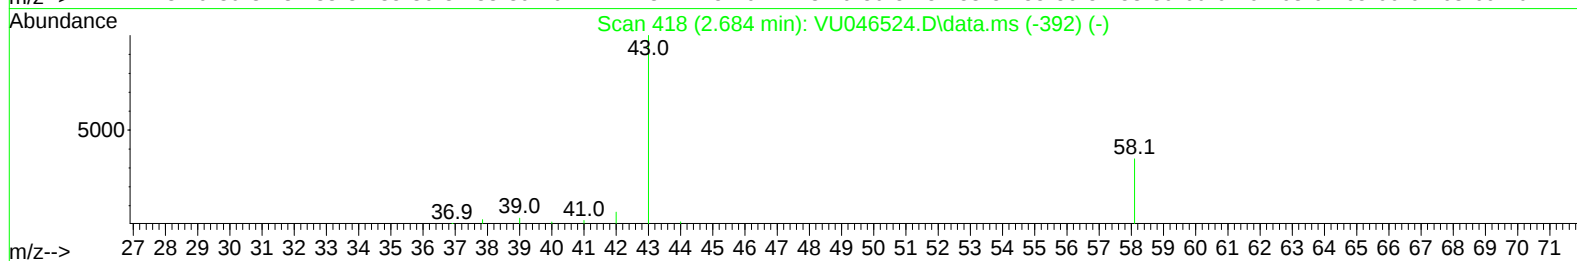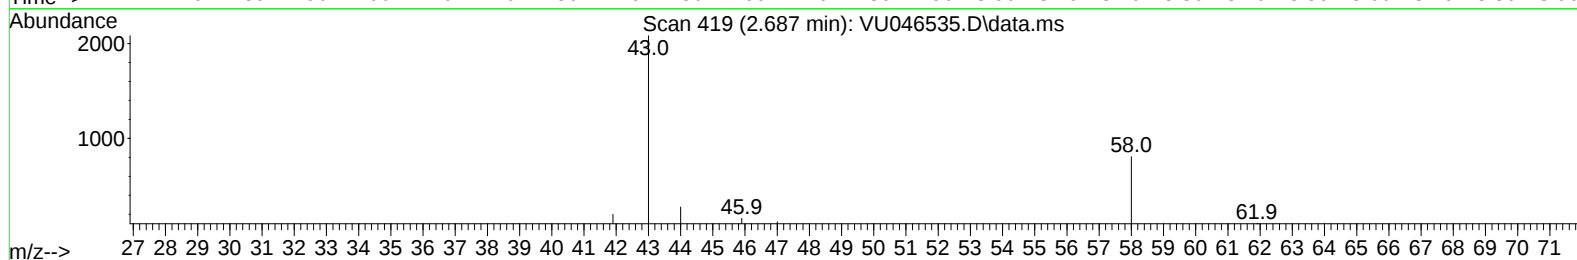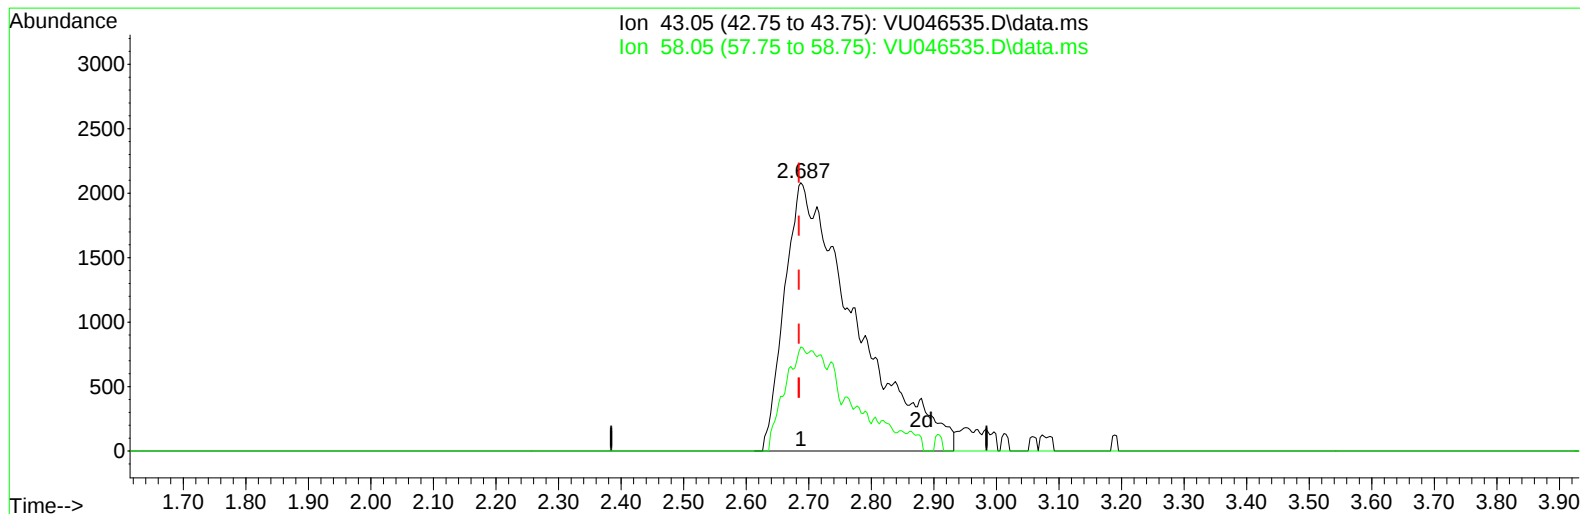

TIC: VU046535.D\data.ms

(13) Acetone (T)

2.687min (+ 0.003) 9.73 ug/L m

response 16324

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	12.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
 Data File : VU046535.D
 Acq On : 21 Dec 2021 20:09
 Operator : SY/MD
 Sample : M5149-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBT2

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:47:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 21 14:35:13 2021
 Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Mahesh Dadoda 12/28/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	78357	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	76598	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	34048	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	31104	5.039	ug/L	0.01
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.800%		
7) Chloroethane-d5	1.919	69	25478	5.242	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 104.800%		
11) 1,1-Dichloroethene-d2	2.575	65	13677	5.255	ug/L	0.01
Spiked Amount	5.000	Range 60 - 125	Recovery	= 105.200%		
20) 2-Butanone-d5	4.655	46	101170	56.511	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 113.020%		
24) Chloroform-d	5.070	84	57701	5.102	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 102.000%		
26) 1,2-Dichloroethane-d4	5.706	65	34910	5.400	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 108.000%		
32) Benzene-d6	5.732	84	114712	5.372	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 107.400%		
36) 1,2-Dichloropropane-d6	6.694	67	34595	5.392	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 107.800%		
41) Toluene-d8	7.899	98	97002	5.005	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 100.200%		
43) trans-1,3-Dichloroprop...	8.182	79	14491	4.883	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 97.600%		
46) 2-Hexanone-d5	8.639	63	96671	55.486	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 110.980%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	33749	5.125	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 102.400%		
66) 1,2-Dichlorobenzene-d4	12.195	152	36147	5.763	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 115.200%		
Target Compounds						Qvalue
13) Acetone	2.687	43	16324m	9.725	ug/L	
30) Cyclohexane	5.388	56	2088	0.199	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
Data File : VU046535.D
Acq On : 21 Dec 2021 20:09
Operator : SY/MD
Sample : M5149-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBT2

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:47:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 21 14:35:13 2021
Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
Supervised By :Mahesh Dadoda 12/28/2021

