




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
Data File : VU046537.D
Acq On : 21 Dec 2021 20:56
Operator : SY/MD
Sample : M5149-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBT4

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
Supervised By :Mahesh Dadoda 12/28/2021

Quant Time: Dec 22 06:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 22 06:54:42 2021
Response via : Initial Calibration

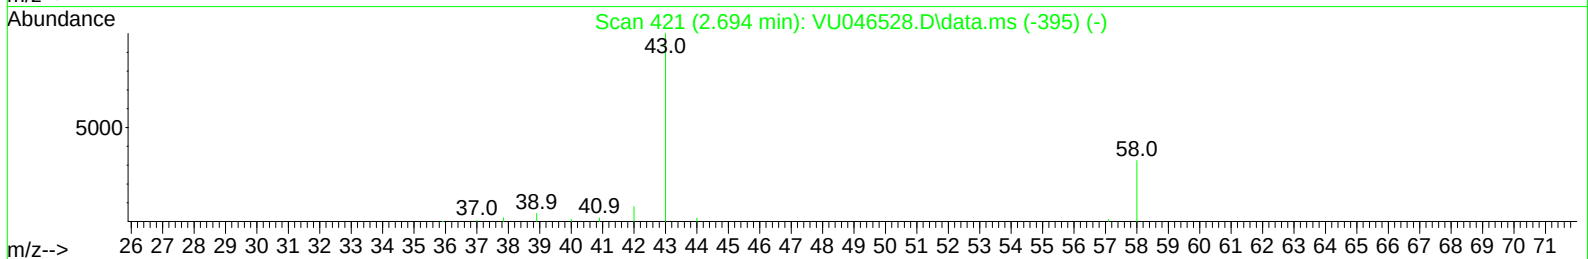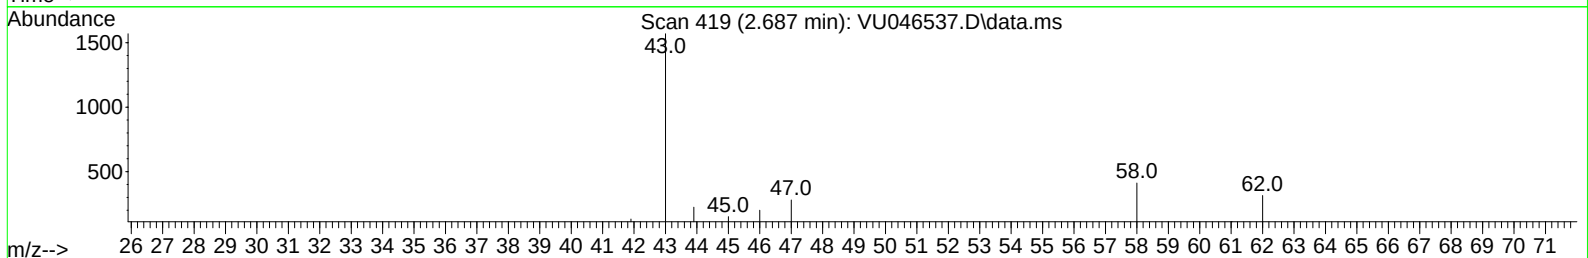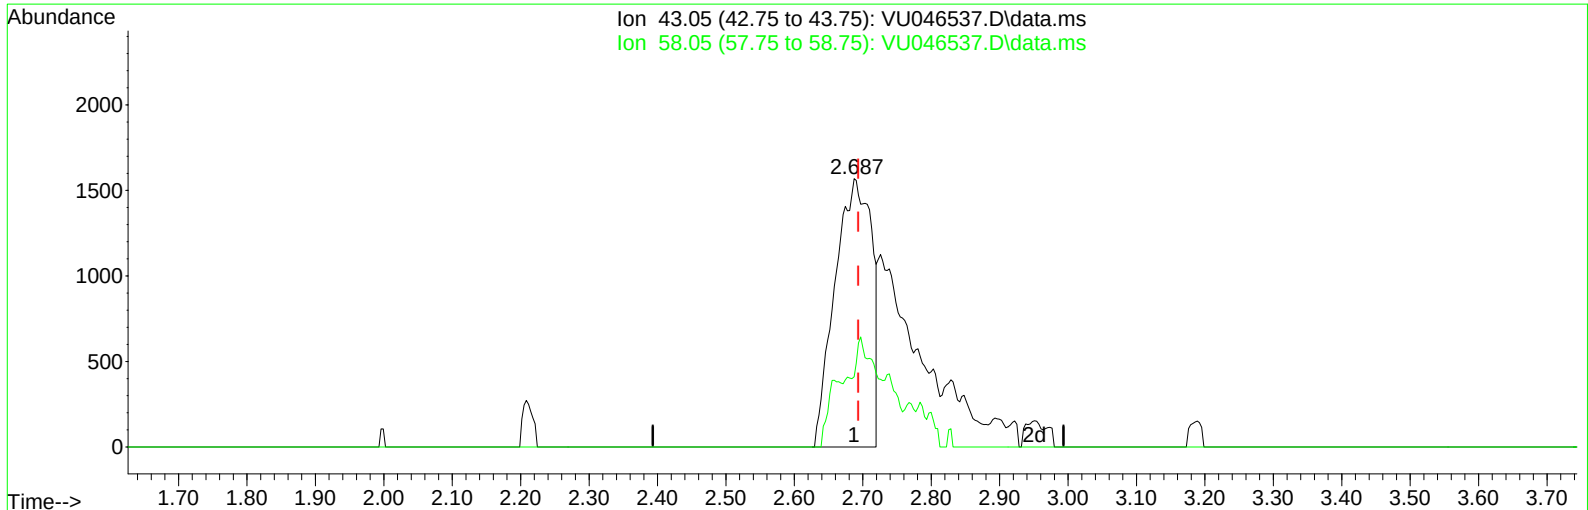

TIC: VU046537.D\data.ms

(13) Acetone (T)

2.687min (-0.006) 3.46 ug/L

response 5813

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	9.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
 Data File : VU046537.D
 Acq On : 21 Dec 2021 20:56
 Operator : SY/MD
 Sample : M5149-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBT4

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Mahesh Dadoda 12/28/2021

Quant Time: Dec 22 06:54:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 22 06:54:42 2021
 Response via : Initial Calibration

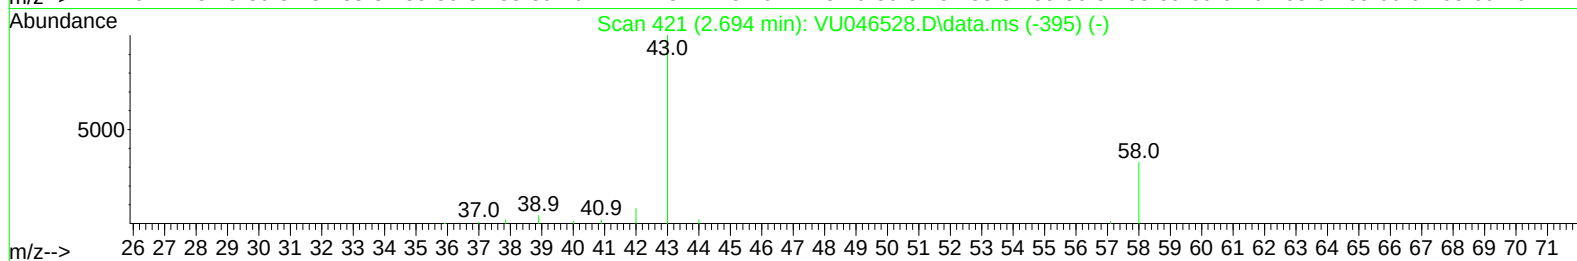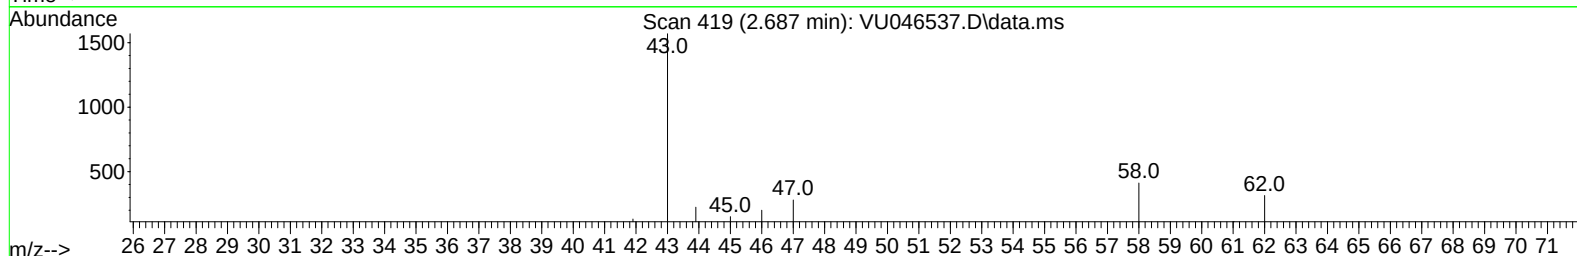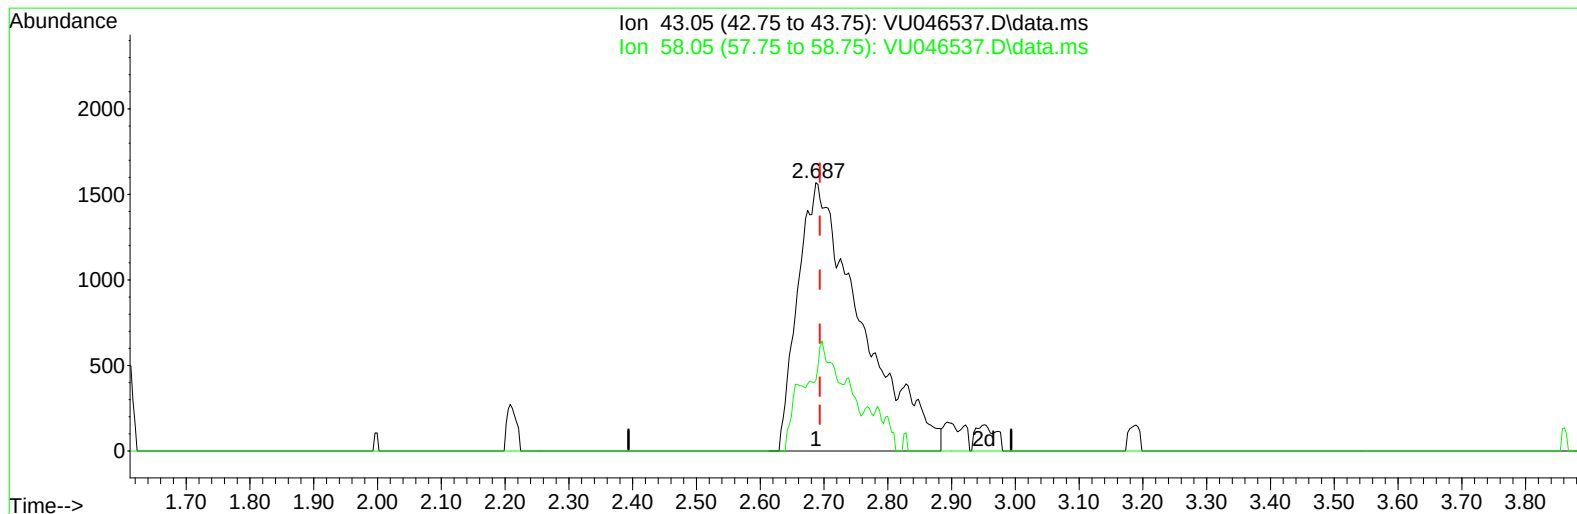

TIC: VU046537.D\data.ms

(13) Acetone (T)

2.687min (-0.006) 6.40 ug/L m

response 10769

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	4.98
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
 Data File : VU046537.D
 Acq On : 21 Dec 2021 20:56
 Operator : SY/MD
 Sample : M5149-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBT4

Manual IntegrationsAPPROVED

Quant Time: Dec 22 06:54:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 22 06:54:42 2021
 Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Mahesh Dadoda 12/28/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	78515	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	76875	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	34292	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	31381	5.074	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 101.400%			
7) Chloroethane-d5	1.919	69	24900	5.113	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 102.200%			
11) 1,1-Dichloroethene-d2	2.575	65	13492	5.174	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 103.400%			
20) 2-Butanone-d5	4.658	46	100038	55.766	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 111.540%			
24) Chloroform-d	5.070	84	57242	5.051	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 101.000%			
26) 1,2-Dichloroethane-d4	5.706	65	35106	5.419	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 108.400%			
32) Benzene-d6	5.732	84	114635	5.349	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 107.000%			
36) 1,2-Dichloropropane-d6	6.694	67	34427	5.346	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 107.000%			
41) Toluene-d8	7.899	98	95970	4.934	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 98.600%			
43) trans-1,3-Dichloroprop...	8.182	79	14812	4.973	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 99.400%			
46) 2-Hexanone-d5	8.639	63	95518	54.626	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 109.260%			
56) 1,1,2,2-Tetrachloroeth...	10.758	84	33846	5.121	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 102.400%			
66) 1,2-Dichlorobenzene-d4	12.195	152	36458	5.772	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 115.400%			
Target Compounds					Qvalue	
13) Acetone	2.687	43	10769m	6.403	ug/L	
30) Cyclohexane	5.395	56	8187	0.779	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
Data File : VU046537.D
Acq On : 21 Dec 2021 20:56
Operator : SY/MD
Sample : M5149-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBT4

Manual IntegrationsAPPROVED

Quant Time: Dec 22 06:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 22 06:54:42 2021
Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
Supervised By :Mahesh Dadoda 12/28/2021

