


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122121\
 Data File : VU046521.D
 Acq On : 21 Dec 2021 11:24
 Operator : SY/MD
 Sample : BFB033
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB033

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 30 04:21:35 2021

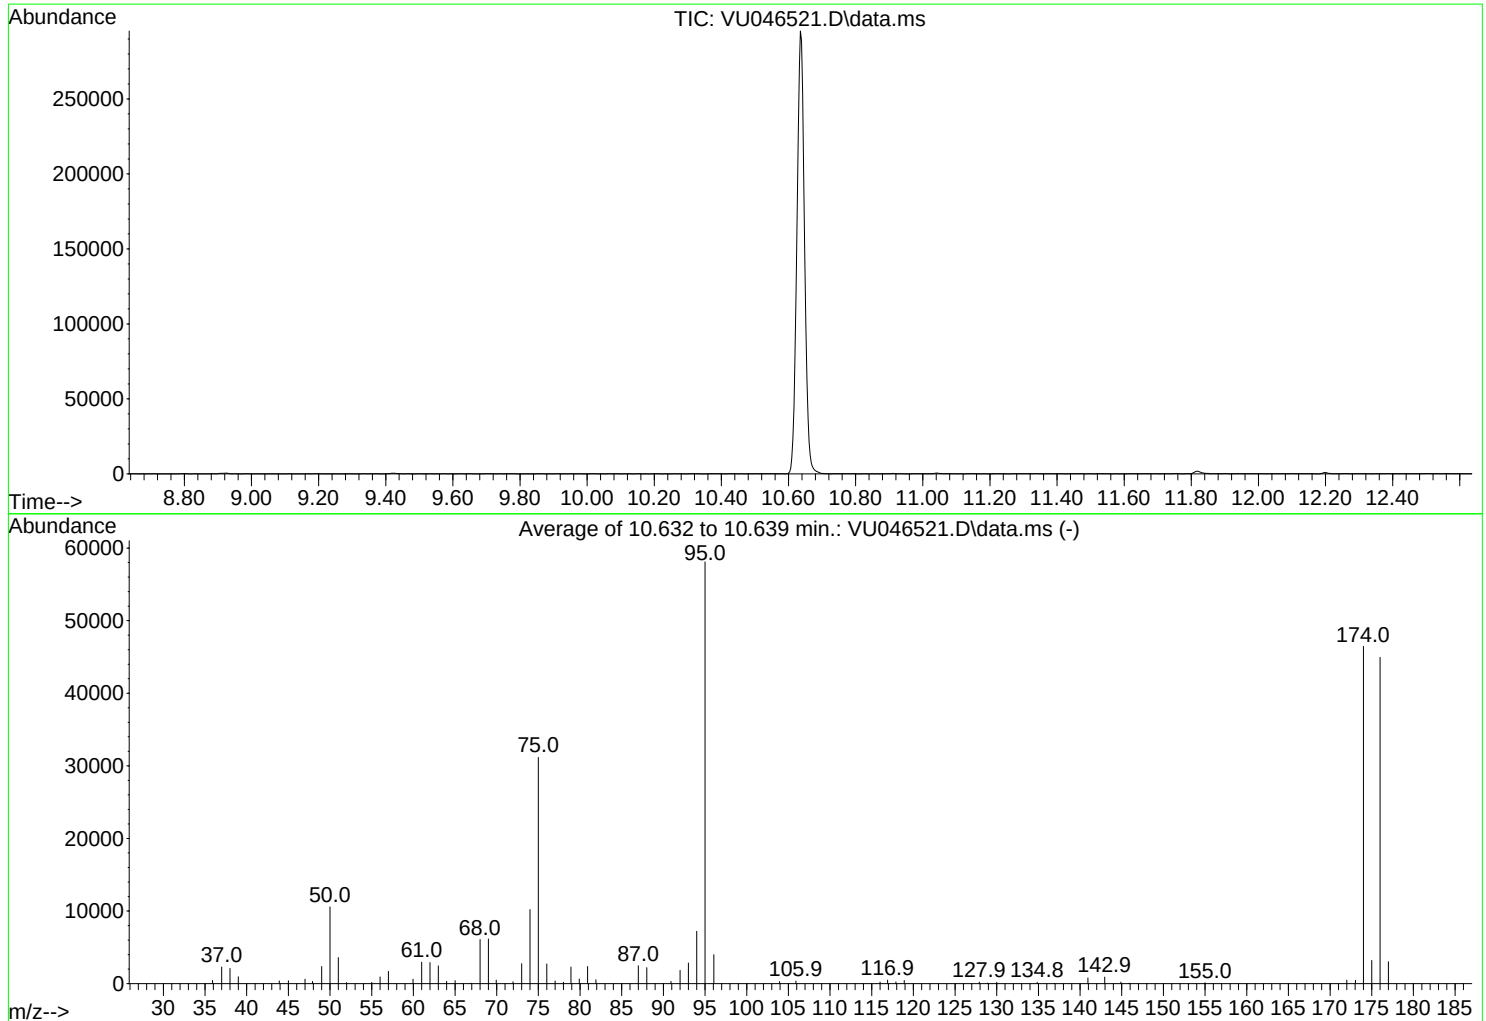

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	10580	PASS
75	95	30	80	53.7	31171	PASS
95	95	100	100	100.0	58099	PASS
96	95	5	9	6.9	3988	PASS
173	174	0.00	2	1.0	463	PASS
174	95	50	120	80.0	46456	PASS
175	174	5	9	6.9	3205	PASS
176	174	95	101	96.7	44939	PASS
177	176	5	9	6.7	3024	PASS

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	414.0
37.00	2246.0
38.00	2125.0
39.00	993.0
43.90	391.0
45.00	441.0
47.00	587.0
47.90	319.0
49.00	2214.0
50.00	10363.0
51.00	3372.0
52.00	121.0
55.00	159.0
56.00	902.0
57.00	1558.0
59.90	574.0
61.00	2909.0
62.00	2705.0
63.00	2413.0
64.00	312.0
65.00	357.0
66.90	119.0
68.00	5838.0
69.00	5975.0
70.00	457.0
71.90	224.0
73.00	2667.0
74.00	9833.0
75.00	30440.0
76.00	2617.0
77.00	340.0
78.00	207.0
78.90	2350.0
79.90	625.0
80.90	2325.0
81.90	540.0
87.00	2488.0
88.00	2170.0
90.90	282.0
92.00	1692.0
93.00	2702.0
94.00	6889.0
95.00	55392.0
96.00	4040.0
97.00	105.0
104.00	276.0
105.90	308.0
116.00	236.0
116.90	490.0
117.90	213.0
118.90	439.0
127.90	210.0
128.90	133.0
130.00	211.0
134.80	185.0
140.90	704.0
143.00	874.0
144.90	190.0
145.90	106.0
155.00	138.0
172.00	517.0
173.10	459.0
174.00	43256.0
175.00	2960.0
176.00	41840.0
177.00	2914.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	474.0
37.00	2367.0
38.00	2129.0
39.00	996.0
43.90	389.0
45.00	413.0
47.00	628.0
47.90	332.0
49.00	2427.0
50.00	10927.0
51.00	3750.0
52.00	172.0
55.00	192.0
56.00	960.0
57.00	1753.0
59.90	628.0
61.00	3044.0
62.00	3018.0
63.00	2555.0
64.00	321.0
65.00	428.0
66.90	110.0
68.00	6324.0
69.00	6334.0
70.00	520.0
72.00	282.0
73.00	2852.0
74.00	10453.0
75.00	32128.0
76.00	2829.0
77.00	382.0
78.00	207.0
78.90	2395.0
79.90	657.0
80.90	2469.0
81.90	547.0
87.00	2609.0
88.00	2294.0
90.90	330.0
92.00	1912.0
93.00	2925.0
94.00	7538.0
95.00	60232.0
96.00	4110.0
103.90	285.0
105.90	353.0
116.00	237.0
116.90	507.0
117.90	254.0
118.90	460.0
127.90	237.0
128.90	117.0
130.00	210.0
134.90	200.0
141.00	791.0
142.90	944.0
144.90	229.0
145.90	113.0
155.00	135.0
172.00	494.0
173.00	481.0
174.00	48008.0
175.00	3255.0
176.00	46496.0
177.00	3128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	464.0
37.00	2274.0
38.00	2004.0
39.00	884.0
43.90	360.0
45.00	359.0
47.00	609.0
47.90	285.0
49.00	2426.0
50.00	10450.0
51.00	3658.0
52.00	181.0
55.00	178.0
56.00	902.0
57.00	1779.0
60.00	632.0
61.00	2878.0
62.00	2993.0
63.00	2370.0
64.00	337.0
65.00	469.0
68.00	6119.0
69.00	6112.0
69.90	503.0
72.00	283.0
73.00	2780.0
74.00	10352.0
75.00	30944.0
76.00	2717.0
77.00	376.0
78.00	188.0
78.90	2149.0
79.90	627.0
80.90	2281.0
81.90	499.0
87.00	2331.0
88.00	2170.0
90.90	309.0
92.00	1883.0
93.00	2935.0
94.00	7195.0
95.00	58672.0
96.10	3814.0
103.90	299.0
105.90	375.0
116.00	213.0
116.90	458.0
117.90	289.0
118.90	422.0
127.90	237.0
130.00	189.0
134.90	190.0
136.90	104.0
141.00	862.0
143.00	890.0
144.90	233.0
148.00	115.0
155.00	135.0
157.00	101.0
172.00	453.0
173.00	450.0
174.00	48104.0
175.00	3400.0
176.00	46480.0
177.00	3030.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033