




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052472.D
 Acq On : 21 Dec 2022 12:02
 Operator : JC/MD
 Sample : N6156-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 23CC01-22

Manual IntegrationsAPPROVED

Quant Time: Dec 22 00:29:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 22 00:28:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/23/2022
 Supervised By :Mahesh Dadoda 12/23/2022

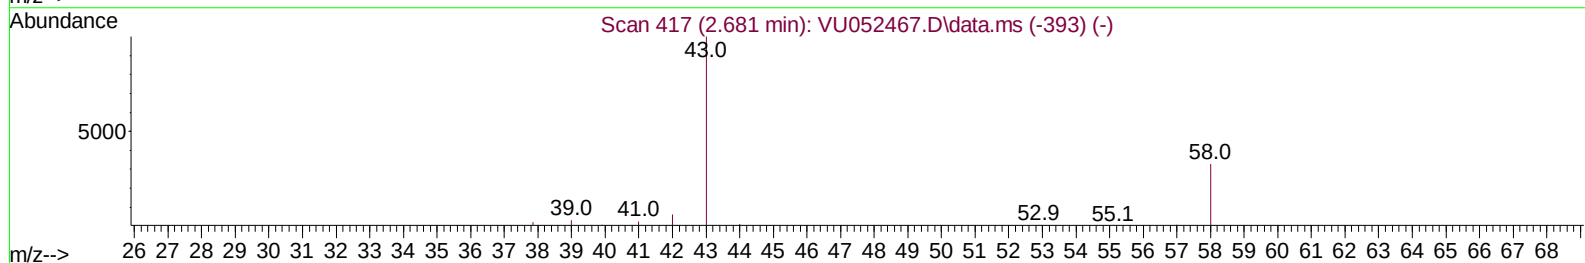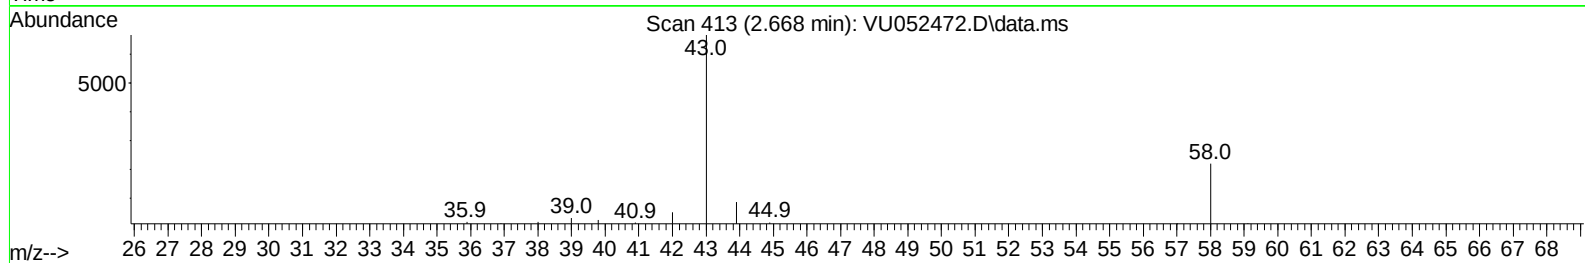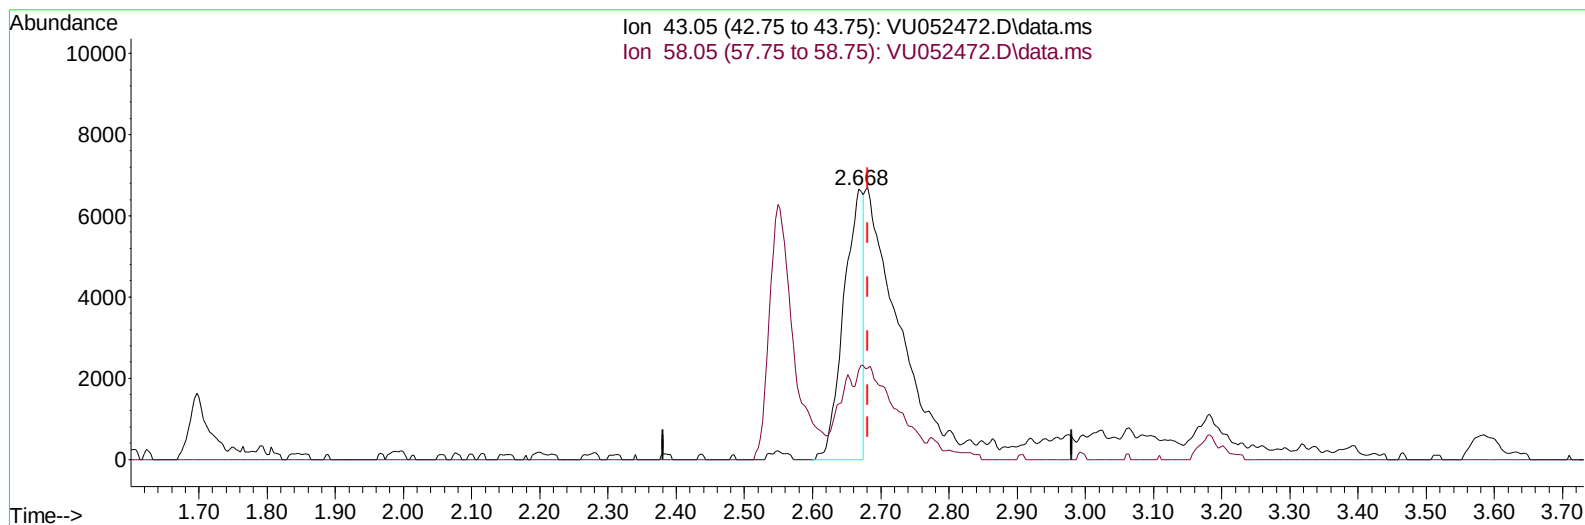

TIC: VU052472.D\data.ms

(13) Acetone (T)

2.668min (-0.013) 3.91 ug/L

response 13298

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.70	60.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052472.D
 Acq On : 21 Dec 2022 12:02
 Operator : JC/MD
 Sample : N6156-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 23CC01-22

Manual IntegrationsAPPROVED

Quant Time: Dec 22 00:29:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 22 00:28:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/23/2022
 Supervised By :Mahesh Dadoda 12/23/2022

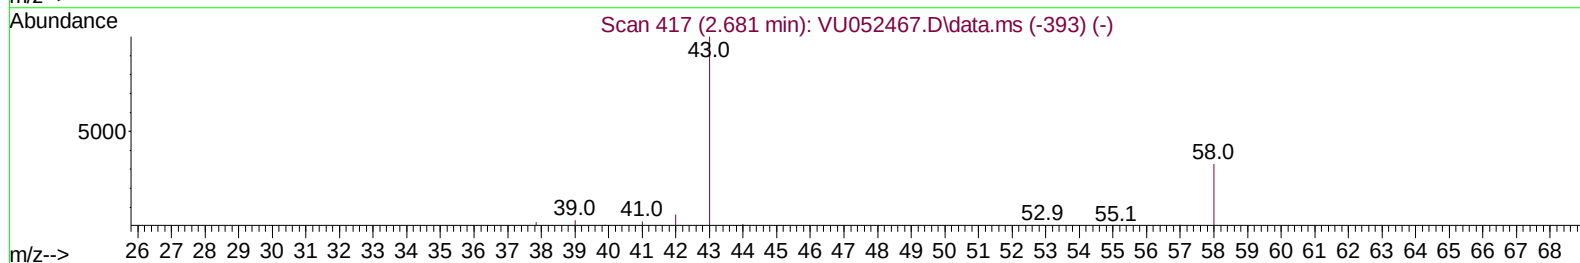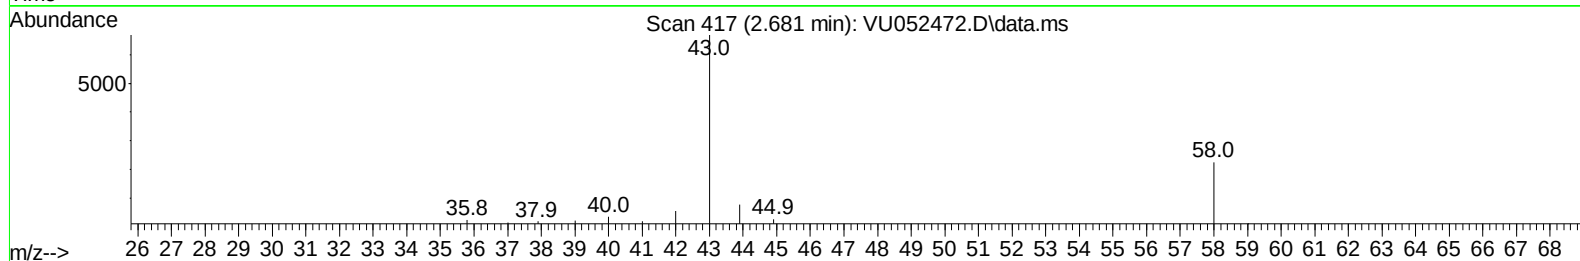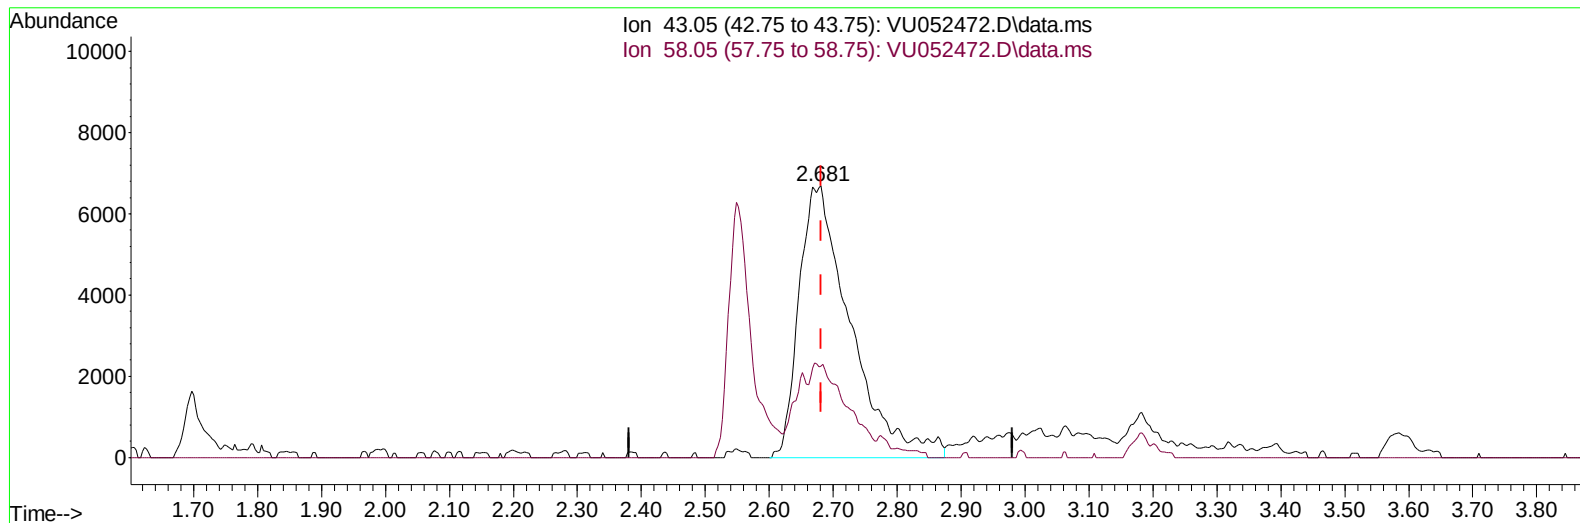

TIC: VU052472.D\data.ms

(13) Acetone (T)

2.681min (-0.000) 10.97 ug/L m

response 37365

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.70	21.45
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052472.D
 Acq On : 21 Dec 2022 12:02
 Operator : JC/MD
 Sample : N6156-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 23CC01-22

Manual IntegrationsAPPROVED

Quant Time: Dec 22 00:29:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 22 00:28:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/23/2022
 Supervised By :Mahesh Dadoda 12/23/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	147021	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	144750	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	61021	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	76714	5.150	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 103.000%			
7) Chloroethane-d5	1.916	69	65813	5.124	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 102.400%			
11) 1,1-Dichloroethene-d2	2.568	65	32301	5.040	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 100.800%			
20) 2-Butanone-d5	4.645	46	270586	58.582	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 117.160%			
24) Chloroform-d	5.060	84	131536	5.234	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 104.600%			
26) 1,2-Dichloroethane-d4	5.700	65	79967	5.486	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 109.800%			
32) Benzene-d6	5.726	84	258182	5.202	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 104.000%			
36) 1,2-Dichloropropane-d6	6.687	67	90955	5.324	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 106.400%			
41) Toluene-d8	7.896	98	207352	4.977	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 99.600%			
43) trans-1,3-Dichloroprop...	8.179	79	32049	5.479	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 109.600%			
46) 2-Hexanone-d5	8.632	63	181810	56.808	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 113.620%			
56) 1,1,2,2-Tetrachloroeth...	10.751	84	81626	5.628	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 112.600%			
66) 1,2-Dichlorobenzene-d4	12.188	152	76739	6.177	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 123.600%#			
Target Compounds						
					Qvalue	
13) Acetone	2.681	43	37365m	10.974	ug/L	
42) Toluene	7.967	91	34573	0.692	ug/L	97
53) m,p-Xylene	9.690	106	4673	0.245	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052472.D
Acq On : 21 Dec 2022 12:02
Operator : JC/MD
Sample : N6156-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
23CC01-22

Manual IntegrationsAPPROVED

Quant Time: Dec 22 00:29:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 22 00:28:27 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 12/23/2022
Supervised By :Mahesh Dadoda 12/23/2022

