

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052472.D
 Acq On : 21 Dec 2022 12:02
 Operator : JC/MD
 Sample : N6156-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 23CC01-22

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 12/23/2022
 Supervised By :Mahesh Dadoda 12/23/2022

Quant Time: Dec 22 00:29:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 22 00:28:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	147021	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	144750	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	61021	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	76714	5.150	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	103.000%	
7) Chloroethane-d5	1.916	69	65813	5.124	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.400%	
11) 1,1-Dichloroethene-d2	2.568	65	32301	5.040	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	100.800%	
20) 2-Butanone-d5	4.645	46	270586	58.582	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	117.160%	
24) Chloroform-d	5.060	84	131536	5.234	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.600%	
26) 1,2-Dichloroethane-d4	5.700	65	79967	5.486	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.800%	
32) Benzene-d6	5.726	84	258182	5.202	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.000%	
36) 1,2-Dichloropropane-d6	6.687	67	90955	5.324	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.400%	
41) Toluene-d8	7.896	98	207352	4.977	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	8.179	79	32049	5.479	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	109.600%	
46) 2-Hexanone-d5	8.632	63	181810	56.808	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	113.620%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	81626	5.628	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	112.600%	
66) 1,2-Dichlorobenzene-d4	12.188	152	76739	6.177	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	123.600%#	
Target Compounds					Qvalue	
13) Acetone	2.681	43	37365m	10.974	ug/L	
42) Toluene	7.967	91	34573	0.692	ug/L	97
53) m,p-Xylene	9.690	106	4673	0.245	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052472.D
Acq On : 21 Dec 2022 12:02
Operator : JC/MD
Sample : N6156-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
23CC01-22

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 12/23/2022
Supervised By :Mahesh Dadoda 12/23/2022

Quant Time: Dec 22 00:29:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 22 00:28:27 2022
Response via : Initial Calibration

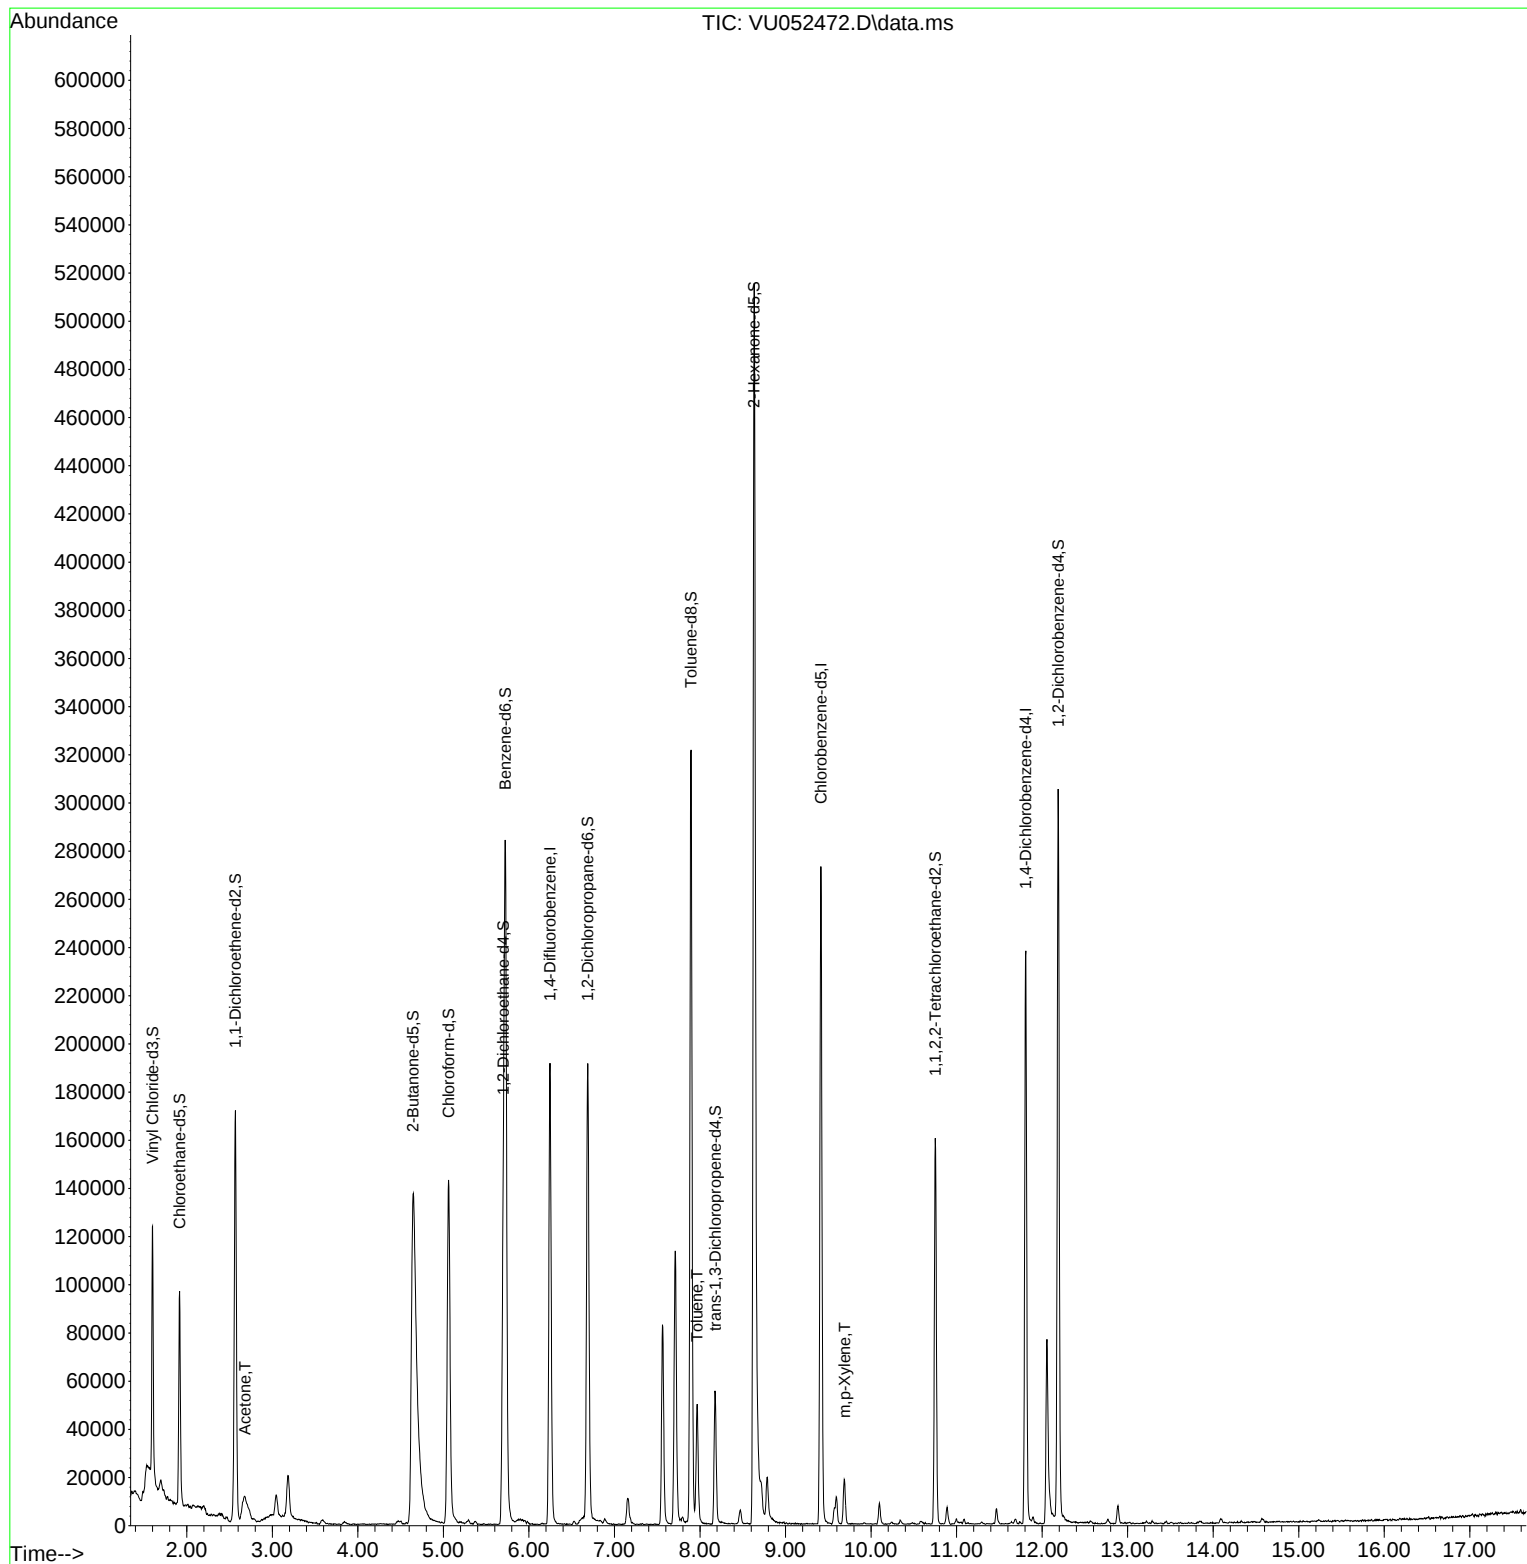

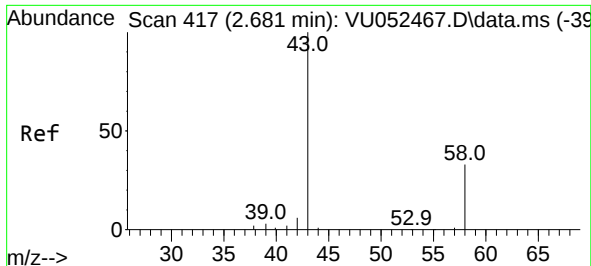

#13

Acetone

Concen: 10.974 ug/L m

RT: 2.681 min Scan# 41

Delta R.T. -0.000 min

Lab File: VU052472.D

Acq: 21 Dec 2022 12:02

Instrument :

MSVOA_U

ClientSampleId :

23CC01-22

Tgt Ion: 43 Resp: 3736

Ion Ratio Lower Upper

43 100





58 21.5 0.0 65.4

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 12/23/2022

Supervised By :Mahesh Dadoda 12/23/2022

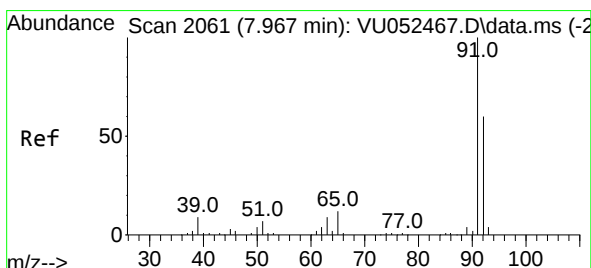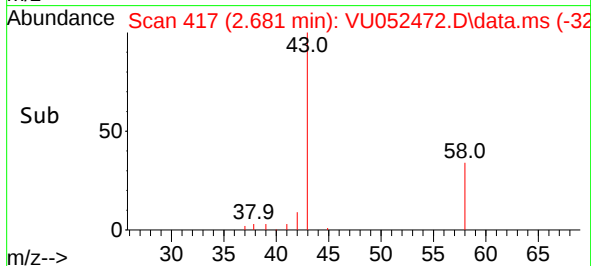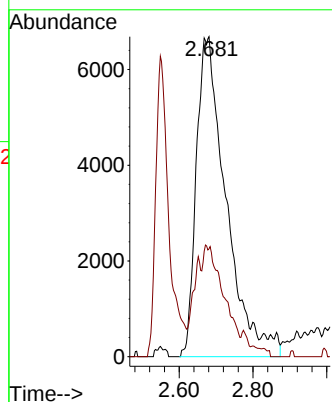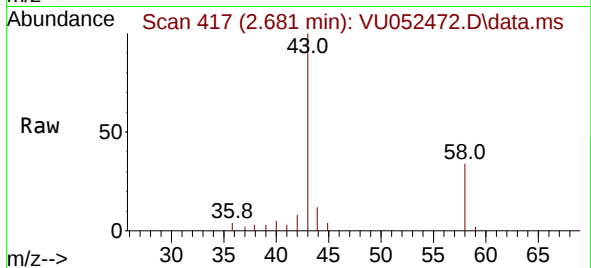

#42

Toluene

Concen: 0.692 ug/L

RT: 7.967 min Scan# 2061

Delta R.T. -0.000 min

Lab File: VU052472.D




Acq: 21 Dec 2022 12:02


Tgt Ion: 91 Resp: 34573

Ion Ratio Lower Upper

91 100

92 60.6 40.6 75.4

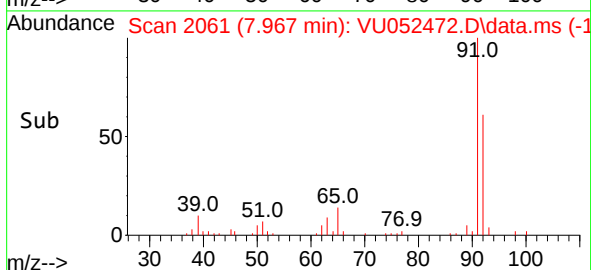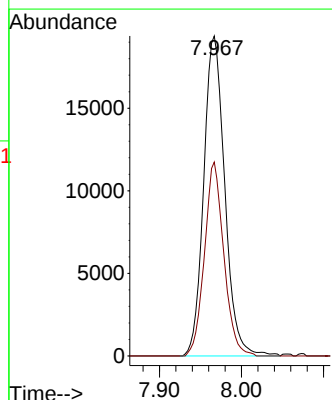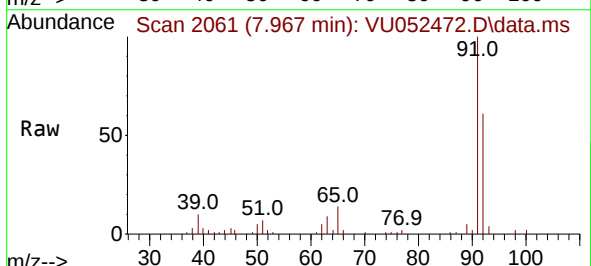

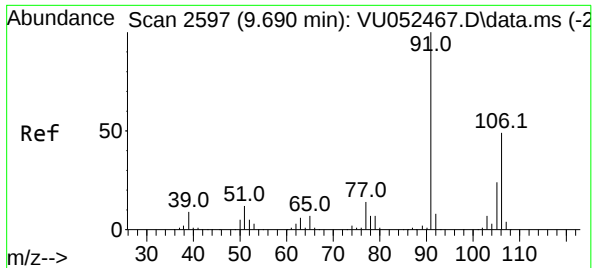

#53
 m,p-Xylene
 Concen: 0.245 ug/L
 RT: 9.690 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VU052472.D
 Acq: 21 Dec 2022 12:02

Instrument : MSVOA_U
 ClientSampleId : 23CC01-22

Tgt Ion:106 Resp: 467

Ion	Ratio	Lower	Upper
106	100		
91	201.5	148.2	275.2

Manual Integrations
APPROVED
 Reviewed By :Krupa Patel 12/23/2022
 Supervised By :Mahesh Dadoda 12/23/2022

