

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052470.D
 Acq On : 21 Dec 2022 11:16
 Operator : JC/MD
 Sample : N6034-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	107835	125718	12.83%	1.925%
2	1.916	170	179	194	rVB	97617	131399	13.41%	2.011%
3	2.568	369	382	401	rVB	171233	279633	28.53%	4.281%
4	3.047	517	531	542	rVB2	6146	11732	1.20%	0.180%
5	4.655	1012	1031	1077	rBV	83020	414050	42.25%	6.338%
6	5.060	1141	1157	1181	rBV	149175	328627	33.53%	5.031%
7	5.722	1341	1363	1401	rBV2	308358	812998	82.95%	12.446%
8	6.247	1510	1526	1548	rBV	228675	436374	44.53%	6.680%
9	6.687	1647	1663	1690	rBV	196079	395433	40.35%	6.053%
10	7.562	1924	1935	1955	rBV	85899	154135	15.73%	2.360%
11	7.896	2026	2039	2061	rBV	328548	572329	58.40%	8.761%
12	8.176	2115	2126	2145	rBV	54922	95301	9.72%	1.459%
13	8.468	2204	2217	2231	rBV3	8955	17368	1.77%	0.266%
14	8.635	2256	2269	2303	rBV2	462939	980049	100.00%	15.003%
15	9.414	2498	2511	2535	rBV	331513	557326	56.87%	8.532%
16	10.751	2913	2927	2947	rBV	155930	249580	25.47%	3.821%
17	10.889	2961	2970	2981	rVB3	9714	15795	1.61%	0.242%
18	11.809	3242	3256	3276	rBV	292994	463871	47.33%	7.101%
19	12.188	3361	3374	3398	rBV	306250	490704	50.07%	7.512%




Sum of corrected areas: 6532422

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052470.D
Acq On : 21 Dec 2022 11:16
Operator : JC/MD
Sample : N6034-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

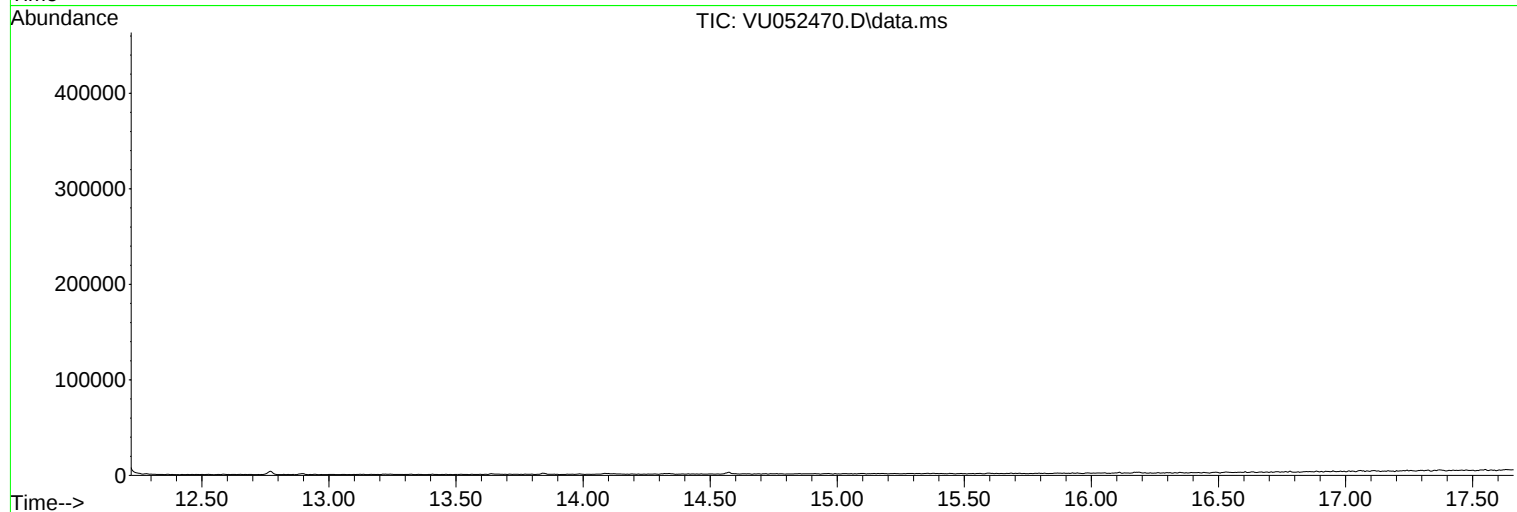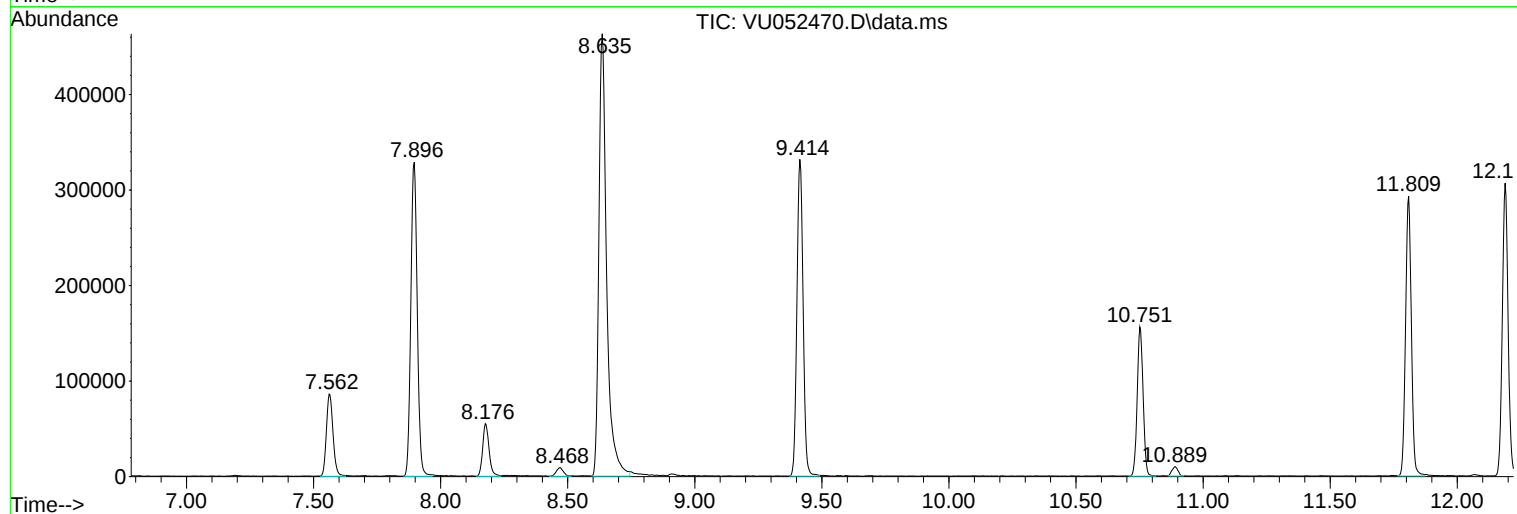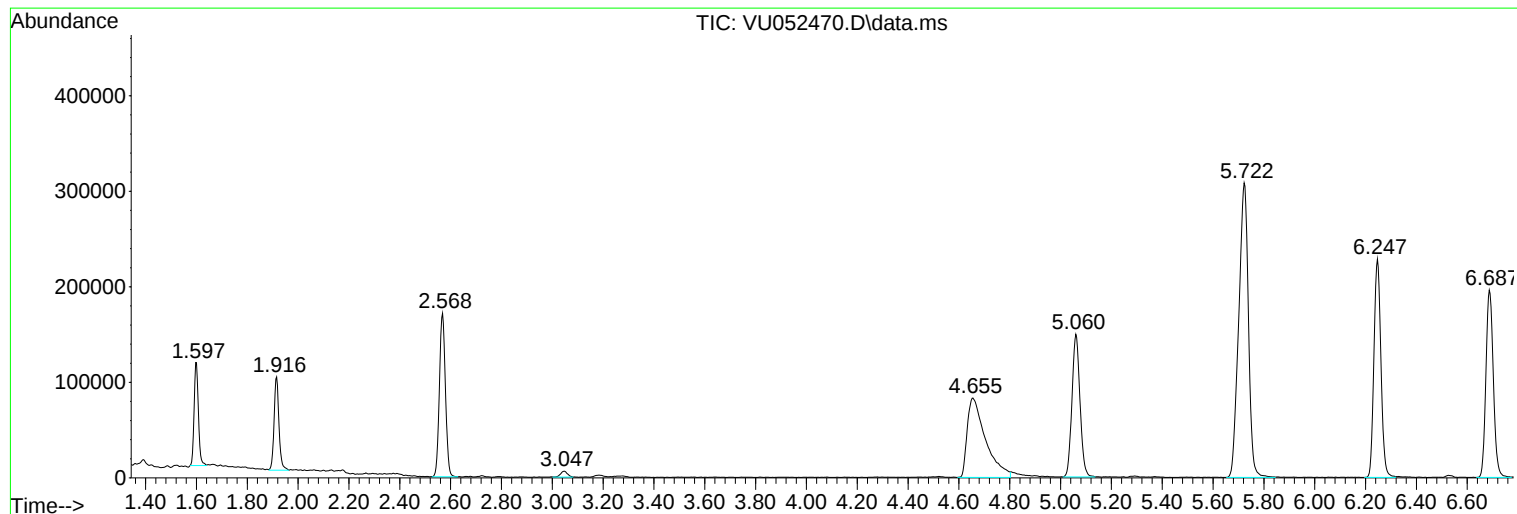

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052470.D
Acq On : 21 Dec 2022 11:16
Operator : JC/MD
Sample : N6034-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052470.D
Acq On : 21 Dec 2022 11:16
Operator : JC/MD
Sample : N6034-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
