

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052475.D
 Acq On : 21 Dec 2022 13:13
 Operator : JC/MD
 Sample : N6156-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEL9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	109897	131012	12.70%	1.961%
2	1.732	115	122	132	rVB	36529	46851	4.54%	0.701%
3	1.916	171	179	193	rVB	94175	123423	11.97%	1.847%
4	2.375	315	322	337	rVB5	5389	10356	1.00%	0.155%
5	2.568	370	382	399	rBV	171215	282642	27.41%	4.230%
6	3.044	520	530	544	rBV2	6219	11999	1.16%	0.180%
7	4.658	1012	1032	1070	rBV2	114730	502404	48.72%	7.518%
8	4.816	1076	1081	1100	rVB2	13713	30679	2.97%	0.459%
9	5.060	1140	1157	1182	rBV	144064	320968	31.12%	4.803%
10	5.722	1341	1363	1389	rBV2	292270	778553	75.49%	11.651%
11	6.247	1512	1526	1549	rBV	211532	402772	39.06%	6.027%
12	6.539	1606	1617	1630	rBV3	17212	32919	3.19%	0.493%
13	6.687	1649	1663	1683	rBV	193904	382640	37.10%	5.726%
14	7.565	1923	1936	1960	rBV	82491	149429	14.49%	2.236%
15	7.896	2026	2039	2061	rBV	315430	548903	53.23%	8.214%
16	8.176	2115	2126	2142	rBV2	53952	93108	9.03%	1.393%
17	8.468	2206	2217	2229	rBV3	6074	11573	1.12%	0.173%
18	8.552	2233	2243	2256	rVB2	32839	54864	5.32%	0.821%
19	8.635	2256	2269	2308	rBV2	487468	1031281	100.00%	15.432%
20	8.787	2308	2316	2329	rVB4	8205	15511	1.50%	0.232%
21	9.414	2498	2511	2536	rBV	309968	505700	49.04%	7.567%
22	10.751	2915	2927	2943	rBV	154895	248992	24.14%	3.726%
23	10.889	2961	2970	2983	rVB2	8700	13673	1.33%	0.205%
24	11.806	3243	3255	3274	rBV	262777	422860	41.00%	6.328%
25	12.057	3319	3333	3351	rBV3	19089	38616	3.74%	0.578%
26	12.188	3362	3374	3391	rBV	293380	476330	46.19%	7.128%
27	12.886	3581	3591	3602	rBV4	9526	14479	1.40%	0.217%




Sum of corrected areas: 6682537

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052475.D
Acq On : 21 Dec 2022 13:13
Operator : JC/MD
Sample : N6156-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

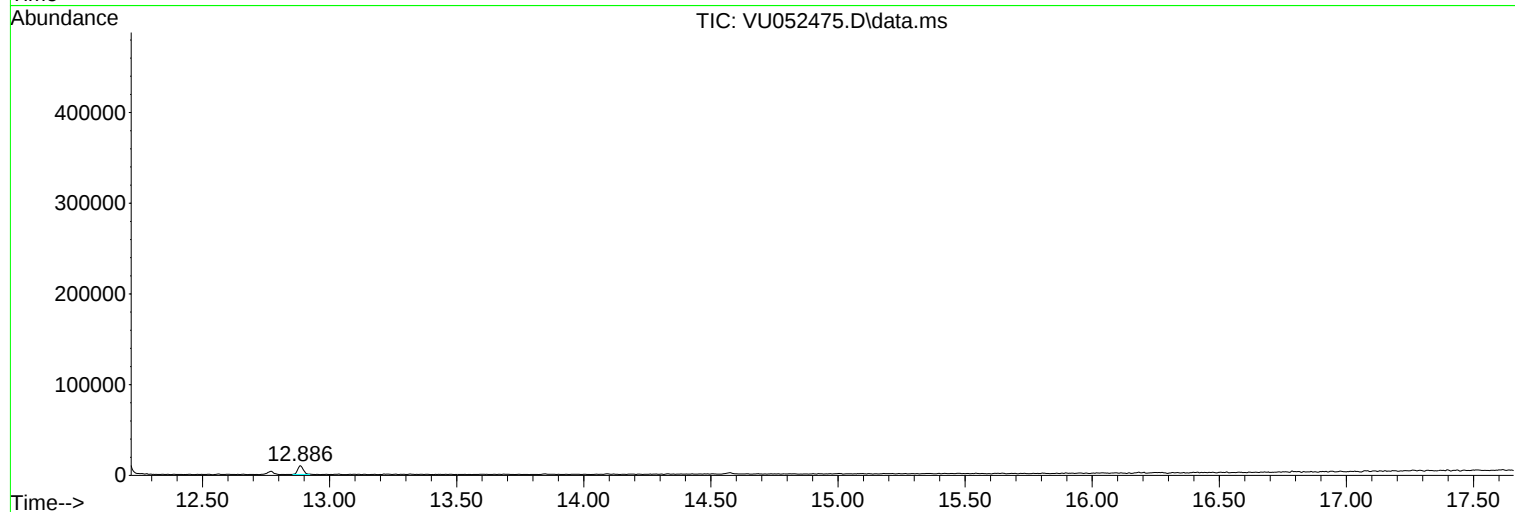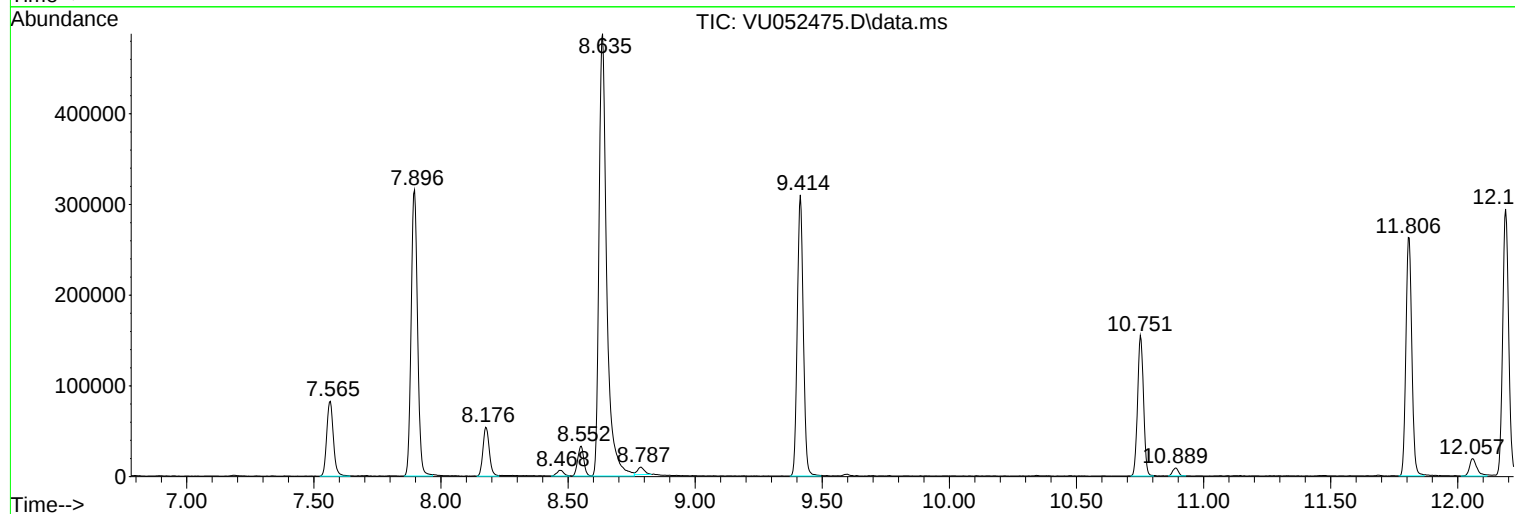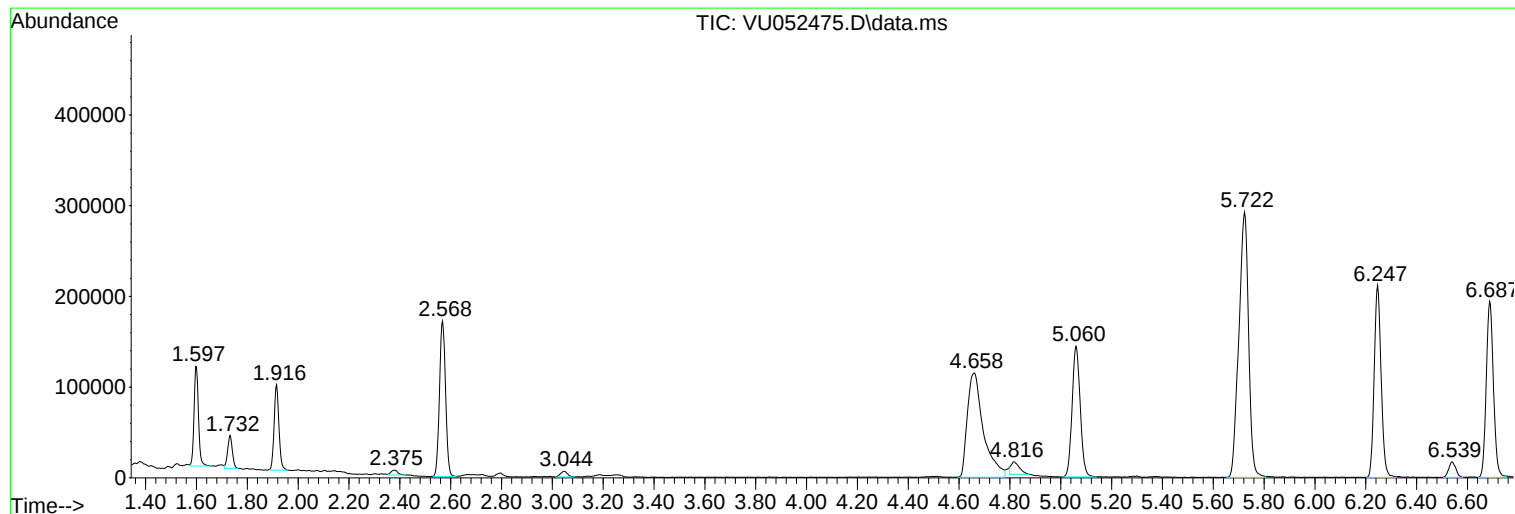

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052475.D
Acq On : 21 Dec 2022 13:13
Operator : JC/MD
Sample : N6156-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052475.D
Acq On : 21 Dec 2022 13:13
Operator : JC/MD
Sample : N6156-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc