

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
 Data File : VU052478.D
 Acq On : 21 Dec 2022 15:33
 Operator : JC/MD
 Sample : N6156-01DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEL7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	91	rVB	117390	136510	14.27%	1.990%
2	1.915	169	179	195	rBV	98417	134468	14.05%	1.960%
3	2.568	368	382	399	rBV	172700	284057	29.69%	4.140%
4	3.047	519	531	543	rVB2	8255	15398	1.61%	0.224%
5	3.179	561	572	587	rBV	5793	14544	1.52%	0.212%
6	4.655	1006	1031	1072	rBV2	181844	691620	72.28%	10.081%
7	5.060	1140	1157	1175	rBV	151469	334081	34.92%	4.869%
8	5.722	1341	1363	1387	rBV2	307479	811900	84.86%	11.834%
9	6.246	1512	1526	1550	rBV	211965	402415	42.06%	5.865%
10	6.539	1605	1617	1640	rVB2	46220	89620	9.37%	1.306%
11	6.687	1647	1663	1683	rBV	202511	398670	41.67%	5.811%
12	7.562	1924	1935	1954	rBV	85555	152489	15.94%	2.223%
13	7.896	2025	2039	2058	rBV	338474	578063	60.42%	8.426%
14	8.176	2114	2126	2140	rBV	54202	93320	9.75%	1.360%
15	8.549	2232	2242	2255	rVB	69629	116601	12.19%	1.700%
16	8.632	2255	2268	2308	rBV2	471821	956805	100.00%	13.946%
17	9.414	2498	2511	2528	rBV	304866	505735	52.86%	7.371%
18	10.751	2912	2927	2944	rBV	150982	242865	25.38%	3.540%
19	11.806	3243	3255	3277	rBV	258842	415284	43.40%	6.053%
20	12.188	3362	3374	3397	rBV	299797	486286	50.82%	7.088%




Sum of corrected areas: 6860731

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052478.D
Acq On : 21 Dec 2022 15:33
Operator : JC/MD
Sample : N6156-01DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEL7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

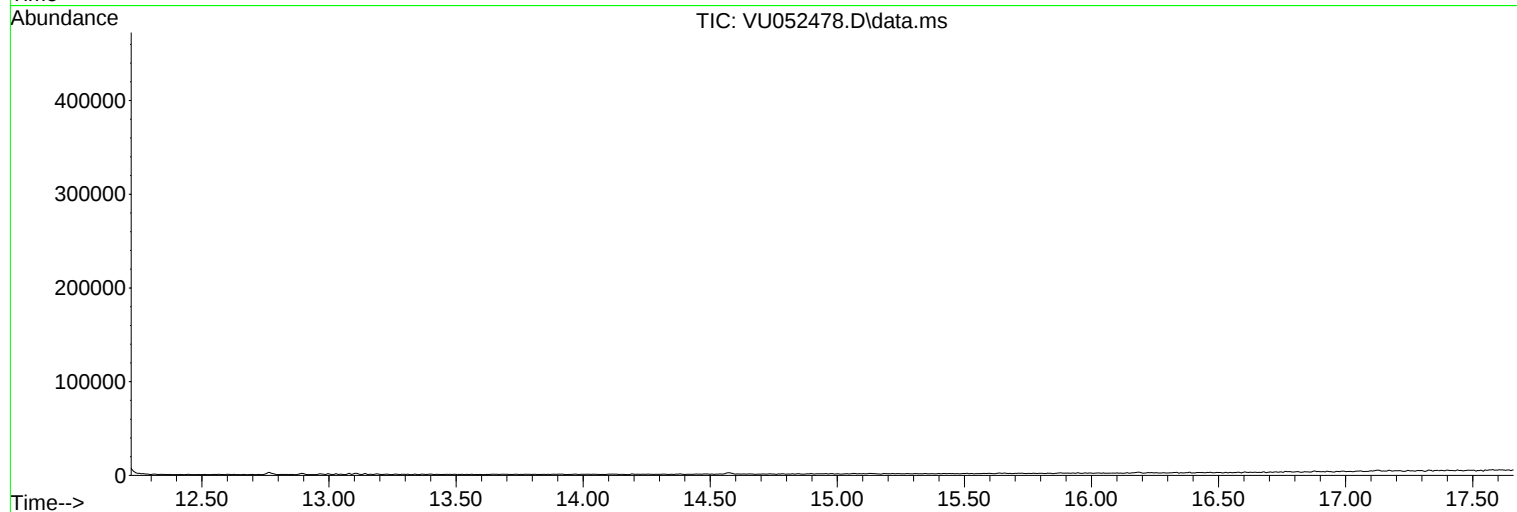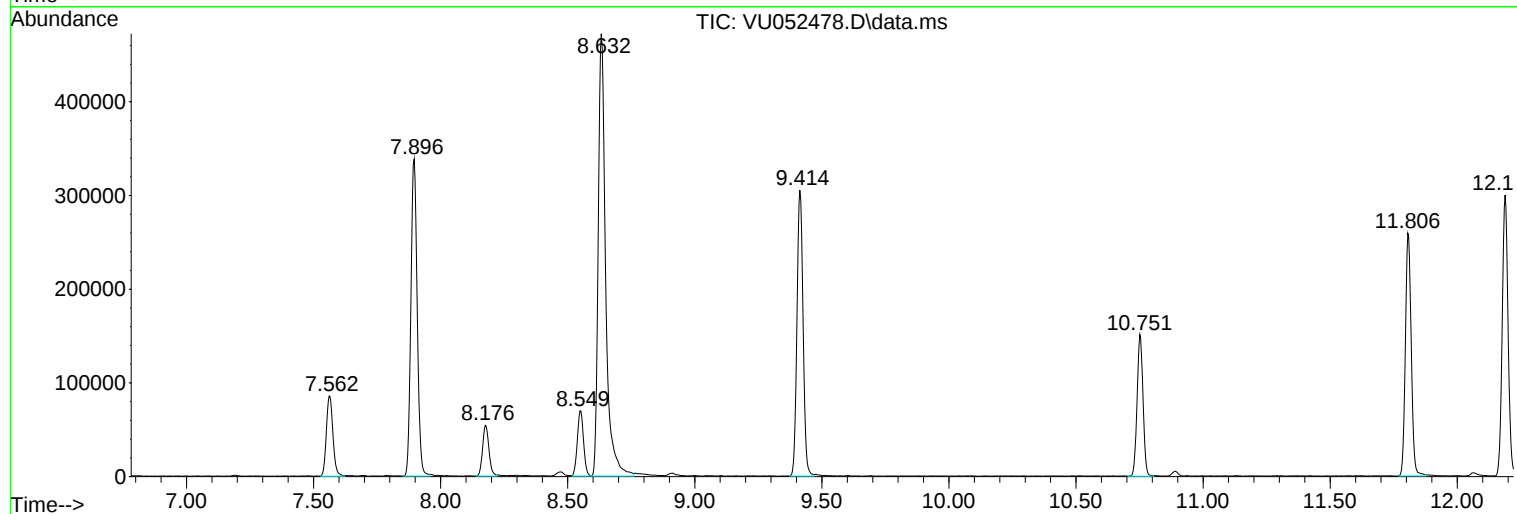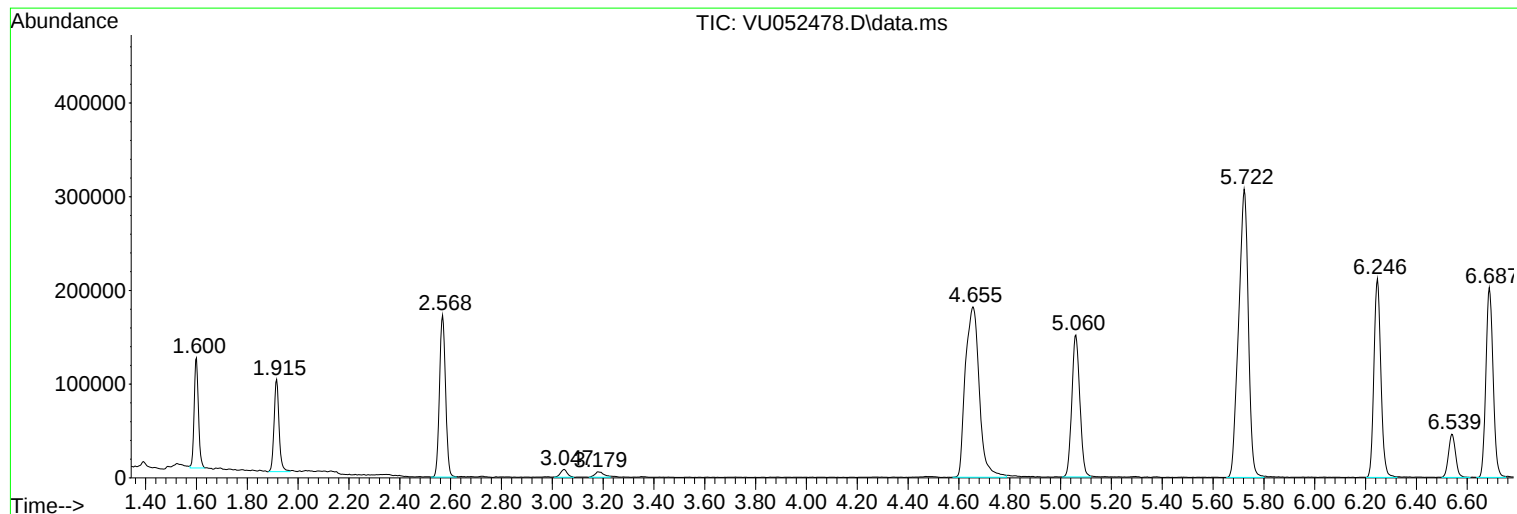

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052478.D
Acq On : 21 Dec 2022 15:33
Operator : JC/MD
Sample : N6156-01DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEL7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052478.D
Acq On : 21 Dec 2022 15:33
Operator : JC/MD
Sample : N6156-01DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEL7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc